




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031623\
Data File : BP014107.D
Acq On : 16 Mar 2023 17:38
Operator : CG/JU
Sample : 01884-11
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB921

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 03/17/2023
Supervised By :Jagrut Upadhyay 03/17/2023

Quant Time: Mar 17 01:00:52 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 17 00:57:25 2023
Response via : Initial Calibration

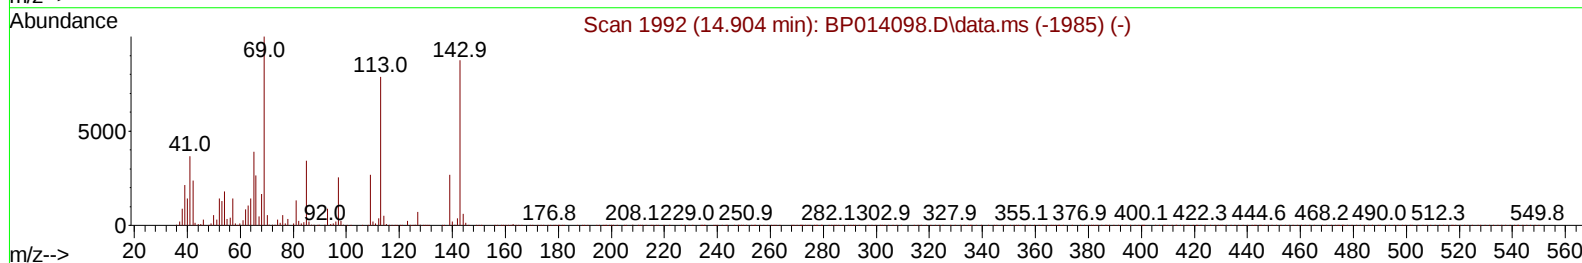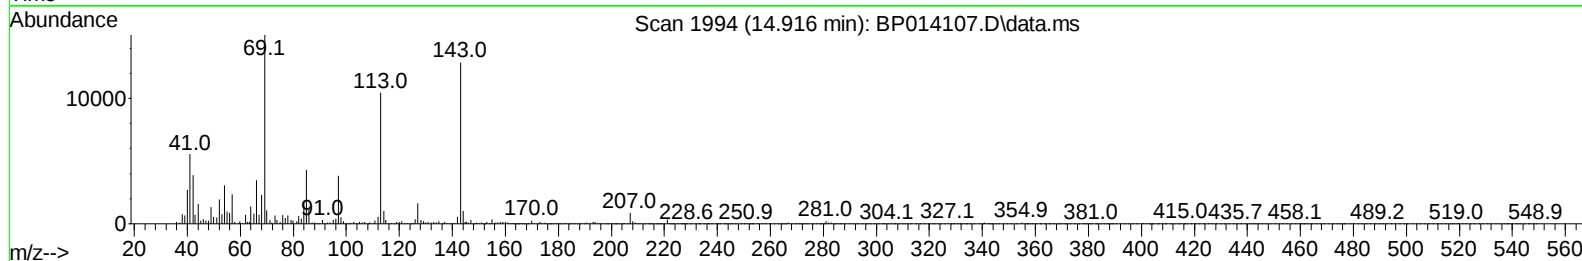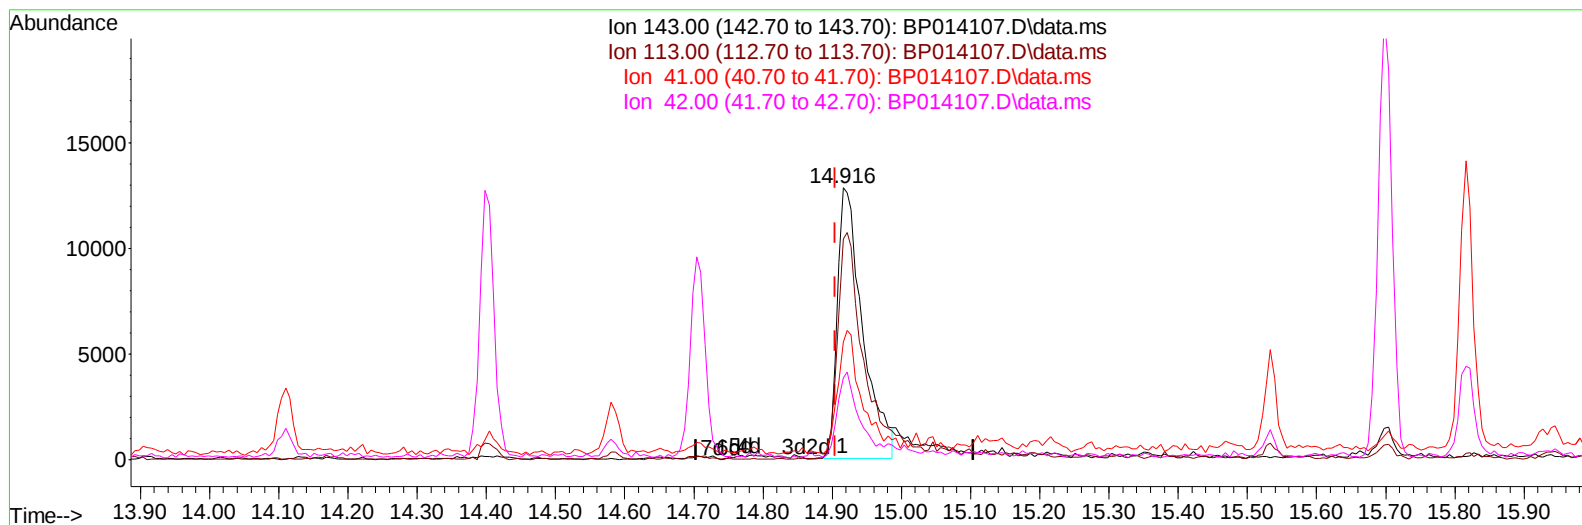

TIC: BP014107.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.916min (+ 0.012) 4.83 ng/u1

response 32353

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	103.10	81.31#
41.00	40.20	43.19
42.00	28.50	30.19




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031623\
Data File : BP014107.D
Acq On : 16 Mar 2023 17:38
Operator : CG/JU
Sample : 01884-11
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB921

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 03/17/2023
Supervised By :Jagrut Upadhyay 03/17/2023

Quant Time: Mar 17 01:00:52 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 17 00:57:25 2023
Response via : Initial Calibration

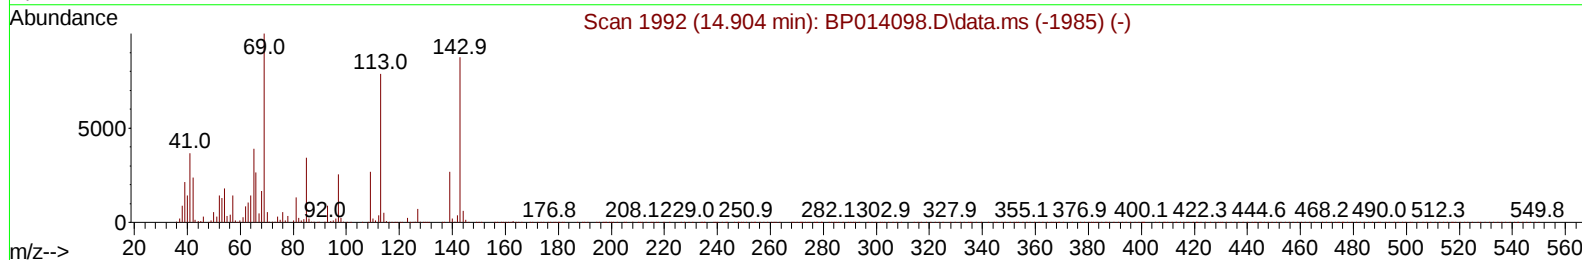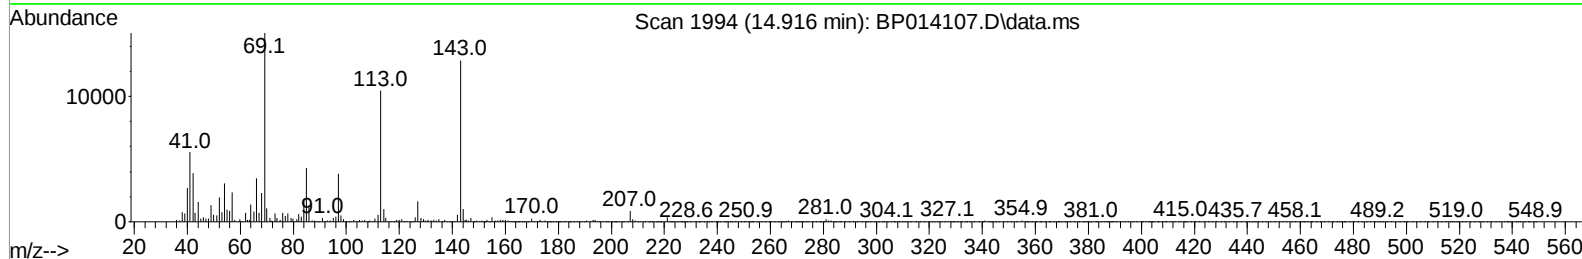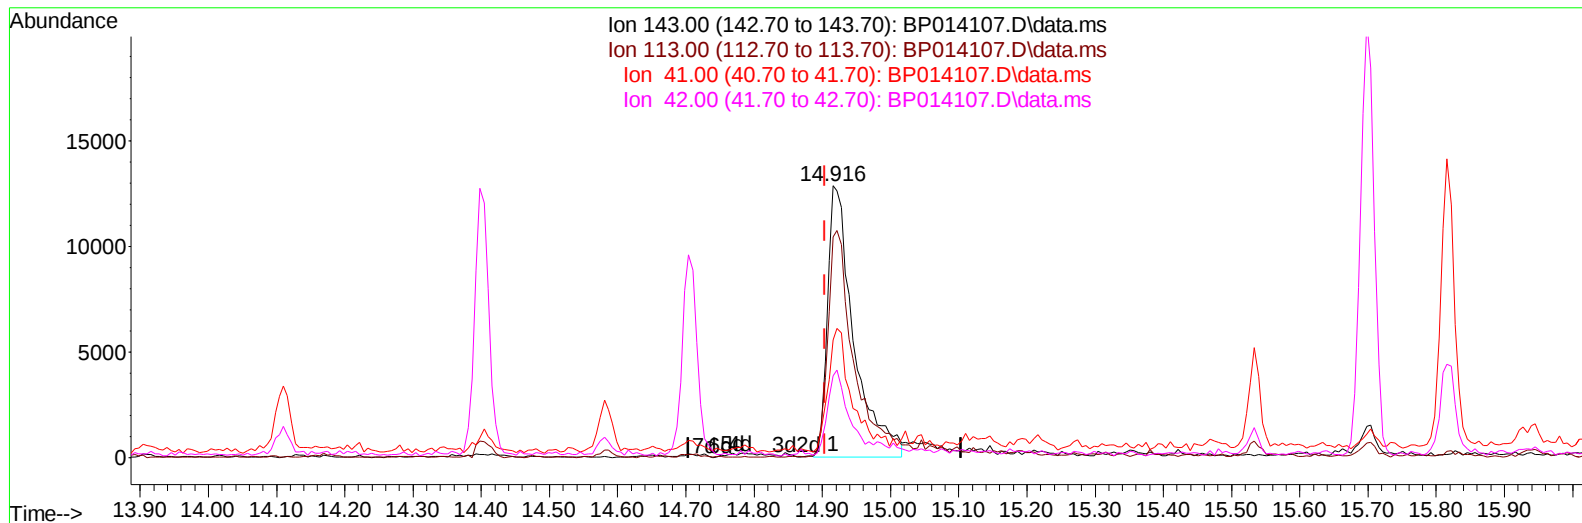

TIC: BP014107.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.916min (+ 0.012) 5.13 ng/ul m

response 34427

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	103.10	81.31#
41.00	40.20	43.19
42.00	28.50	30.19

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031623\
 Data File : BP014107.D
 Acq On : 16 Mar 2023 17:38
 Operator : CG/JU
 Sample : 01884-11
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CB921

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 03/17/2023
 Supervised By :Jagrut Upadhyay 03/17/2023

Quant Time: Mar 17 01:00:52 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Mar 17 00:57:25 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.063	152	149359	20.000	ng/ul	0.00
20) Naphthalene-d8	10.887	136	642304	20.000	ng/ul	# 0.00
38) Acenaphthene-d10	14.710	164	448328	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.463	188	1071190	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.545	240	1121450	20.000	ng/ul	# 0.00
88) Perylene-d12	24.086	264	1117851	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.422	96	17189	4.348	ng/uL	0.00
4) Pyridine-d5	3.869	84	71367	6.520	ng/ul	0.01
7) Phenol-d5	7.222	99	86165	6.537	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.387	67	287064	37.344	ng/ul	0.00
11) 2-Chlorophenol-d4	7.593	132	252911	25.185	ng/ul	0.00
15) 4-Methylphenol-d8	8.775	113	178152	16.547	ng/ul	0.00
21) Nitrobenzene-d5	9.240	128	179088	34.945	ng/ul	0.00
24) 2-Nitrophenol-d4	9.963	143	201169	32.792	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.504	165	341842	29.614	ng/ul	0.00
31) 4-Chloroaniline-d4	11.028	131	315859	20.677	ng/ul	0.00
46) Dimethylphthalate-d6	14.110	166	1382955	36.347	ng/ul	0.00
49) Acenaphthylene-d8	14.404	160	1464427	36.333	ng/ul	0.00
54) 4-Nitrophenol-d4	14.916	143	34427m	5.134	ng/ul	0.01
60) Fluorene-d10	15.698	176	1183018	36.687	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.816	200	241170	29.788	ng/ul	0.00
73) Anthracene-d10	17.563	188	1951841	37.535	ng/ul	0.00
81) Pyrene-d10	19.792	212	2363073	38.206	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.921	264	2275915	38.276	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031623\
Data File : BP014107.D
Acq On : 16 Mar 2023 17:38
Operator : CG/JU
Sample : 01884-11
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB921

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 03/17/2023
Supervised By :Jagrut Upadhyay 03/17/2023

Quant Time: Mar 17 01:00:52 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 17 00:57:25 2023
Response via : Initial Calibration

