




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031623\
Data File : BP014109.D
Acq On : 16 Mar 2023 18:47
Operator : CG/JU
Sample : 01884-13
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB925

Manual IntegrationsAPPROVED

Quant Time: Mar 17 01:01:13 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 17 00:57:25 2023
Response via : Initial Calibration

Reviewed By :Christian Giraldo 03/17/2023
Supervised By :Jagrut Upadhyay 03/17/2023

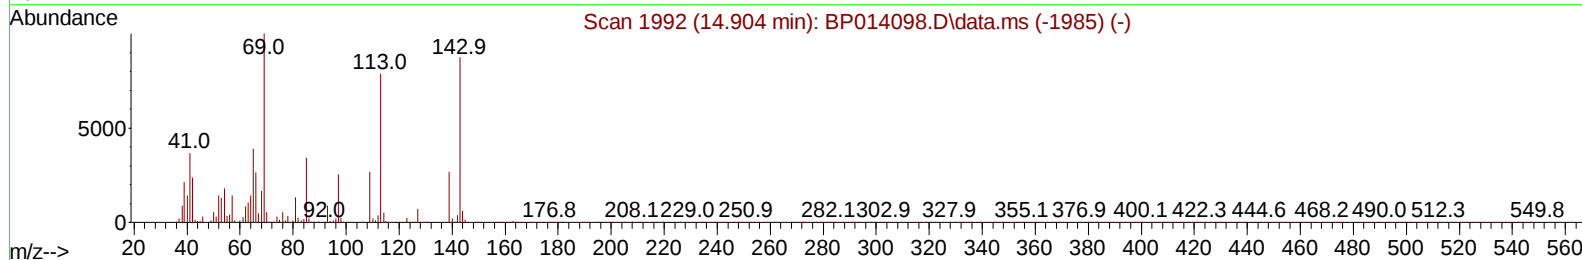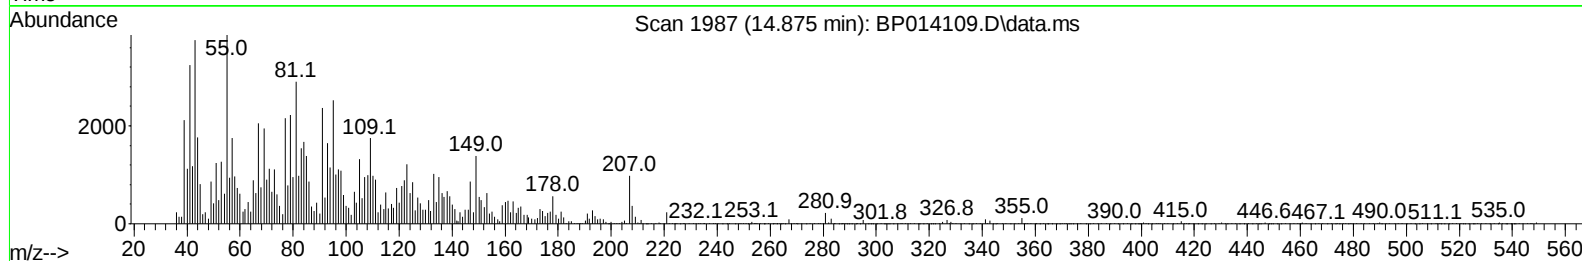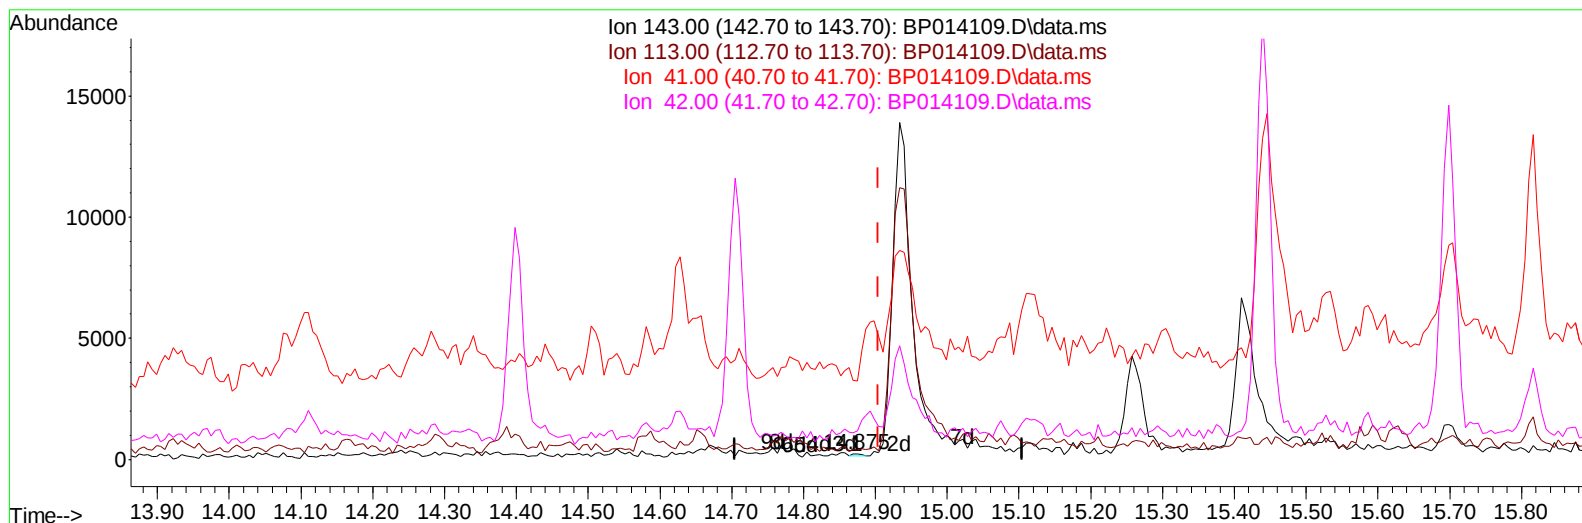

TIC: BP014109.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.875min (-0.029) 0.01 ng/u1

response 80

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	103.10	168.38#
41.00	40.20	1385.90#
42.00	28.50	502.99#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031623\
Data File : BP014109.D
Acq On : 16 Mar 2023 18:47
Operator : CG/JU
Sample : 01884-13
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB925

Manual IntegrationsAPPROVED

Quant Time: Mar 17 01:01:13 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 17 00:57:25 2023
Response via : Initial Calibration

Reviewed By :Christian Giraldo 03/17/2023
Supervised By :Jagrut Upadhyay 03/17/2023

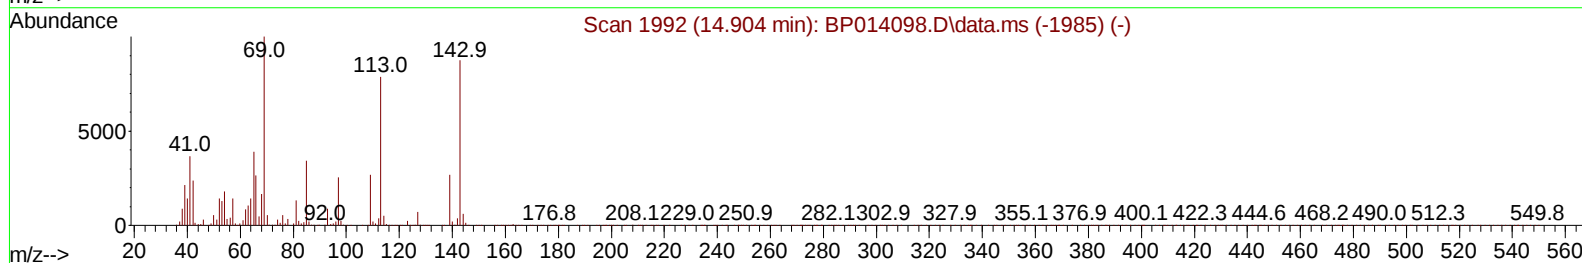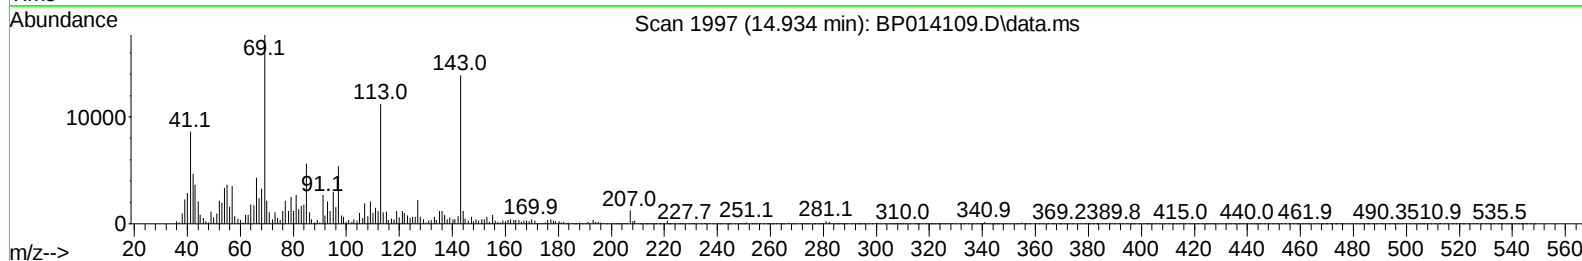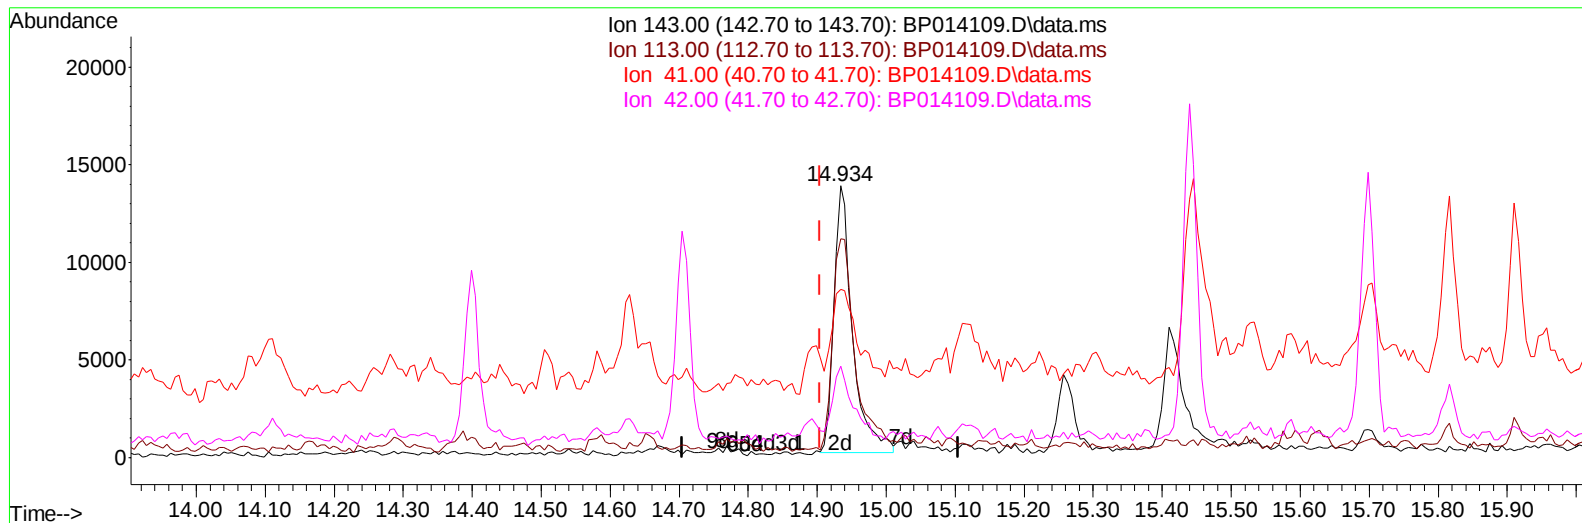

TIC: BP014109.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.934min (+ 0.030) 3.46 ng/ul m

response 25690

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	103.10	80.53#
41.00	40.20	61.96#
42.00	28.50	33.66

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031623\
 Data File : BP014109.D
 Acq On : 16 Mar 2023 18:47
 Operator : CG/JU
 Sample : 01884-13
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CB925

Manual IntegrationsAPPROVED

Quant Time: Mar 17 01:01:13 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Mar 17 00:57:25 2023
 Response via : Initial Calibration

Reviewed By :Christian Giraldo 03/17/2023
 Supervised By :Jagrut Upadhyay 03/17/2023

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.064	152	174036	20.000	ng/ul	0.00
20) Naphthalene-d8	10.887	136	729334	20.000	ng/ul	# 0.00
38) Acenaphthene-d10	14.704	164	496196	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.463	188	1148809	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.545	240	1132899	20.000	ng/ul	# 0.00
88) Perylene-d12	24.080	264	1123575	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.423	96	16477	3.577	ng/uL	0.00
4) Pyridine-d5	3.864	84	157652	12.361	ng/ul	0.00
7) Phenol-d5	7.222	99	77216	5.028	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.387	67	214017	23.894	ng/ul	0.00
11) 2-Chlorophenol-d4	7.593	132	186589	15.946	ng/ul	0.00
15) 4-Methylphenol-d8	8.775	113	144587	11.525	ng/ul	0.00
21) Nitrobenzene-d5	9.240	128	127963	21.989	ng/ul	0.00
24) 2-Nitrophenol-d4	9.963	143	134157	19.259	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.510	165	242888	18.531	ng/ul	0.00
31) 4-Chloroaniline-d4	11.028	131	352937	20.347	ng/ul	0.00
46) Dimethylphthalate-d6	14.110	166	948012	22.512	ng/ul	0.00
49) Acenaphthylene-d8	14.398	160	980067	21.970	ng/ul	0.00
54) 4-Nitrophenol-d4	14.934	143	25690m	3.462	ng/ul	0.03
60) Fluorene-d10	15.698	176	765107	21.438	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.816	200	123100	14.178	ng/ul	0.00
73) Anthracene-d10	17.563	188	1265278	22.688	ng/ul	0.00
81) Pyrene-d10	19.786	212	1501501	24.031	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.916	264	1365607	22.849	ng/ul	0.00
Target Compounds						
52) Acenaphthene	14.769	153	54722	1.672	ng/ul	Qvalue 96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031623\
Data File : BP014109.D
Acq On : 16 Mar 2023 18:47
Operator : CG/JU
Sample : 01884-13
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB925

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 03/17/2023
Supervised By :Jagrut Upadhyay 03/17/2023

Quant Time: Mar 17 01:01:13 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 17 00:57:25 2023
Response via : Initial Calibration

