

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031623\
 Data File : BP014099.D
 Acq On : 16 Mar 2023 13:02
 Operator : CG/JU
 Sample : PB151450BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK450

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
 Title : SVOA CALIBRATION

Signal : TIC: BP014099.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.417	36	39	46	rVB	26296	38155	1.00%	0.114%
2	3.864	112	115	134	rBV	180748	390471	10.24%	1.164%
3	4.187	166	170	175	rVB5	6931	11934	0.31%	0.036%
4	4.852	280	283	287	rBV6	2514	4127	0.11%	0.012%
5	5.405	375	377	380	rVB4	4297	4406	0.12%	0.013%
6	6.552	568	572	574	rBV4	3701	4000	0.10%	0.012%
7	6.857	622	624	627	rBV3	3607	4378	0.11%	0.013%
8	7.163	674	676	679	rVV4	5054	6541	0.17%	0.020%
9	7.216	679	685	695	rVV	433298	738334	19.36%	2.202%
10	7.387	706	714	723	rBV	348945	574673	15.07%	1.714%
11	7.593	742	749	759	rBV	435043	739044	19.38%	2.204%
12	8.063	823	829	838	rBV	354790	579847	15.20%	1.729%
13	8.316	871	872	876	rBV3	4090	4168	0.11%	0.012%
14	8.769	943	949	963	rBV	546424	943629	24.74%	2.814%
15	8.881	966	968	971	rVB2	4323	3957	0.10%	0.012%
16	9.240	1020	1029	1036	rBV	430546	744390	19.52%	2.220%
17	9.381	1052	1053	1060	rVB7	2524	3933	0.10%	0.012%
18	9.663	1100	1101	1104	rVB3	4423	4243	0.11%	0.013%
19	9.746	1113	1115	1121	rVB6	2189	4634	0.12%	0.014%
20	9.963	1145	1152	1164	rBV	378425	645068	16.91%	1.924%
21	10.434	1227	1232	1235	rVB6	3401	4752	0.12%	0.014%
22	10.504	1235	1244	1255	rBV	519715	951791	24.95%	2.838%
23	10.657	1268	1270	1274	rBV5	3589	4240	0.11%	0.013%
24	10.887	1301	1309	1317	rBV	509534	867545	22.74%	2.587%
25	11.028	1326	1333	1355	rBV	578416	1204562	31.58%	3.592%
26	11.163	1355	1356	1360	rVV3	5674	5630	0.15%	0.017%
27	11.216	1363	1365	1370	rVB5	3294	4212	0.11%	0.013%
28	11.881	1476	1478	1483	rVB6	2903	4619	0.12%	0.014%
29	12.481	1575	1580	1586	rBV6	8014	17583	0.46%	0.052%
30	12.692	1613	1616	1619	rVV5	3053	3923	0.10%	0.012%
31	12.998	1665	1668	1671	rVB4	3744	4523	0.12%	0.013%
32	13.128	1688	1690	1693	rBV4	3657	4267	0.11%	0.013%
33	13.257	1710	1712	1716	rBV5	2824	4205	0.11%	0.013%
34	13.375	1730	1732	1735	rVB3	3485	3896	0.10%	0.012%
35	13.404	1735	1737	1740	rBV4	3496	3912	0.10%	0.012%
36	13.587	1763	1768	1776	rVB6	13799	25167	0.66%	0.075%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031623\
 Data File : BP014099.D
 Acq On : 16 Mar 2023 13:02
 Operator : CG/JU
 Sample : PB151450BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK450

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
 Title : SVOA CALIBRATION

37	14.110	1848	1857	1868	rBV	1197591	1657508	43.45%	4.943%
38	14.187	1868	1870	1873	rVB4	4610	4081	0.11%	0.012%
39	14.304	1887	1890	1894	rVB5	2689	4108	0.11%	0.012%
40	14.404	1900	1907	1918	rBV	1207245	1808559	47.41%	5.393%
41	14.704	1952	1958	1970	rVB	850506	1313845	34.45%	3.918%
42	14.904	1986	1992	2011	rBV	349971	779077	20.43%	2.323%
43	15.698	2121	2127	2137	rBV	1616700	2382833	62.47%	7.106%
44	15.816	2142	2147	2164	rVV	493620	802683	21.04%	2.394%
45	15.939	2165	2168	2173	rVB7	7849	11551	0.30%	0.034%
46	16.569	2270	2275	2277	rVB5	3958	5146	0.13%	0.015%
47	17.133	2368	2371	2372	rBV2	3880	3921	0.10%	0.012%
48	17.145	2372	2373	2378	rVB5	4745	5386	0.14%	0.016%
49	17.263	2389	2393	2394	rBV4	4501	6254	0.16%	0.019%
50	17.463	2419	2427	2437	rBV	1167691	1715086	44.96%	5.114%
51	17.563	2437	2444	2458	rBV	1869850	2731291	71.61%	8.145%
52	17.863	2490	2495	2496	rBV4	6333	8309	0.22%	0.025%
53	17.975	2512	2514	2517	rVB4	4400	3870	0.10%	0.012%
54	18.351	2574	2578	2586	rBV9	21952	55774	1.46%	0.166%
55	19.369	2748	2751	2756	rVB2	24609	27848	0.73%	0.083%
56	19.439	2759	2763	2768	rBV2	24069	40602	1.06%	0.121%
57	19.792	2817	2823	2831	rBV	2463244	3375321	88.49%	10.065%
58	21.551	3117	3122	3129	rBV	1585429	2149853	56.36%	6.411%
59	23.921	3518	3525	3536	rVB2	1830091	3814326	100.00%	11.374%
60	24.086	3547	3553	3564	rVB2	1076926	2262499	59.32%	6.747%




Sum of corrected areas: 33534490

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031623\
Data File : BP014099.D
Acq On : 16 Mar 2023 13:02
Operator : CG/JU
Sample : PB151450BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK450

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

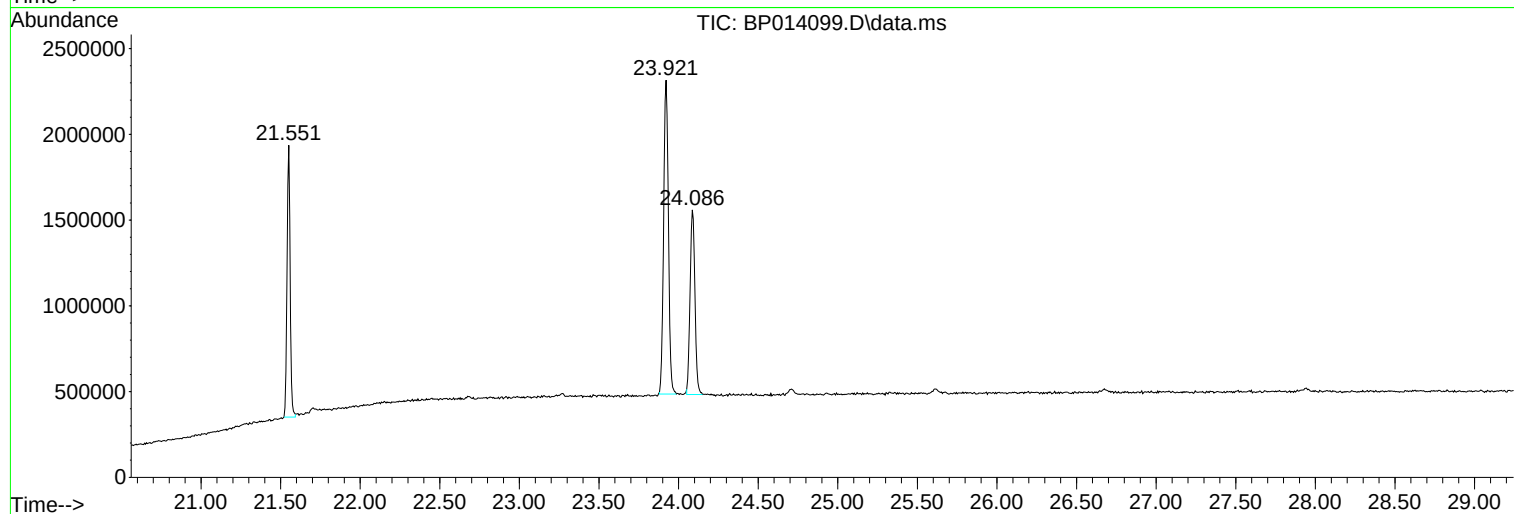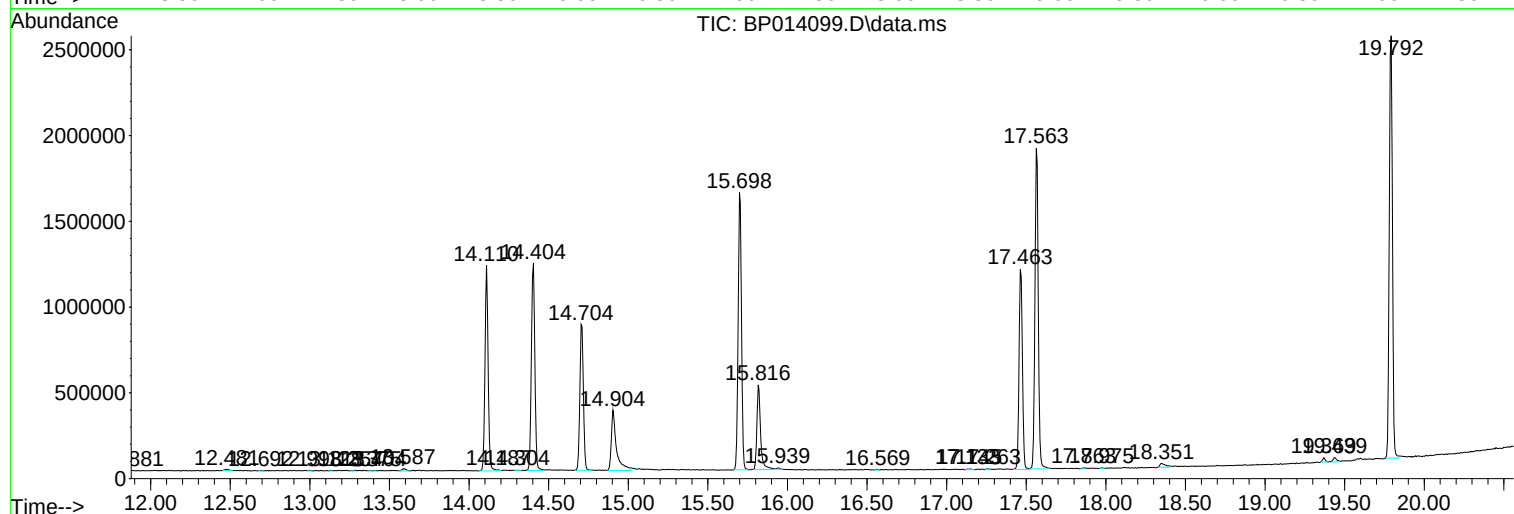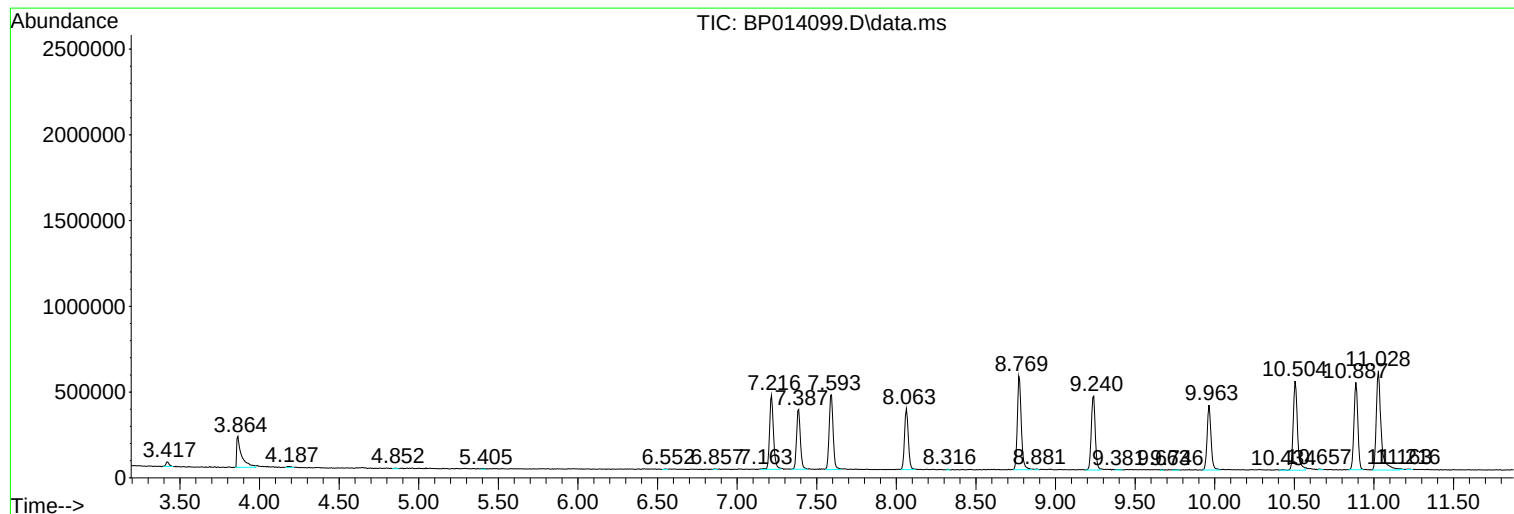

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031623\
Data File : BP014099.D
Acq On : 16 Mar 2023 13:02
Operator : CG/JU
Sample : PB151450BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK450

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031623\
Data File : BP014099.D
Acq On : 16 Mar 2023 13:02
Operator : CG/JU
Sample : PB151450BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK450

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc