

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031623\
 Data File : BP014100.D
 Acq On : 16 Mar 2023 13:36
 Operator : CG/JU
 Sample : PB151453BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK453

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
 Title : SVOA CALIBRATION

Signal : TIC: BP014100.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.416	36	39	46	rBV	26850	39054	1.03%	0.113%
2	3.858	111	114	136	rBV	197820	419125	11.07%	1.215%
3	4.187	167	170	175	rVB5	7169	11206	0.30%	0.032%
4	5.087	320	323	326	rBV4	3231	4446	0.12%	0.013%
5	5.316	360	362	368	rBV7	3564	4858	0.13%	0.014%
6	6.522	564	567	569	rBV3	3409	4469	0.12%	0.013%
7	6.681	590	594	598	rVB7	2924	4480	0.12%	0.013%
8	7.022	648	652	654	rVB4	3735	4716	0.12%	0.014%
9	7.063	654	659	662	rBV6	2491	5644	0.15%	0.016%
10	7.163	672	676	678	rBV5	2672	4380	0.12%	0.013%
11	7.216	678	685	698	rVV	422288	724480	19.14%	2.100%
12	7.387	708	714	724	rBV	336462	563683	14.89%	1.634%
13	7.587	742	748	766	rBV	441053	729858	19.28%	2.116%
14	7.899	796	801	803	rBV6	2704	4055	0.11%	0.012%
15	8.063	821	829	839	rBV	446376	708874	18.73%	2.055%
16	8.769	943	949	961	rBV	527544	919731	24.30%	2.666%
17	9.234	1019	1028	1038	rBV	430794	727995	19.23%	2.110%
18	9.963	1145	1152	1163	rBV	365893	625820	16.54%	1.814%
19	10.504	1236	1244	1260	rBV	506930	940623	24.85%	2.727%
20	10.887	1301	1309	1316	rBV	610859	1024676	27.07%	2.970%
21	11.028	1325	1333	1355	rBV	493717	1027264	27.14%	2.978%
22	11.357	1386	1389	1392	rBV4	3195	5196	0.14%	0.015%
23	12.281	1541	1546	1549	rVB6	3123	5587	0.15%	0.016%
24	12.316	1549	1552	1555	rBV5	3466	3856	0.10%	0.011%
25	12.475	1574	1579	1581	rBV5	5905	9885	0.26%	0.029%
26	12.957	1657	1661	1664	rVB4	3629	4453	0.12%	0.013%
27	13.463	1742	1747	1750	rVB7	2988	5190	0.14%	0.015%
28	13.504	1750	1754	1758	rBV6	2986	5156	0.14%	0.015%
29	14.039	1842	1845	1850	rVB5	2396	4712	0.12%	0.014%
30	14.110	1850	1857	1869	rBV	1139301	1624627	42.92%	4.709%
31	14.398	1899	1906	1915	rBV	1164518	1773708	46.86%	5.141%
32	14.704	1951	1958	1970	rVV	1013243	1544926	40.82%	4.478%
33	14.904	1986	1992	2003	rBV	336390	700575	18.51%	2.031%
34	15.698	2117	2127	2137	rBV	1677313	2356553	62.26%	6.831%
35	15.816	2141	2147	2160	rBV	490810	798568	21.10%	2.315%
36	15.945	2166	2169	2174	rVB7	9618	12396	0.33%	0.036%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031623\
 Data File : BP014100.D
 Acq On : 16 Mar 2023 13:36
 Operator : CG/JU
 Sample : PB151453BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK453

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
 Title : SVOA CALIBRATION

37	16.492	2260	2262	2268	rVB6	4182	4499	0.12%	0.013%
38	16.563	2268	2274	2275	rVB6	2928	4159	0.11%	0.012%
39	16.586	2275	2278	2280	rBV4	3518	3981	0.11%	0.012%
40	17.463	2420	2427	2438	rBV	1431418	2027545	53.57%	5.877%
41	17.563	2438	2444	2455	rBV2	1874983	2669876	70.54%	7.739%
42	17.963	2508	2512	2513	rBV4	3348	4366	0.12%	0.013%
43	18.110	2534	2537	2539	rBV4	8380	8907	0.24%	0.026%
44	18.357	2574	2579	2583	rBV7	21476	49269	1.30%	0.143%
45	19.369	2748	2751	2756	rVB3	25530	33792	0.89%	0.098%
46	19.433	2760	2762	2767	rVB	15183	21385	0.57%	0.062%
47	19.786	2817	2822	2829	rBV	2529470	3326099	87.88%	9.641%
48	21.545	3116	3121	3130	rBV	1797374	2546864	67.29%	7.382%
49	23.915	3517	3524	3536	rBV2	1800907	3784815	100.00%	10.971%
50	24.086	3546	3553	3563	rVB2	1233009	2658534	70.24%	7.706%




Sum of corrected areas: 34498916

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031623\
Data File : BP014100.D
Acq On : 16 Mar 2023 13:36
Operator : CG/JU
Sample : PB151453BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK453

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

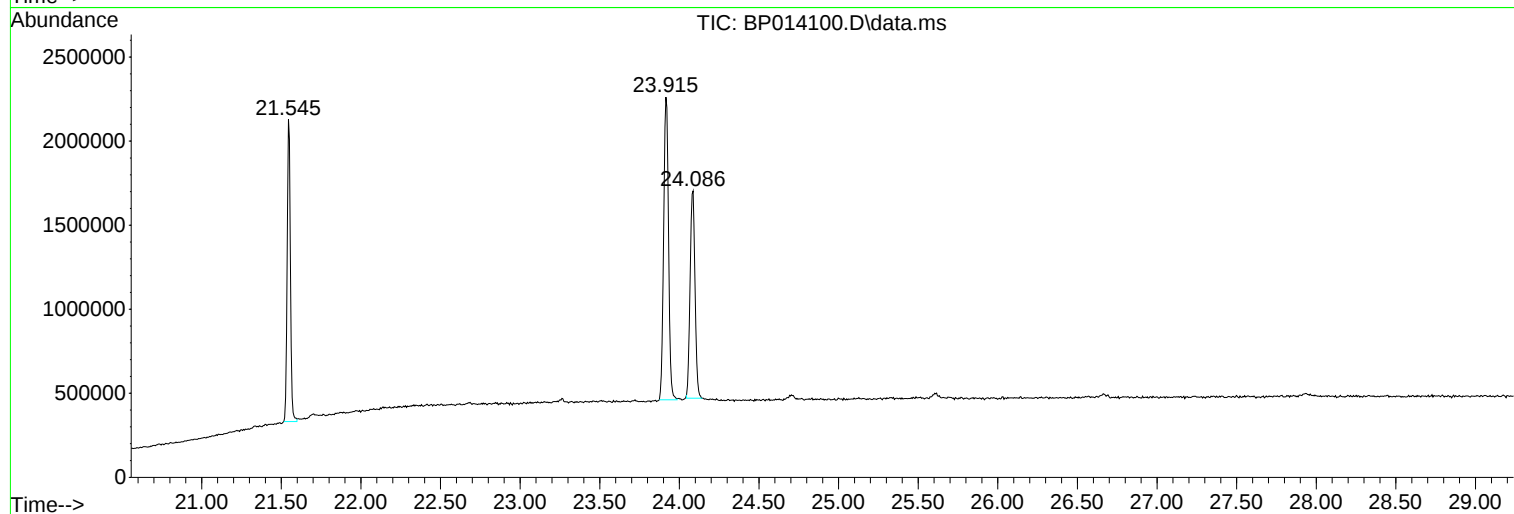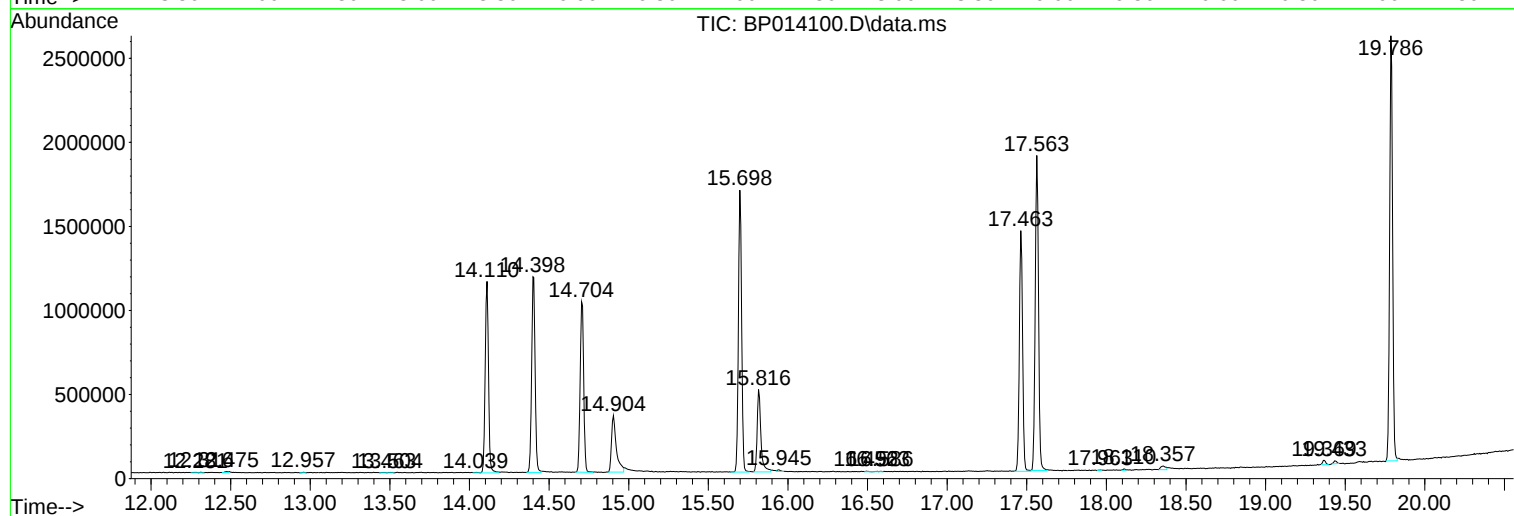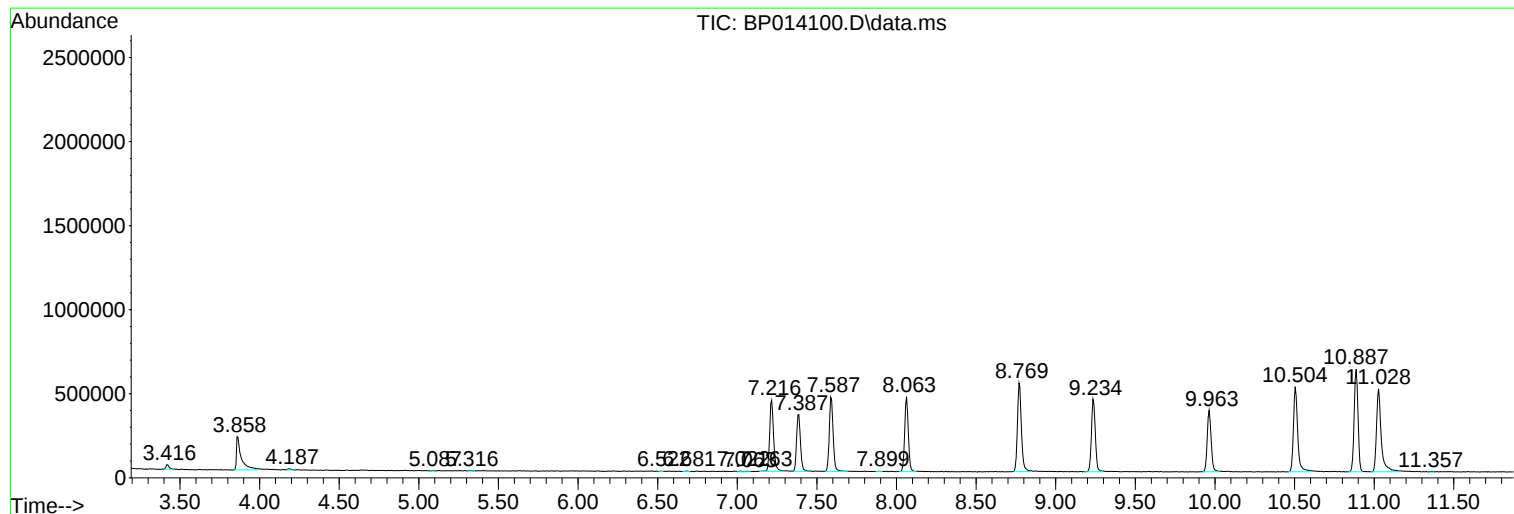

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031623\
Data File : BP014100.D
Acq On : 16 Mar 2023 13:36
Operator : CG/JU
Sample : PB151453BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK453

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031623\
Data File : BP014100.D
Acq On : 16 Mar 2023 13:36
Operator : CG/JU
Sample : PB151453BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK453

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc