
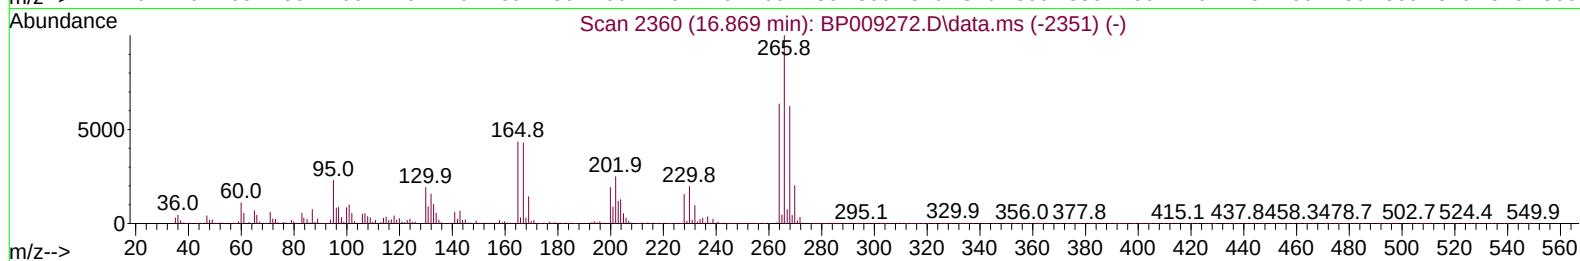
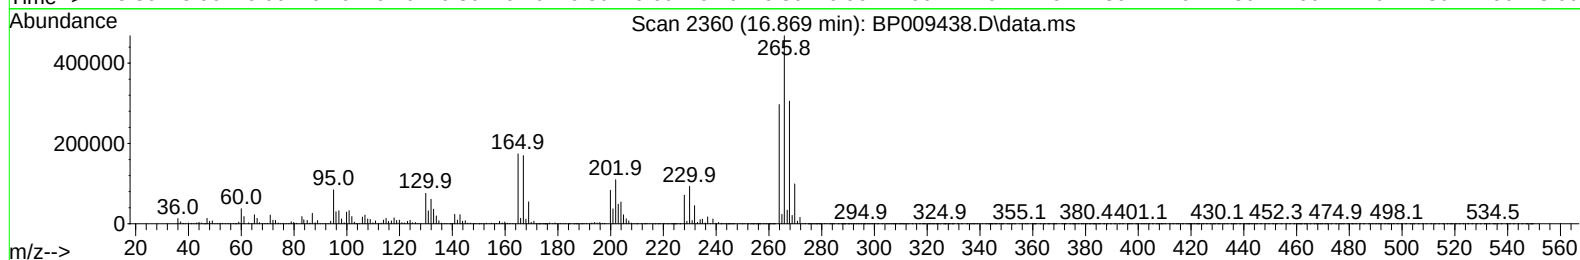


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031722\
 Data File : BP009438.D
 Acq On : 17 Mar 2022 11:02
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 17 17:36:13 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031722.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 17 17:31:41 2022
 Response via : Initial Calibration

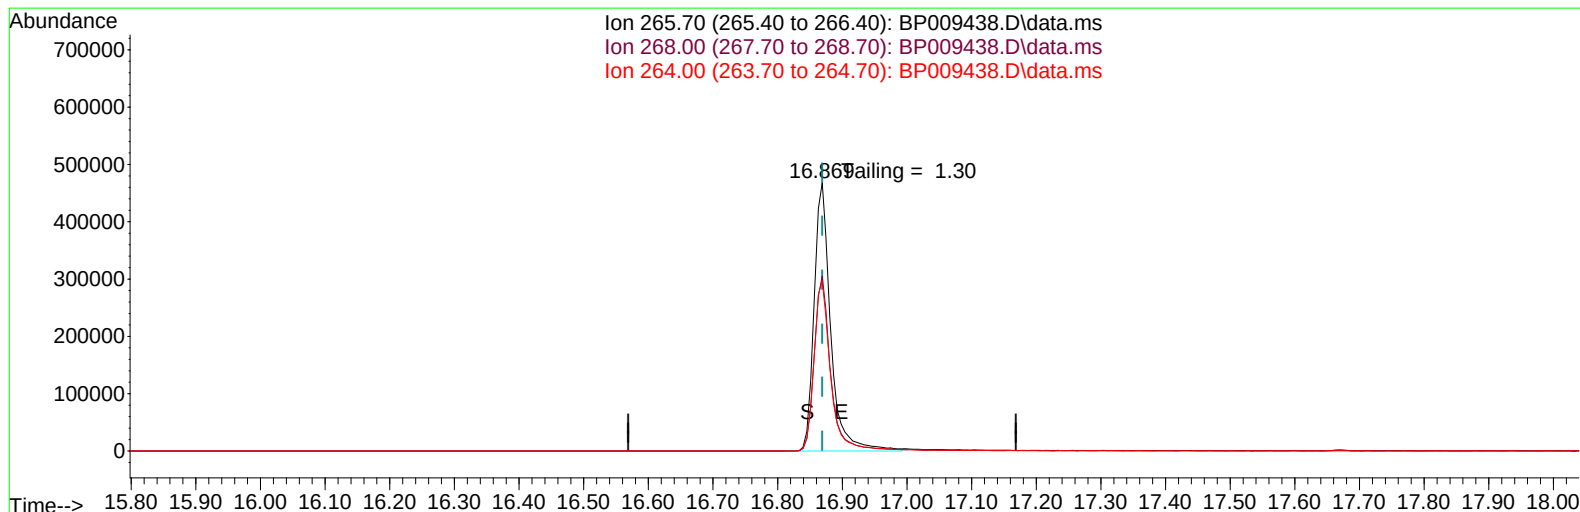

TIC: BP009438.D\data.ms

(70) Pentachlorophenol (C)




16.869min (-0.000) 231964.98 ng

response 844504

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.30	65.16
264.00	63.60	63.40
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031722\
Data File : BP009438.D
Acq On : 17 Mar 2022 11:02
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 17 17:36:13 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 17 17:31:41 2022
Response via : Initial Calibration

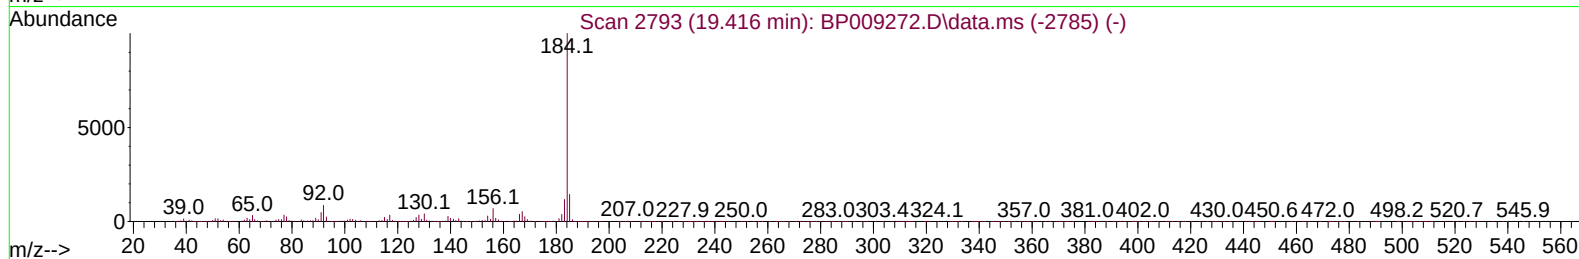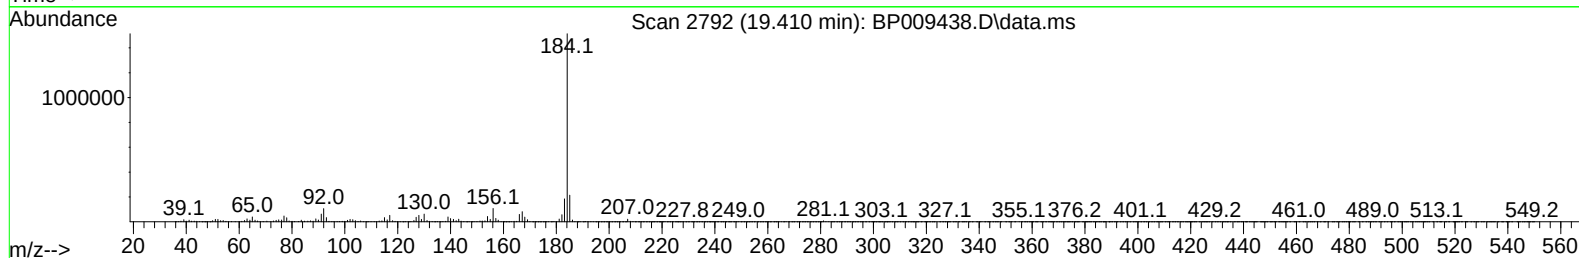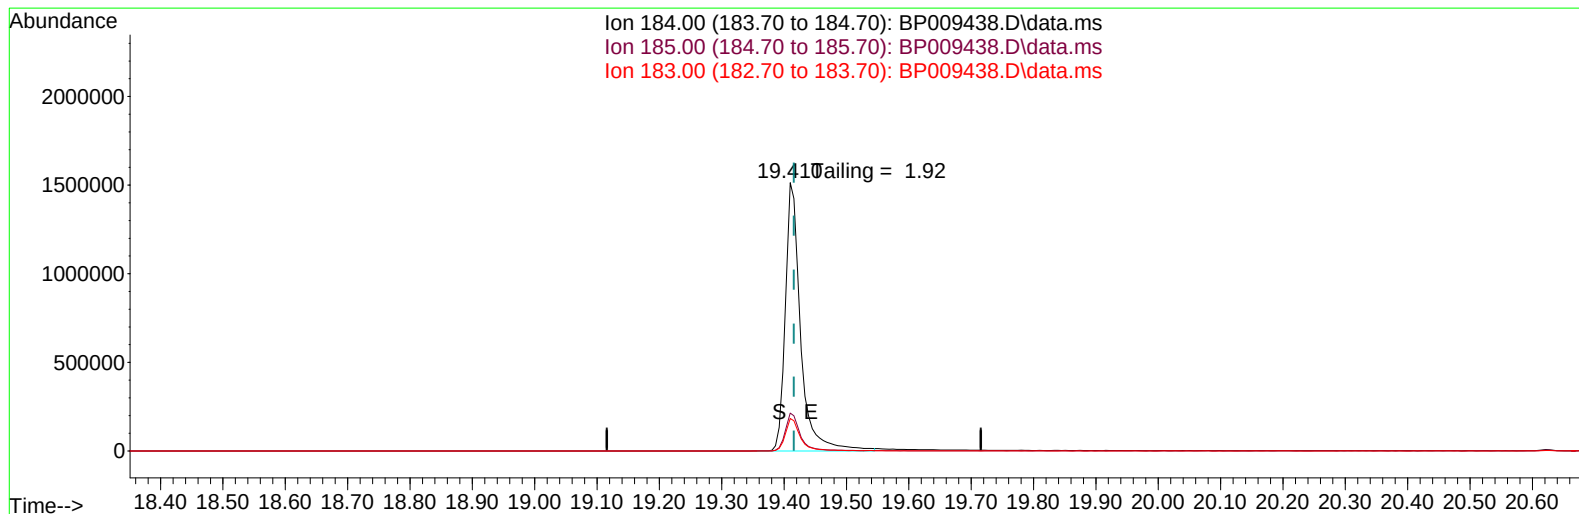

TIC: BP009438.D\data.ms

(77) Benzidine

19.410min (-0.006) 26964.59 ng

response 2650332

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.17
183.00	11.70	12.14
0.00	0.00	0.00