

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031722\
 Data File : BP009448.D
 Acq On : 17 Mar 2022 17:43
 Operator : CG/JU
 Sample : PB143199BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB143199BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031722.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP009448.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.405	404	411	430	rBV	4161253	6992164	46.45%	10.232%
2	6.993	672	681	708	rBV	3819465	7112548	47.25%	10.408%
3	7.799	811	818	829	rBV	811718	1400308	9.30%	2.049%
4	8.958	1006	1015	1039	rBV	2429166	4688580	31.14%	6.861%
5	10.593	1284	1293	1314	rBV	885926	1946594	12.93%	2.849%
6	13.063	1703	1713	1736	rBV	6914354	11493038	76.34%	16.819%
7	14.446	1939	1948	1967	rBV	1440549	2615594	17.37%	3.828%
8	15.940	2194	2202	2236	rBV	4495664	8475611	56.30%	12.403%
9	17.204	2410	2417	2435	rBV	1521518	2937920	19.52%	4.299%
10	19.781	2849	2855	2869	rBV	11194746	15054421	100.00%	22.031%
11	21.316	3111	3116	3129	rBV	1806161	2933933	19.49%	4.293%
12	23.727	3519	3526	3542	rVB2	1112319	2683692	17.83%	3.927%




Sum of corrected areas: 68334403

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031722\
Data File : BP009448.D
Acq On : 17 Mar 2022 17:43
Operator : CG/JU
Sample : PB143199BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB143199BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

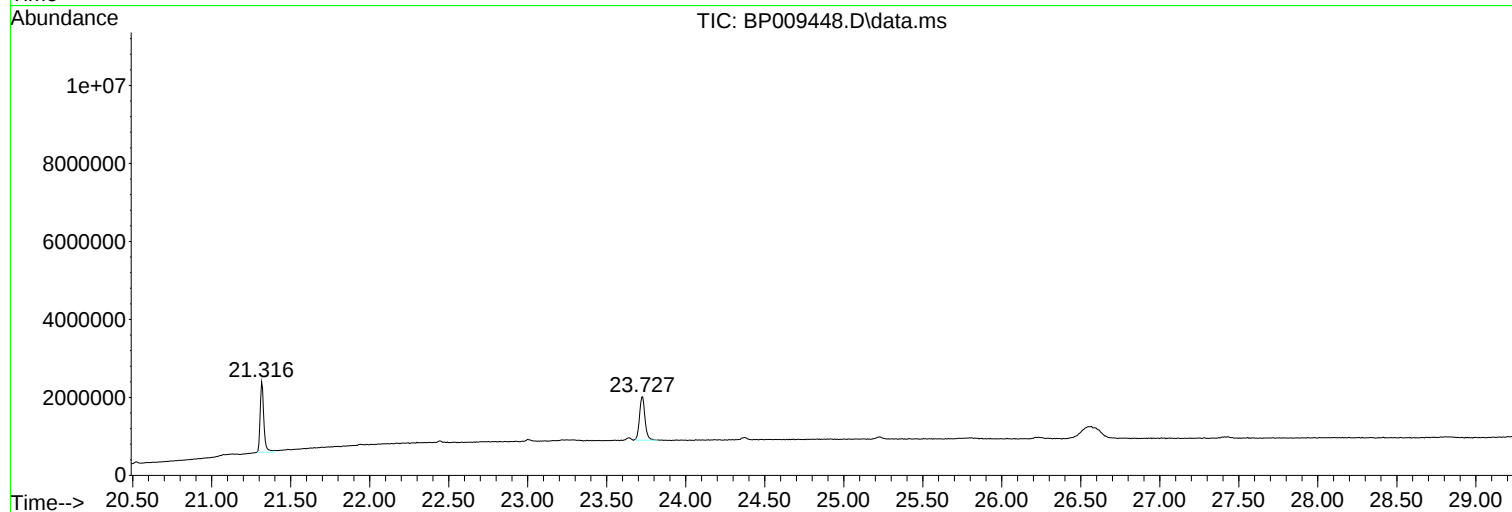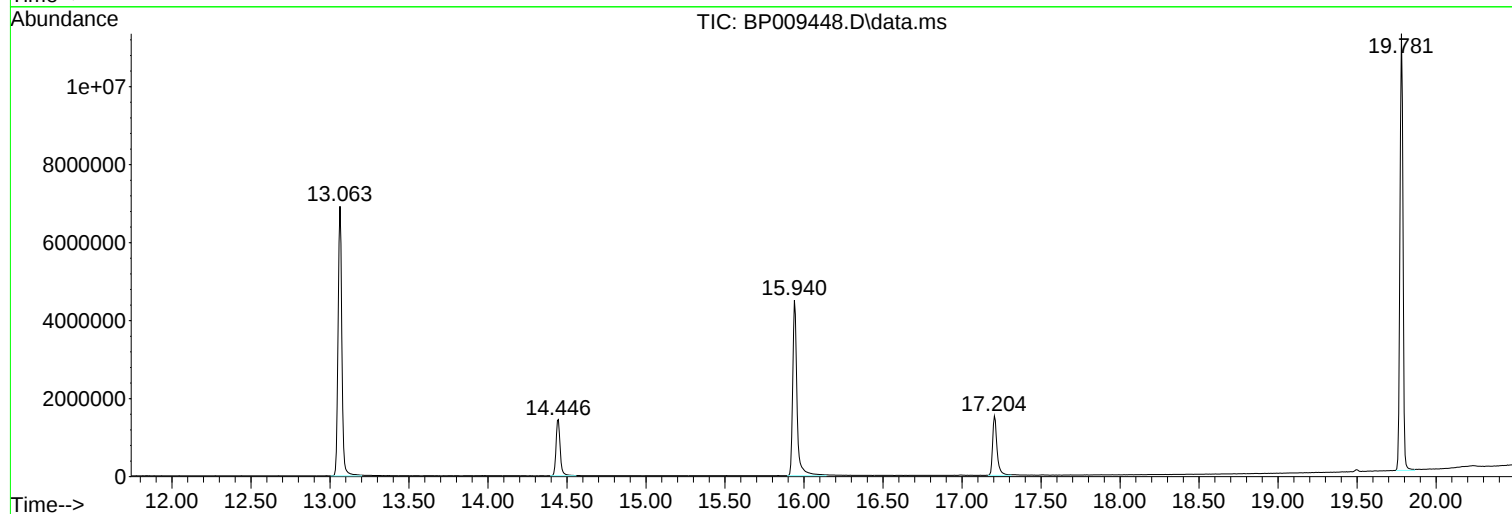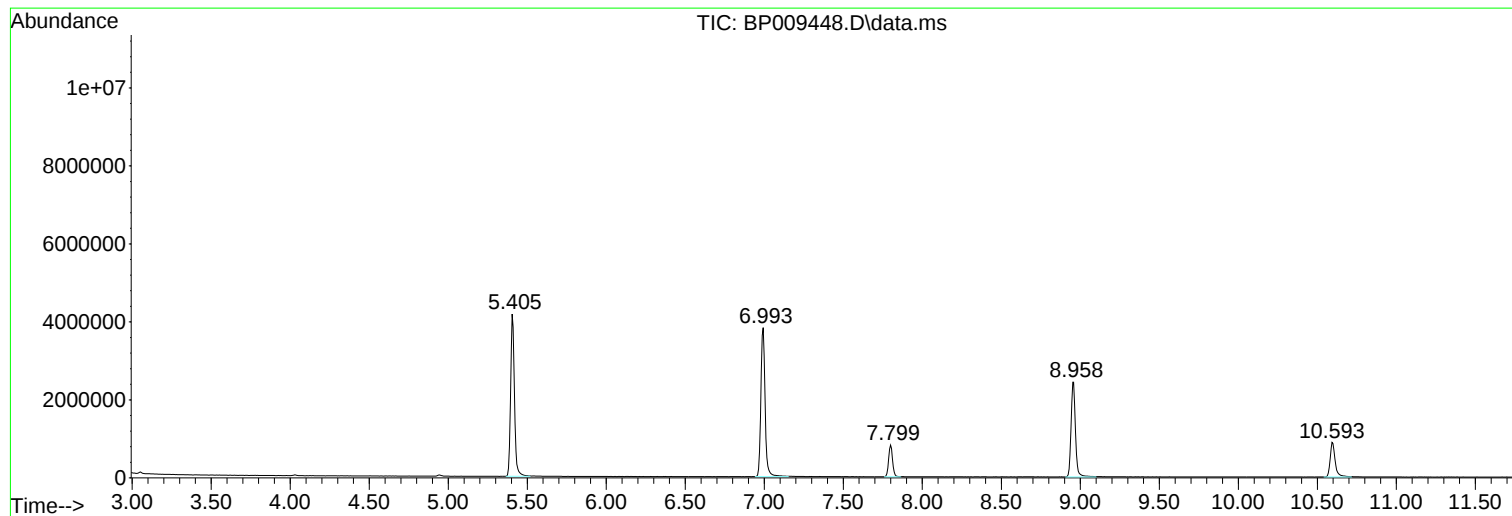

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031722\
Data File : BP009448.D
Acq On : 17 Mar 2022 17:43
Operator : CG/JU
Sample : PB143199BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB143199BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031722\
Data File : BP009448.D
Acq On : 17 Mar 2022 17:43
Operator : CG/JU
Sample : PB143199BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB143199BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------