
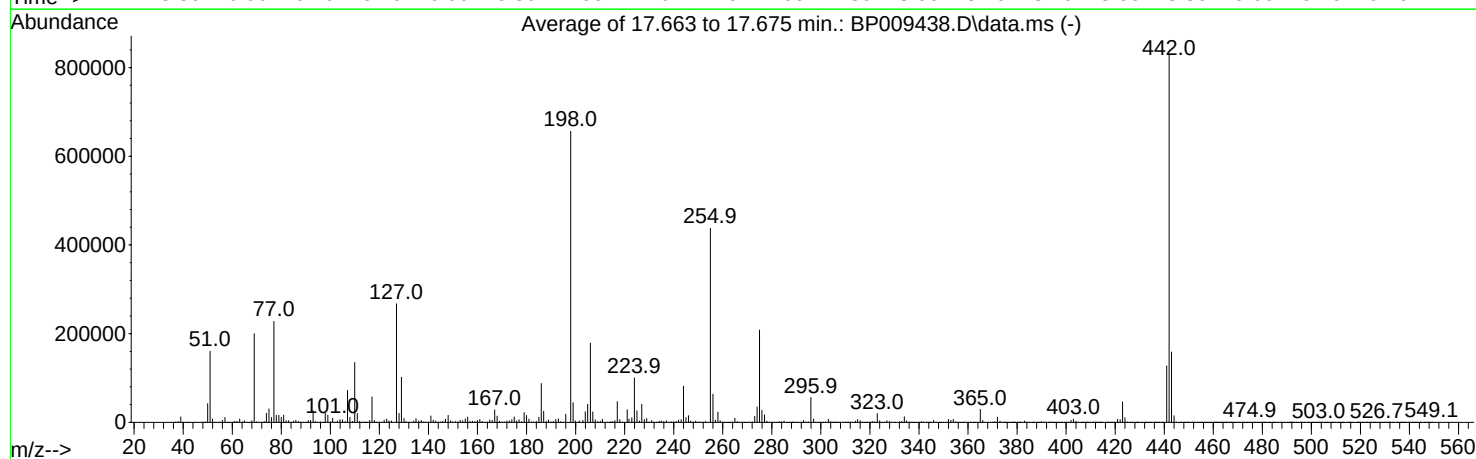


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031722\
 Data File : BP009438.D
 Acq On : 17 Mar 2022 11:02
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031722.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Mar 17 18:26:53 2022

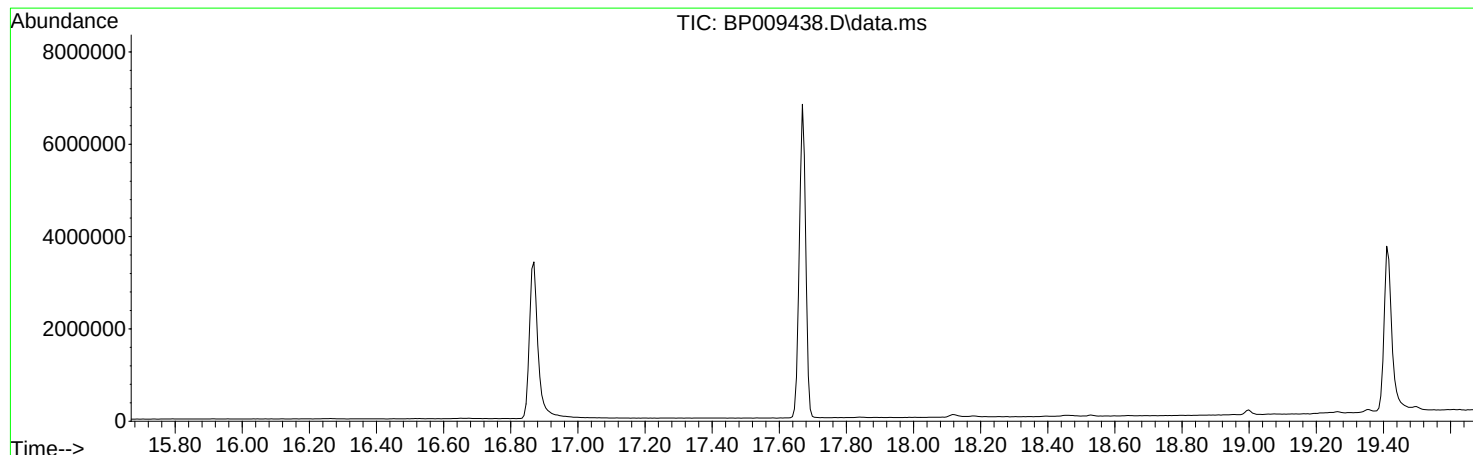




AutoFind: Scans 2495, 2496, 2497; Background Corrected with Scan 2484

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	24.4	160209	PASS
68	69	0.00	2	1.8	3666	PASS
69	198	0.00	100	30.4	199753	PASS
70	69	0.00	2	0.5	1097	PASS
127	198	10	80	40.8	267506	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	656330	PASS
199	198	5	9	6.8	44464	PASS
275	198	10	60	31.7	208043	PASS
365	198	1	100	4.4	29181	PASS
441	198	0.01	100	19.4	127516	PASS
442	442	100	100	100.0	829461	PASS
443	442	15	24	19.1	158797	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031722\
 Data File : BP009438.D
 Acq On : 17 Mar 2022 11:02
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Mar 17 17:36:13 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031722.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 17 17:31:41 2022
 Response via : Initial Calibration

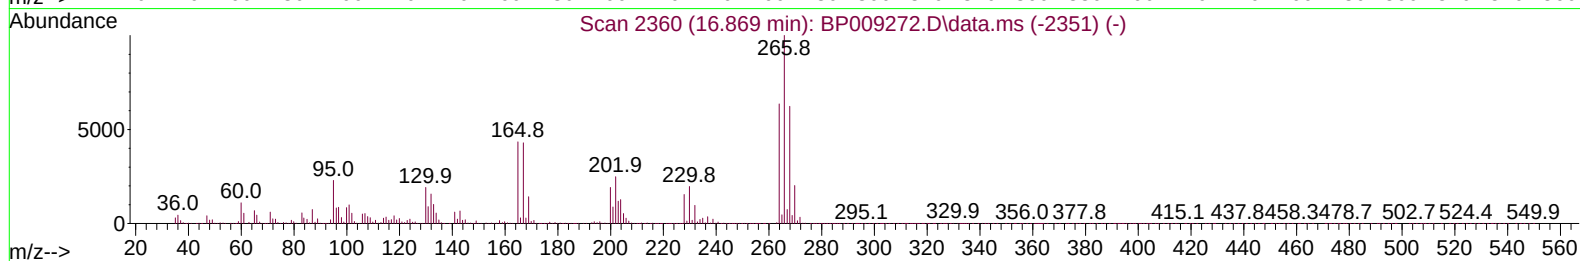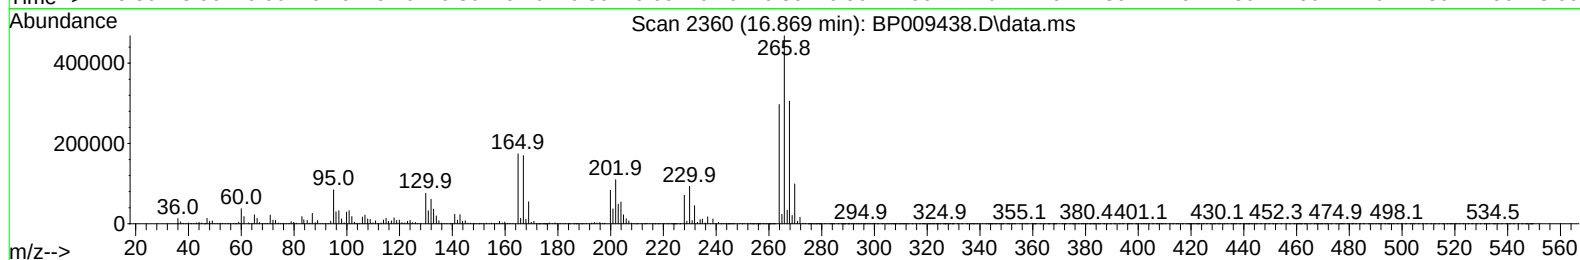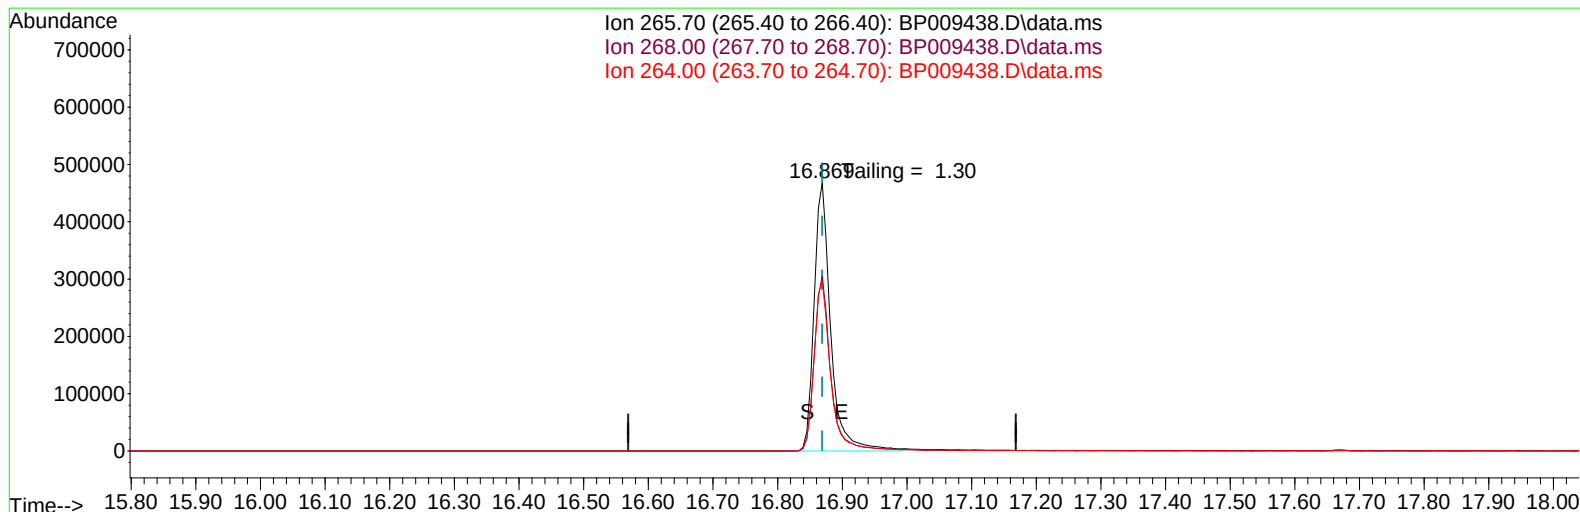

TIC: BP009438.D\data.ms

(70) Pentachlorophenol (C)

16.869min (-0.000) 231964.98 ng




response 844504

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.30	65.16
264.00	63.60	63.40
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031722\
Data File : BP009438.D
Acq On : 17 Mar 2022 11:02
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Mar 17 17:36:13 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 17 17:31:41 2022
Response via : Initial Calibration

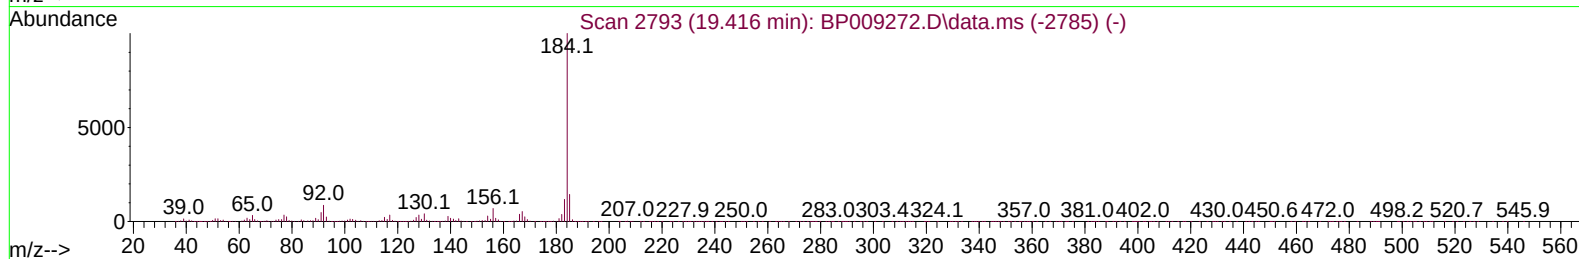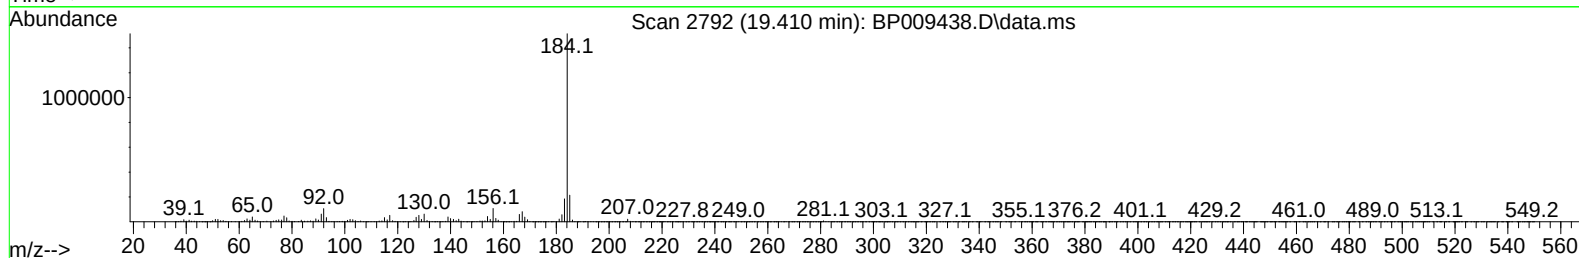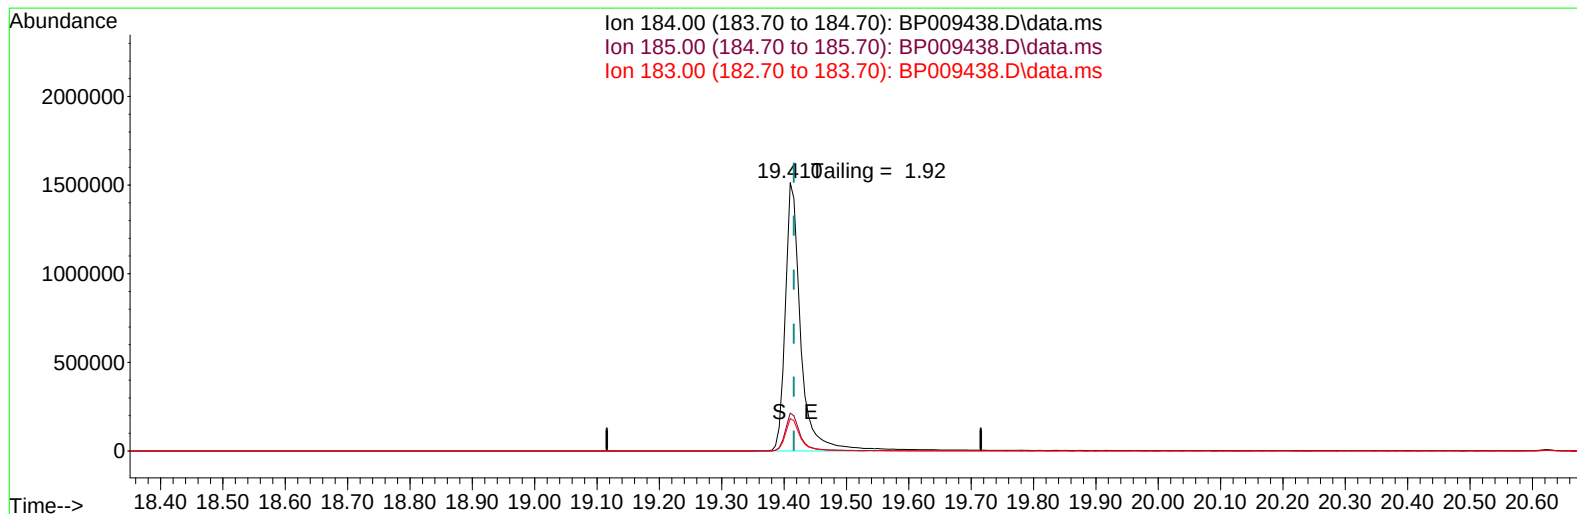

TIC: BP009438.D\data.ms

(77) Benzidine

19.410min (-0.006) 26964.59 ng

response 2650332

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.17
183.00	11.70	12.14
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/17/2022	BNA_P	<u>BP009438.D</u>
Compound Name	Response	Retention Time
DDT	2227573	20.62
DDD	25967	20.19
DDE	3356	19.69
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
29323	2256896	1.30

Instrument :
BNA_P
ClientSampleId :
DFTPP