


Data Path : Z:\SVOASRV\HPCHEM1\BNA_P\DATA\BP031820\
 Data File : BP002215.D
 Acq On : 18 Mar 2020 14:45
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_P\METHODS\8270-BP031820.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Mar 18 19:28:43 2020

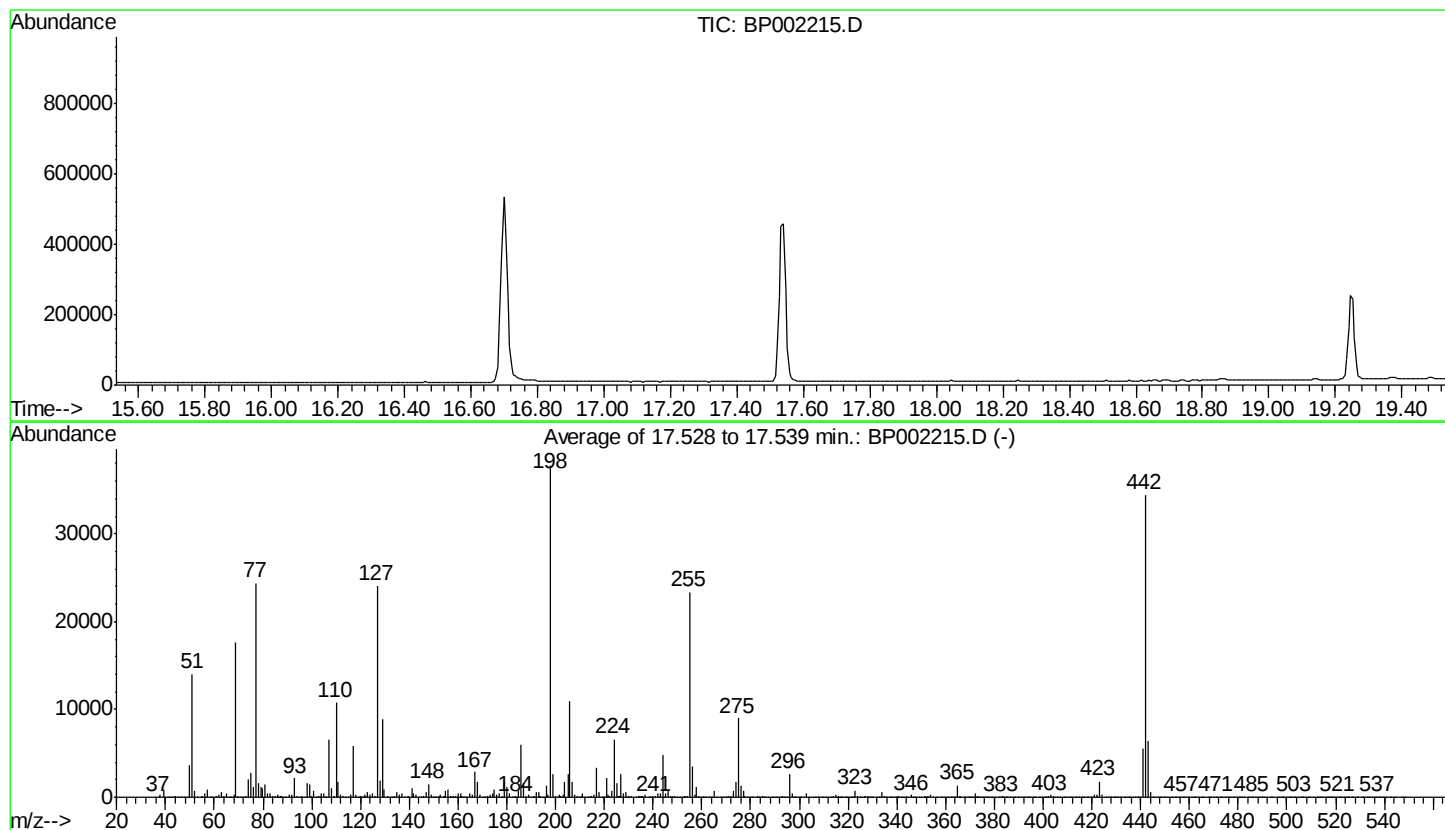

AutoFind: Scans 2489, 2490, 2491; Background Corrected with Scan 2483

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.2	14067	PASS
68	69	0.00	2	1.7	291	PASS
69	198	0.00	100	46.6	17591	PASS
70	69	0.00	2	0.7	129	PASS
127	198	10	80	63.7	24065	PASS
197	198	0.00	2	0.8	306	PASS
198	198	100	100	100.0	37773	PASS
199	198	5	9	6.8	2578	PASS
275	198	10	60	23.9	9029	PASS
365	198	1	100	3.5	1317	PASS
441	198	0.01	100	14.7	5563	PASS
442	198	50	100	91.2	34460	PASS
443	442	15	24	18.5	6384	PASS