
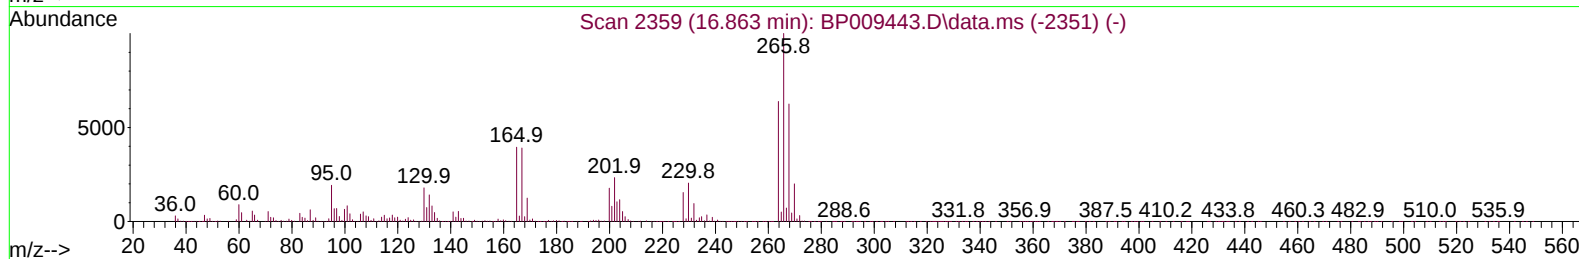
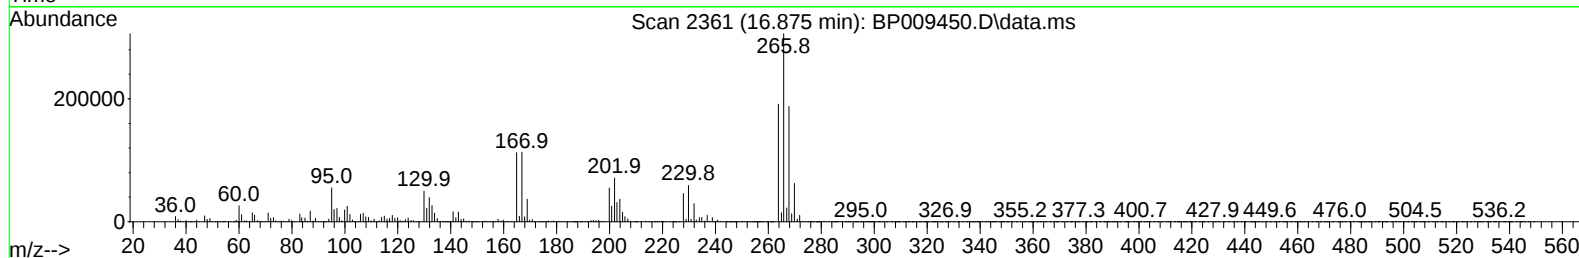


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031822\
Data File : BP009450.D
Acq On : 18 Mar 2022 10:36
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 18 15:06:43 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 17 18:26:53 2022
Response via : Initial Calibration

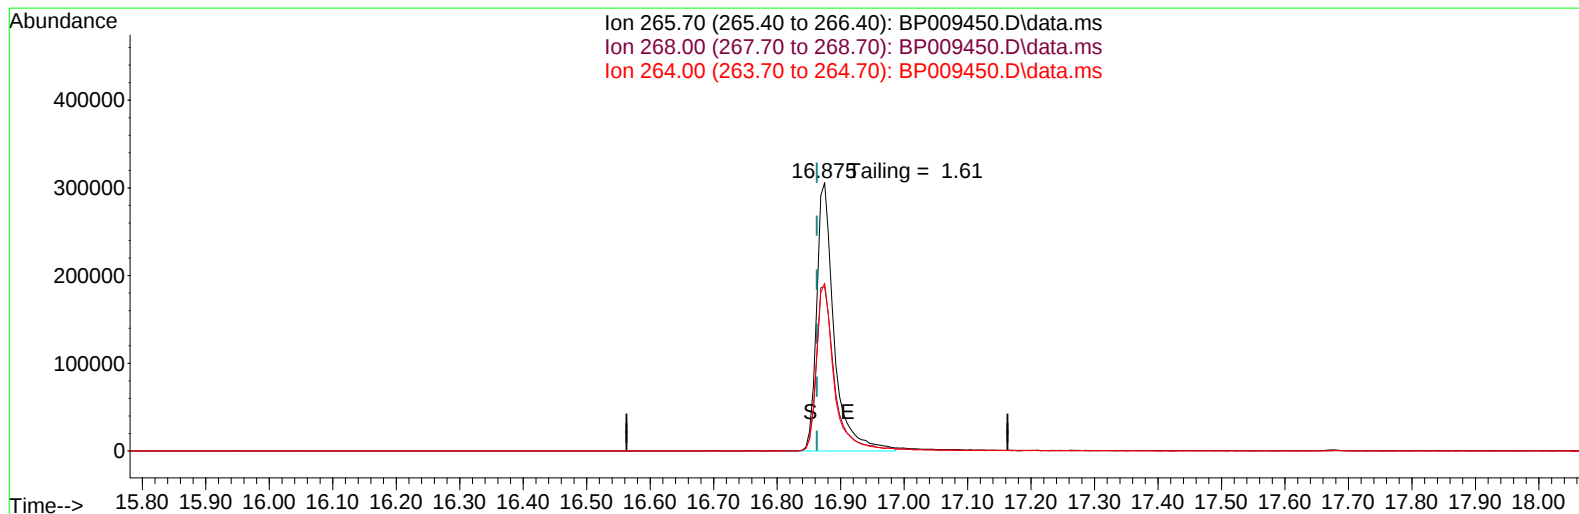

TIC: BP009450.D\data.ms

(70) Pentachlorophenol (C)




16.875min (+ 0.012) 46455.55 ng

response 594887

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.30	61.31
264.00	63.60	62.54
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031822\
 Data File : BP009450.D
 Acq On : 18 Mar 2022 10:36
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 18 15:06:43 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031722.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 17 18:26:53 2022
 Response via : Initial Calibration

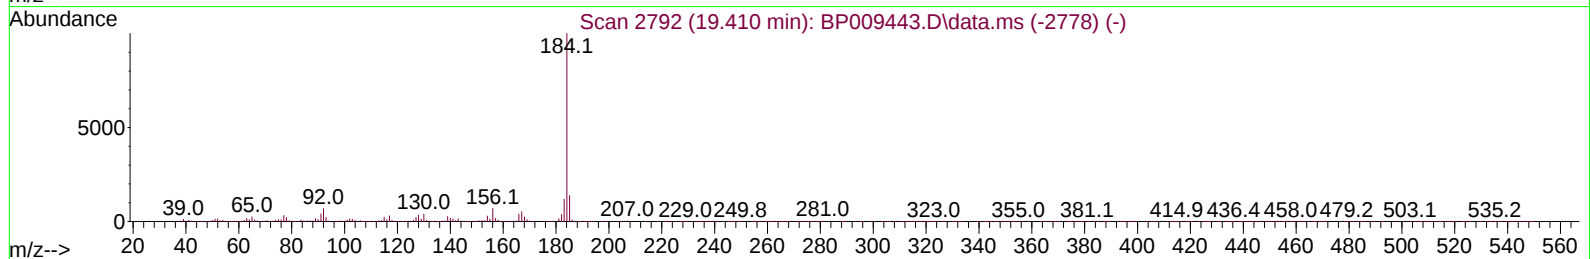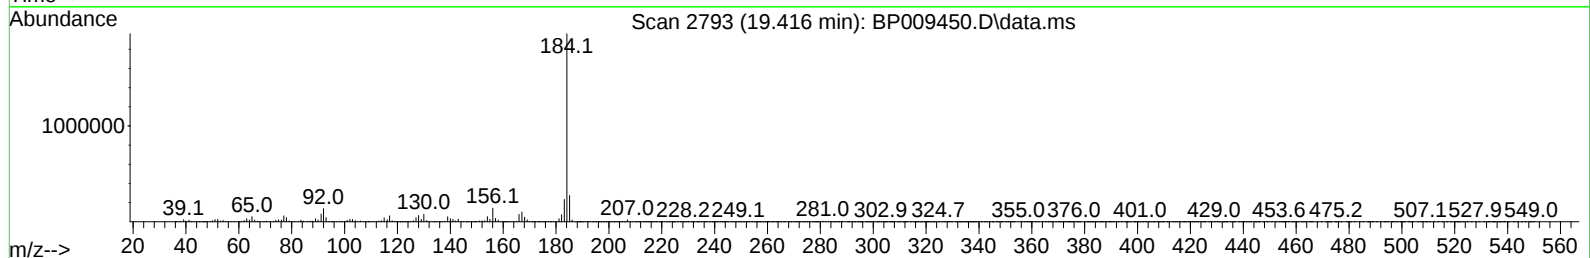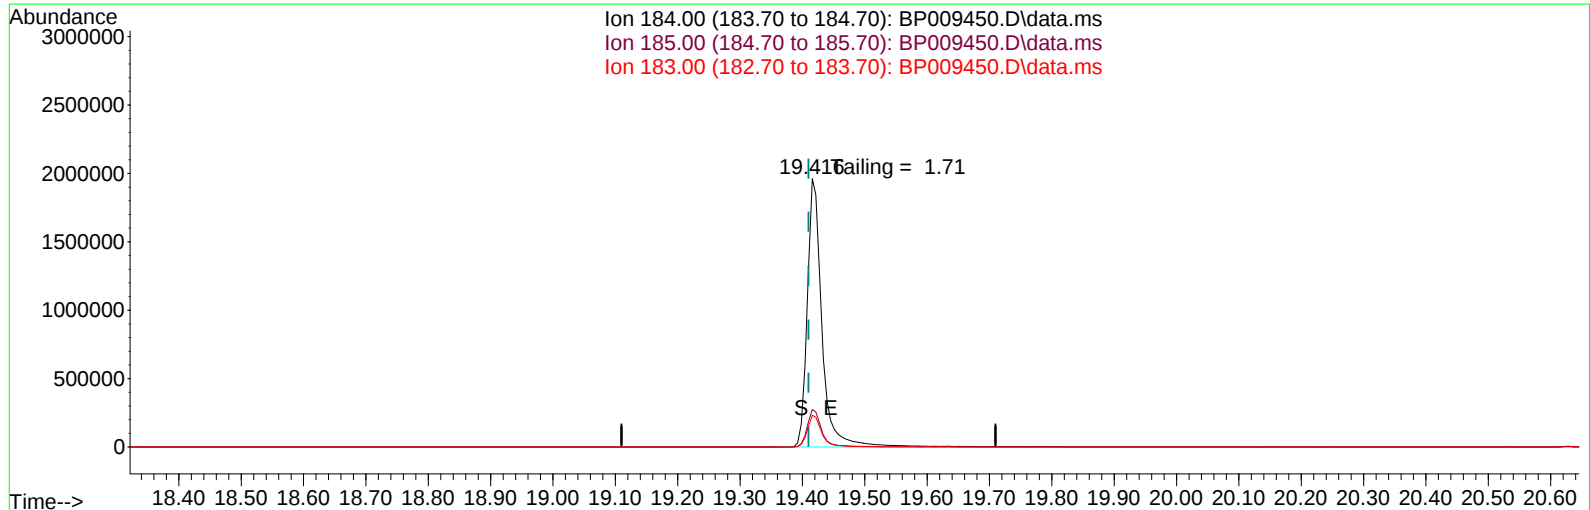

TIC: BP009450.D\data.ms

(77) Benzidine**19.416min (+ 0.006) 14059.22 ng****response 3226583**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	13.97
183.00	11.70	11.81
0.00	0.00	0.00