

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031822\
 Data File : BP009452.D
 Acq On : 18 Mar 2022 11:53
 Operator : CG/JU
 Sample : PB143161BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB143161BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031722.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP009452.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.405	404	411	436	rBV	4402437	7455995	44.01%	9.802%
2	6.993	672	681	708	rBV	3875053	7368475	43.49%	9.687%
3	7.799	811	818	831	rBV	968736	1673004	9.87%	2.199%
4	8.958	1005	1015	1042	rBV	2499222	4894104	28.89%	6.434%
5	10.593	1283	1293	1313	rBV	1047011	2281047	13.46%	2.999%
6	13.063	1705	1713	1740	rBV	7340976	12261632	72.37%	16.120%
7	14.445	1939	1948	1969	rBV	1727511	3172045	18.72%	4.170%
8	15.940	2195	2202	2234	rBV	5162789	9453093	55.79%	12.428%
9	17.204	2410	2417	2437	rBV	2015315	3650851	21.55%	4.800%
10	19.780	2849	2855	2868	rBV	12692662	16942956	100.00%	22.275%
11	21.316	3111	3116	3128	rBV	2211688	3561123	21.02%	4.682%
12	23.721	3518	3525	3540	rVB2	1353918	3349357	19.77%	4.403%




Sum of corrected areas: 76063682

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031822\
Data File : BP009452.D
Acq On : 18 Mar 2022 11:53
Operator : CG/JU
Sample : PB143161BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB143161BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

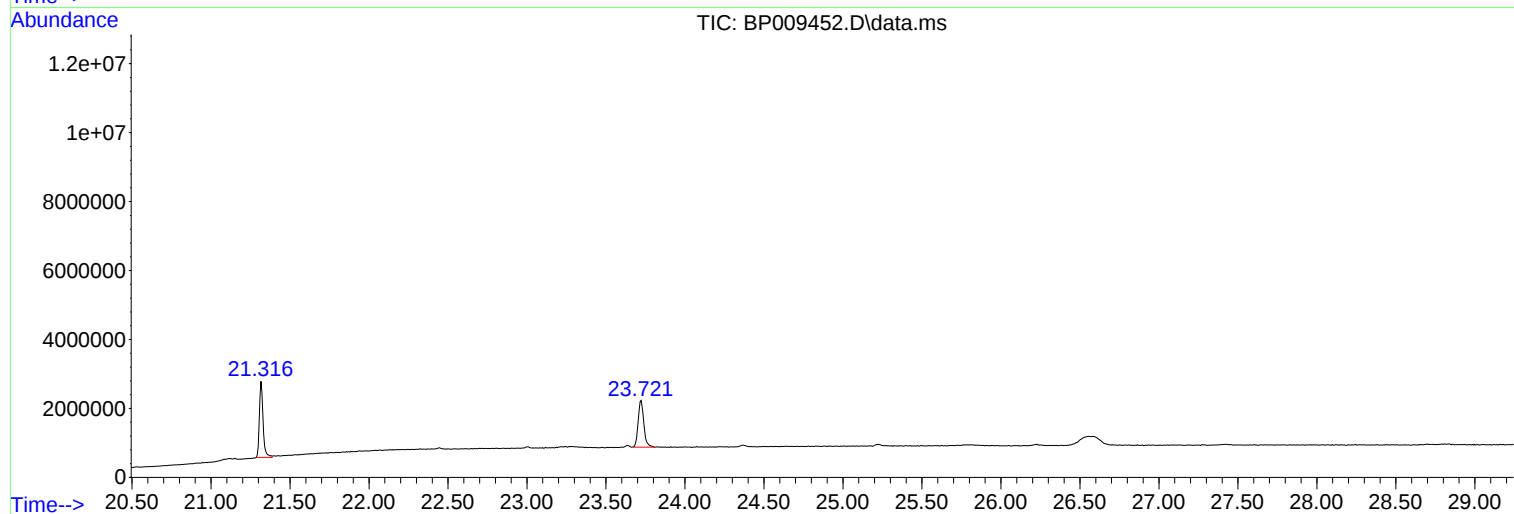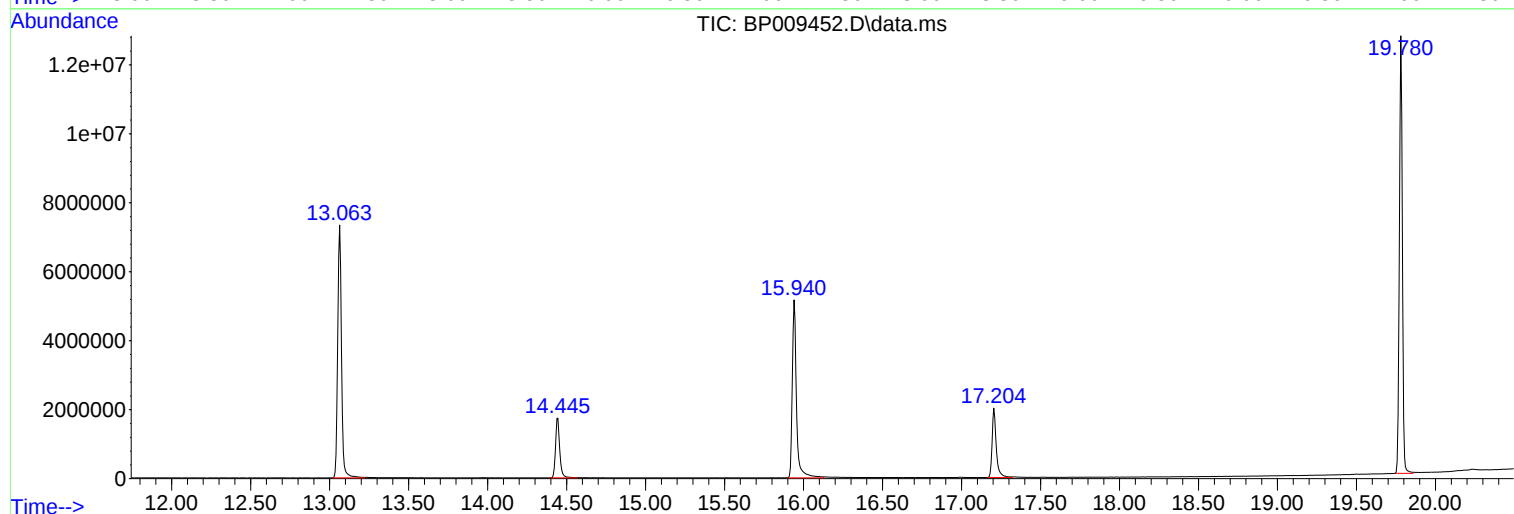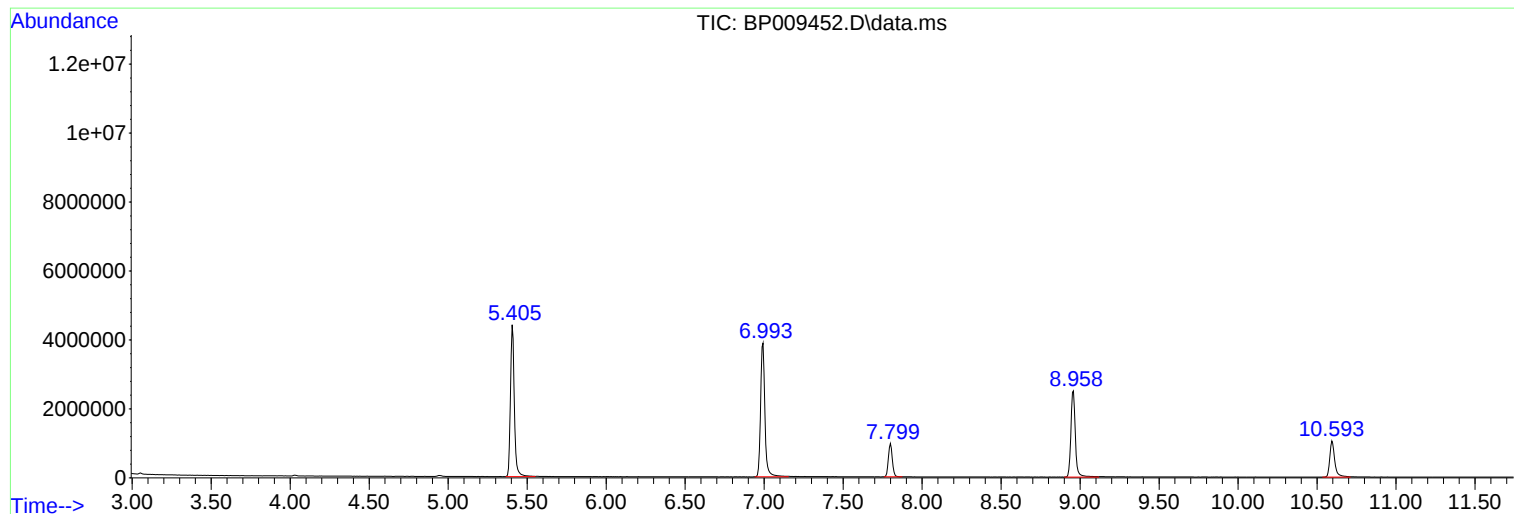

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031822\
Data File : BP009452.D
Acq On : 18 Mar 2022 11:53
Operator : CG/JU
Sample : PB143161BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB143161BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031822\
Data File : BP009452.D
Acq On : 18 Mar 2022 11:53
Operator : CG/JU
Sample : PB143161BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB143161BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------