

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031822\
Data File : BP009457.D
Acq On : 18 Mar 2022 14:54
Operator : CG/JU
Sample : PB143171BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB143171BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031722.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP009457.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.405	404	411	430	rBV	4488864	7658186	47.31%	10.091%
2	6.987	672	680	699	rBV	4079016	7588687	46.88%	9.999%
3	7.799	809	818	835	rBV	1004907	1752235	10.82%	2.309%
4	8.952	1006	1014	1039	rBV	2612462	5107128	31.55%	6.730%
5	10.593	1284	1293	1318	rBV	1079320	2349597	14.51%	3.096%
6	13.063	1705	1713	1737	rBV	7360702	12472412	77.05%	16.435%
7	14.439	1938	1947	1974	rBV	1821605	3236983	20.00%	4.265%
8	15.939	2193	2202	2233	rBV	5187367	9293752	57.41%	12.246%
9	17.204	2409	2417	2437	rBV	1899900	3621197	22.37%	4.772%
10	19.780	2849	2855	2868	rBV	12328161	16187884	100.00%	21.330%
11	21.316	3111	3116	3128	rBV	2032654	3408617	21.06%	4.491%
12	23.715	3518	3524	3542	rVB2	1258256	3214714	19.86%	4.236%




Sum of corrected areas: 75891392

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031822\
Data File : BP009457.D
Acq On : 18 Mar 2022 14:54
Operator : CG/JU
Sample : PB143171BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB143171BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

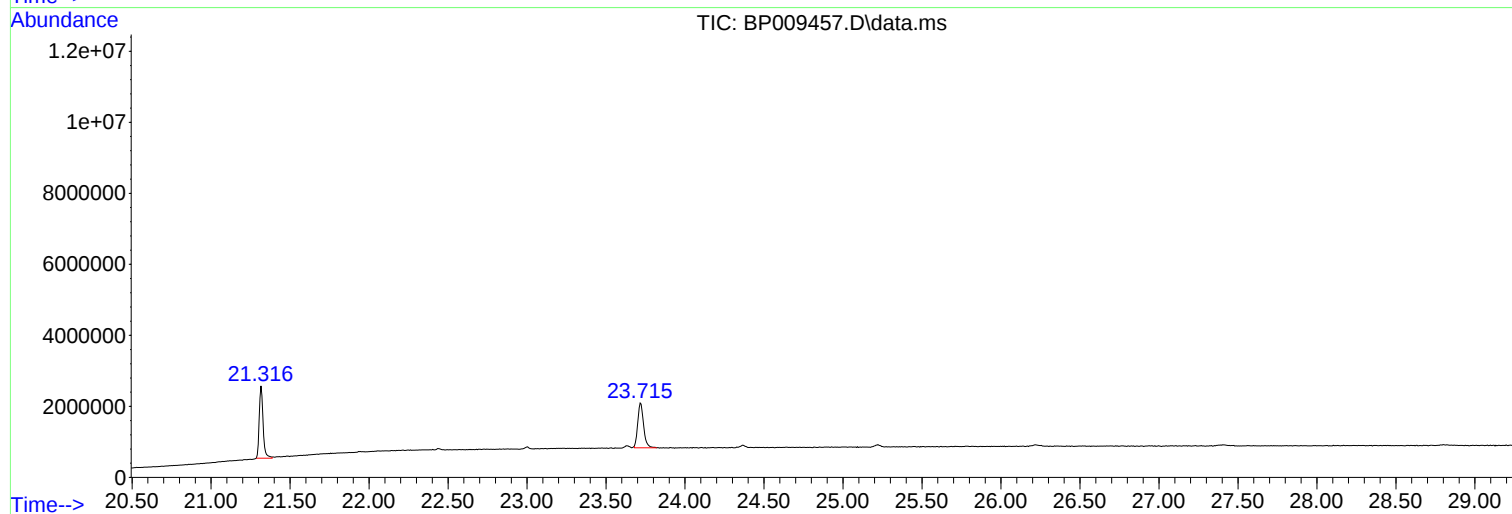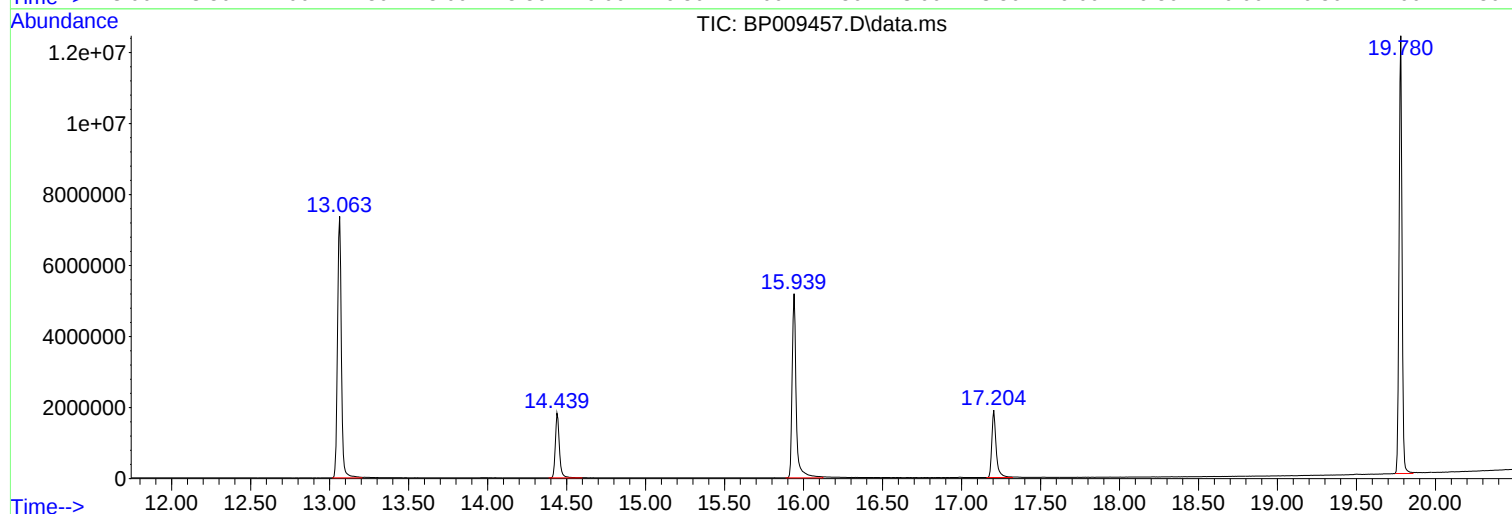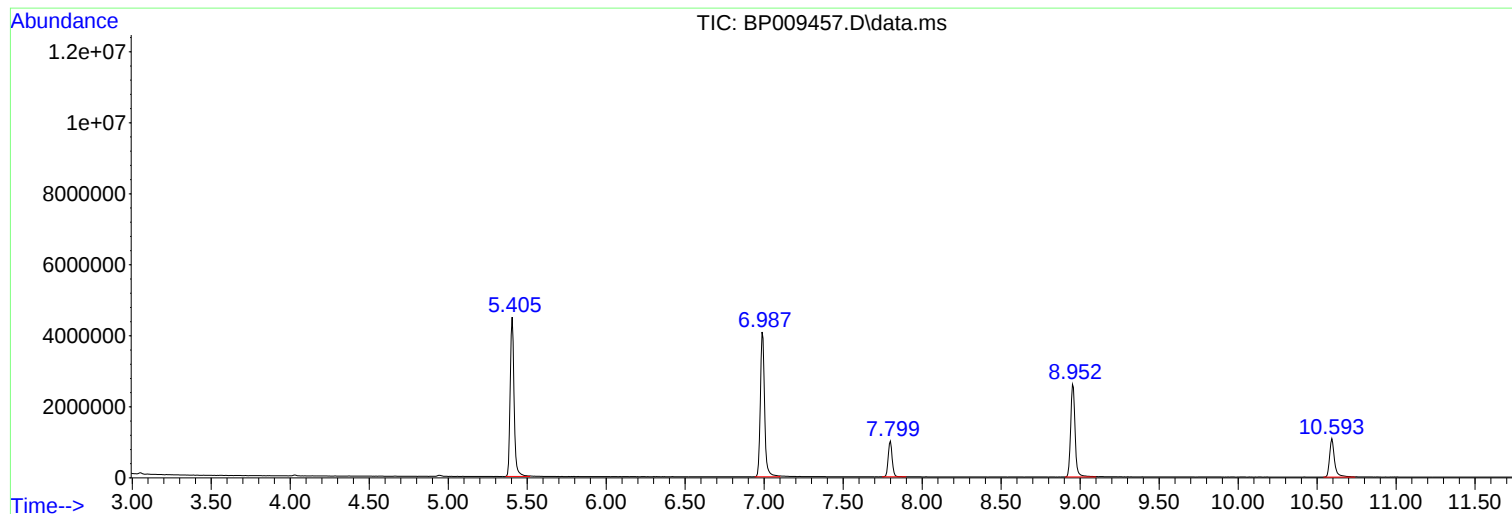

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031822\
Data File : BP009457.D
Acq On : 18 Mar 2022 14:54
Operator : CG/JU
Sample : PB143171BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB143171BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031822\
Data File : BP009457.D
Acq On : 18 Mar 2022 14:54
Operator : CG/JU
Sample : PB143171BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB143171BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------