
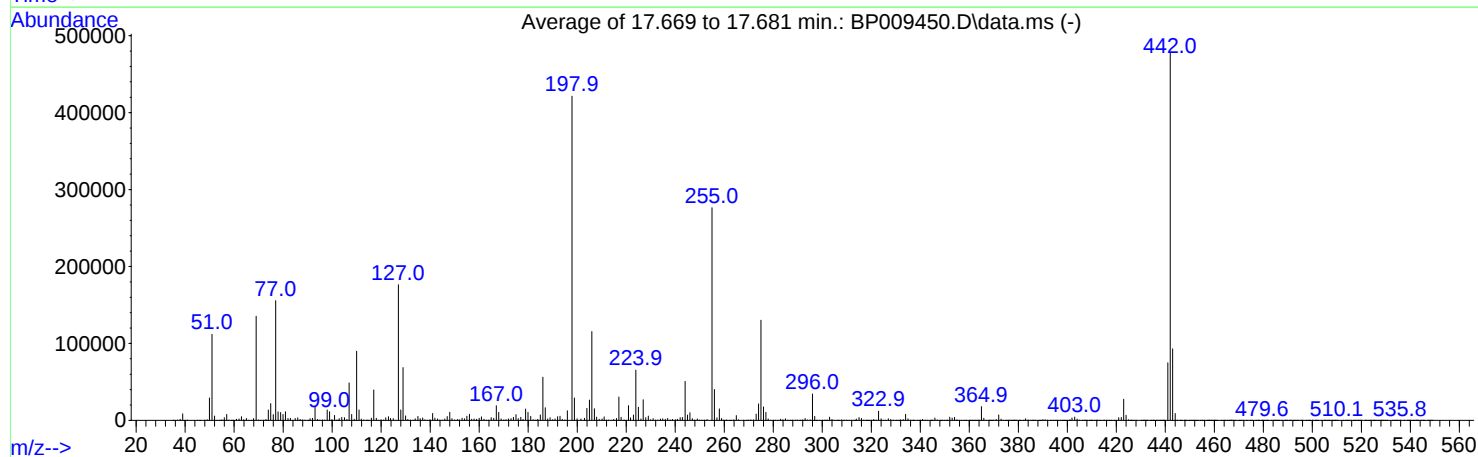


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031822\
 Data File : BP009450.D
 Acq On : 18 Mar 2022 10:36
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031722.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Mar 17 18:26:53 2022

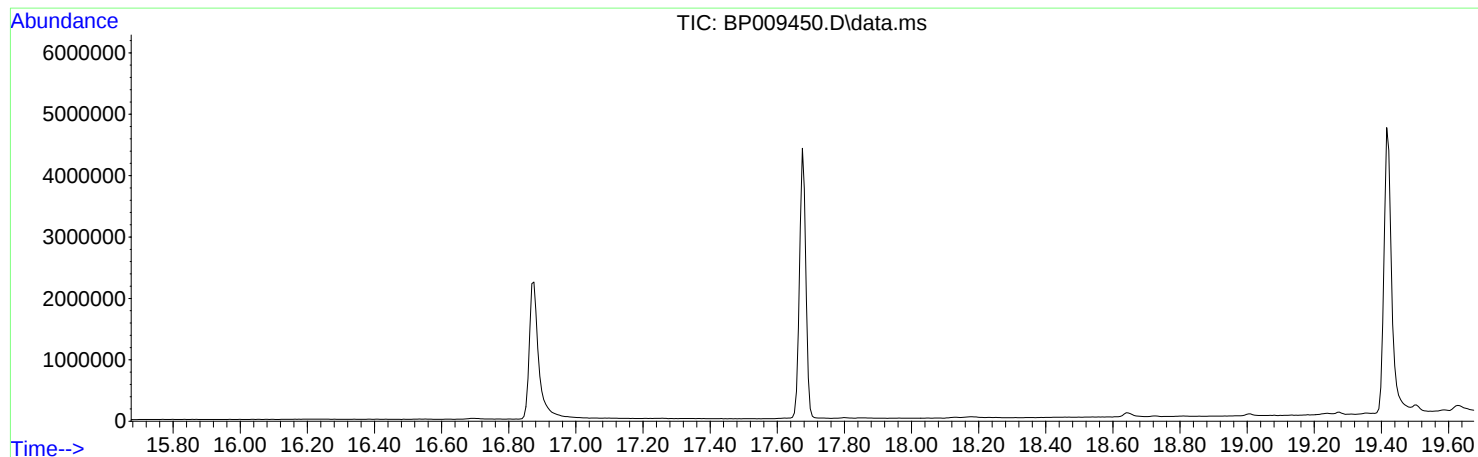




AutoFind: Scans 2496, 2497, 2498; Background Corrected with Scan 2485

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	26.6	111993	PASS
68	69	0.00	2	1.7	2322	PASS
69	198	0.00	100	32.1	135348	PASS
70	69	0.00	2	0.5	734	PASS
127	198	10	80	41.8	176299	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	421347	PASS
199	198	5	9	6.9	29103	PASS
275	198	10	60	30.9	130231	PASS
365	198	1	100	4.2	17826	PASS
441	198	0.01	100	17.8	74978	PASS
442	442	100	100	100.0	478165	PASS
443	442	15	24	19.5	93080	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031822\
Data File : BP009450.D
Acq On : 18 Mar 2022 10:36
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Mar 18 15:06:43 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 17 18:26:53 2022
Response via : Initial Calibration

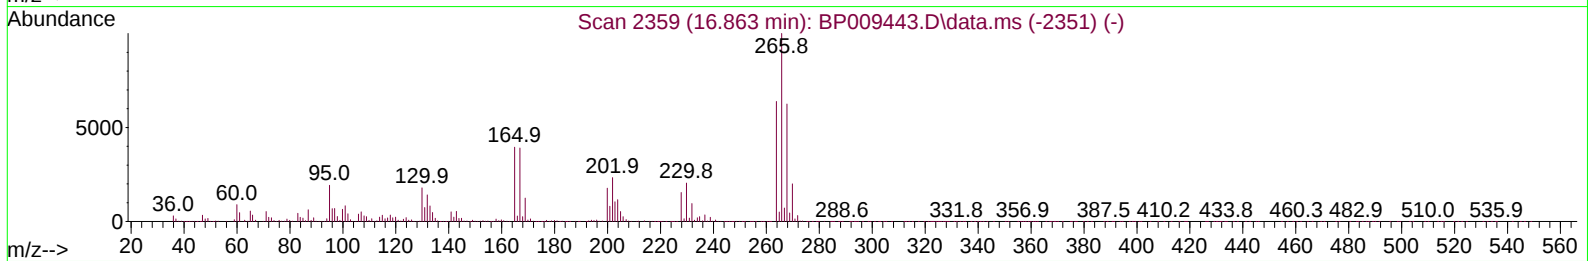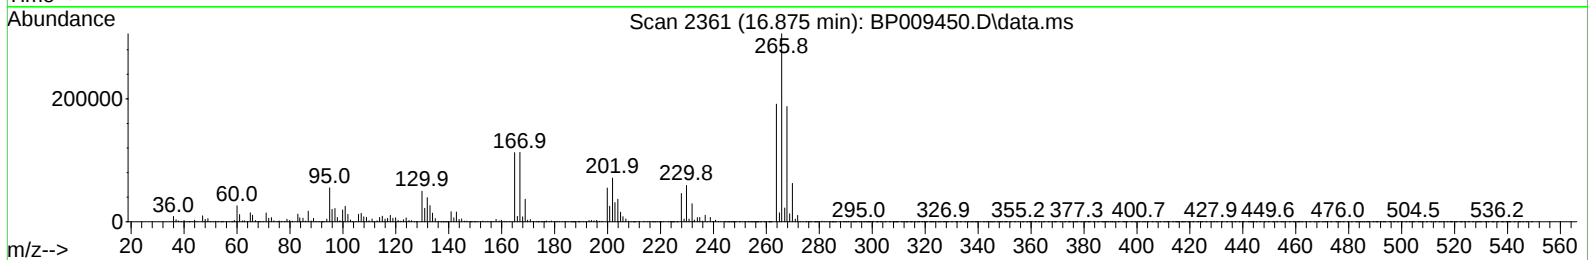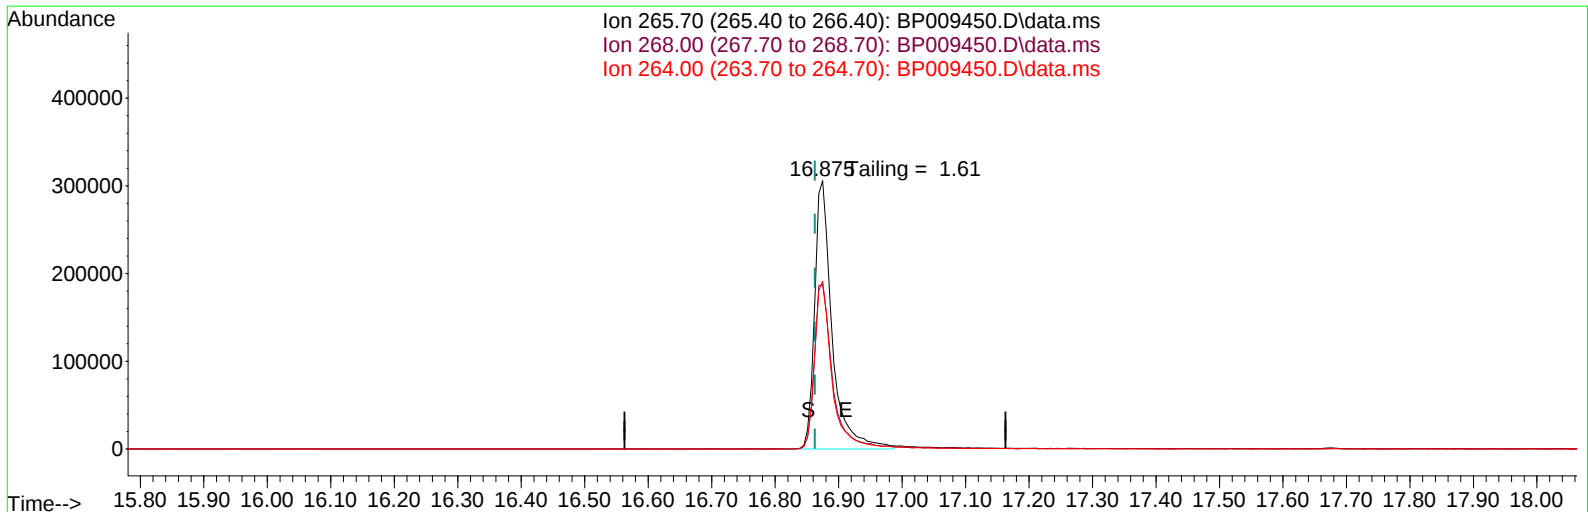

TIC: BP009450.D\data.ms

(70) Pentachlorophenol (C)

16.875min (+ 0.012) 46455.55 ng




response 594887

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.30	61.31
264.00	63.60	62.54
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031822\
Data File : BP009450.D
Acq On : 18 Mar 2022 10:36
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Mar 18 15:06:43 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 17 18:26:53 2022
Response via : Initial Calibration

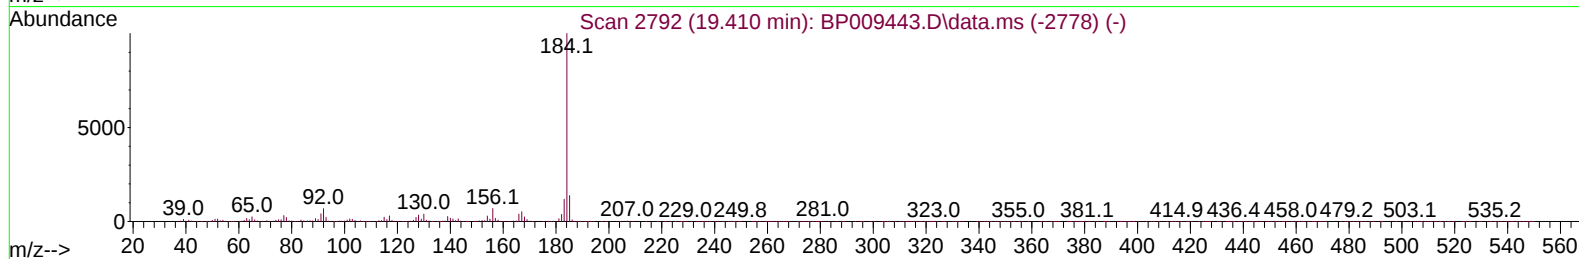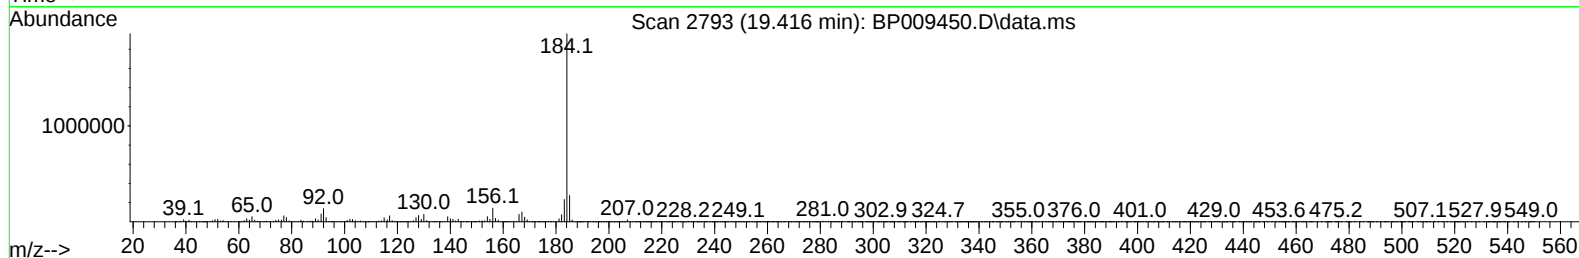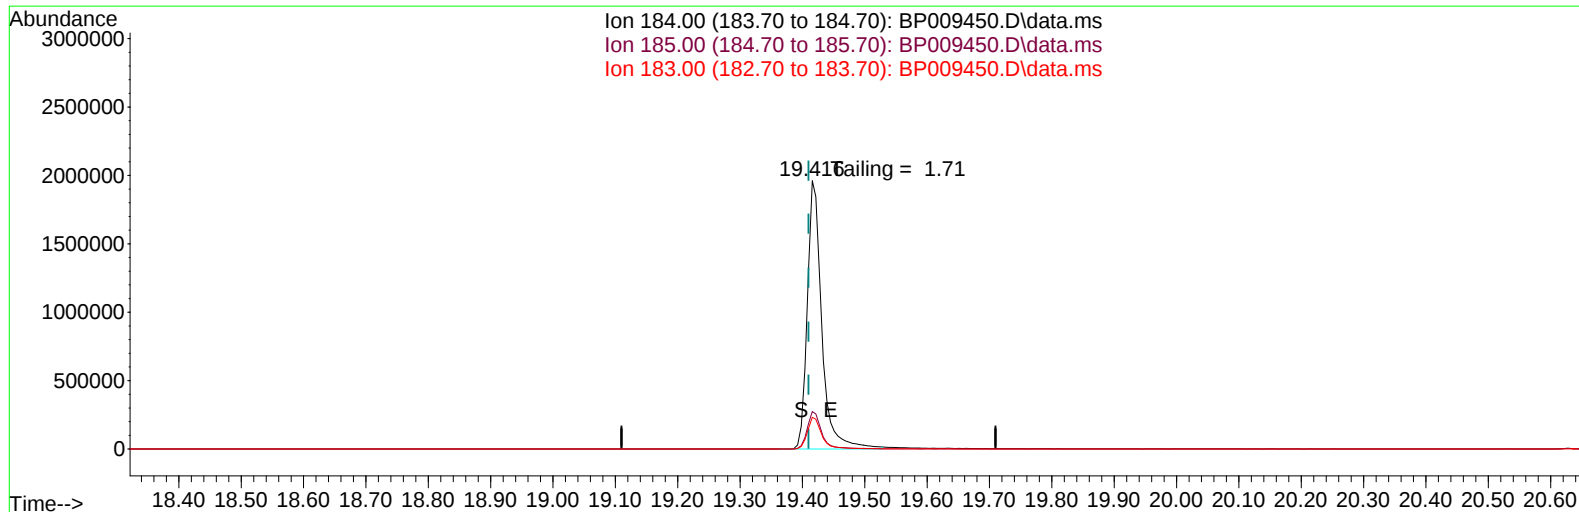

TIC: BP009450.D\data.ms

(77) Benzidine

19.416min (+ 0.006) 14059.22 ng

response 3226583

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	13.97
183.00	11.70	11.81
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/18/2022	BNA_P	<u>BP009450.D</u>
Compound Name	Response	Retention Time
DDT	1569890	20.62
DDD	11468	20.04
DDE	2551	19.71
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
14019	1583909	0.89

Instrument :
BNA_P
ClientSampleId :
DFTPP