
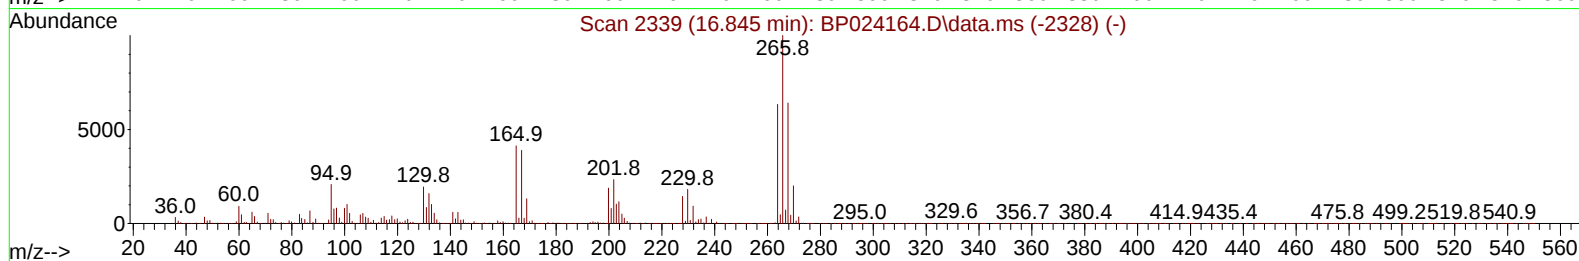
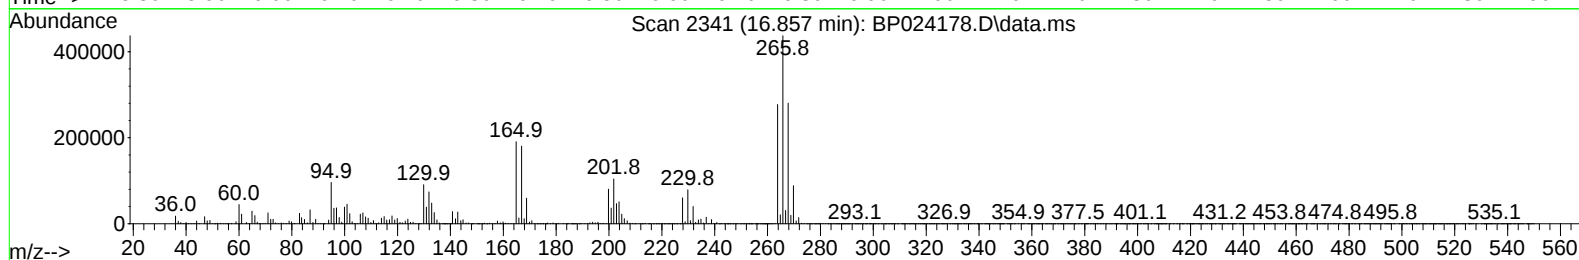


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031825\
Data File : BP024178.D
Acq On : 18 Mar 2025 09:05
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 18 11:07:09 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 13 05:55:58 2025
Response via : Initial Calibration

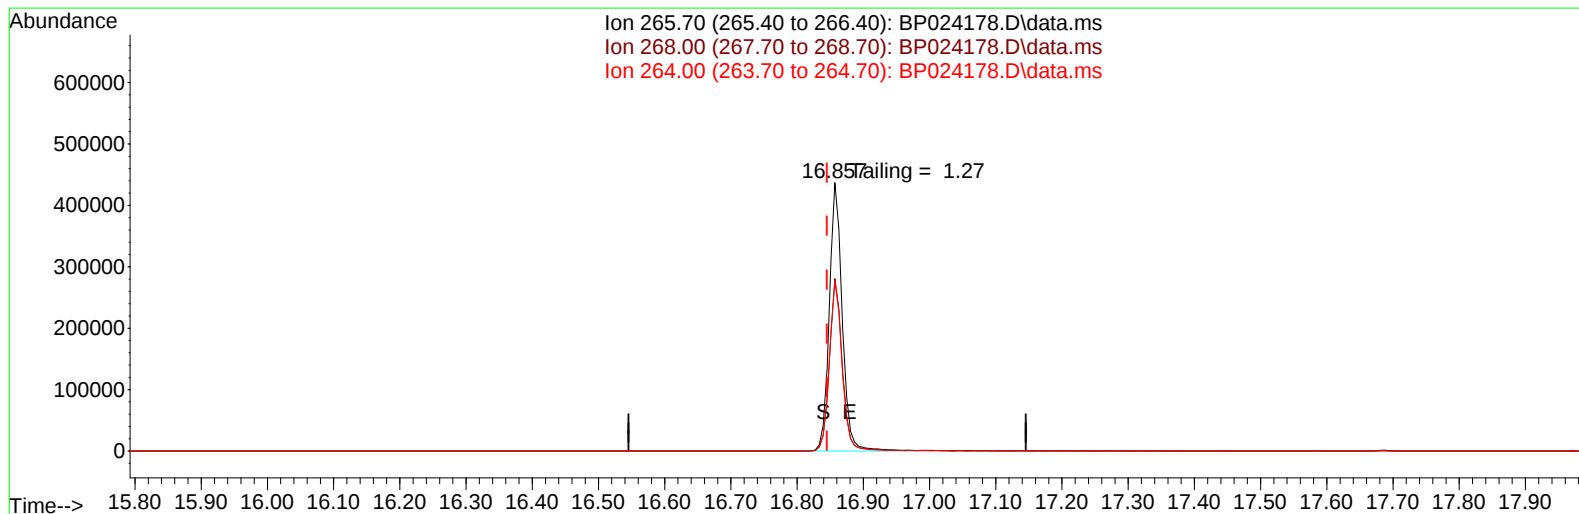

TIC: BP024178.D\data.ms

(70) Pentachlorophenol (C)




16.857min (+ 0.012) 196786.88 ng

response 593684

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	64.10	64.20
264.00	63.30	63.44
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031825\
Data File : BP024178.D
Acq On : 18 Mar 2025 09:05
Operator : RC/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 18 14:43:45 2025
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 13 05:55:58 2025
Response via : Initial Calibration

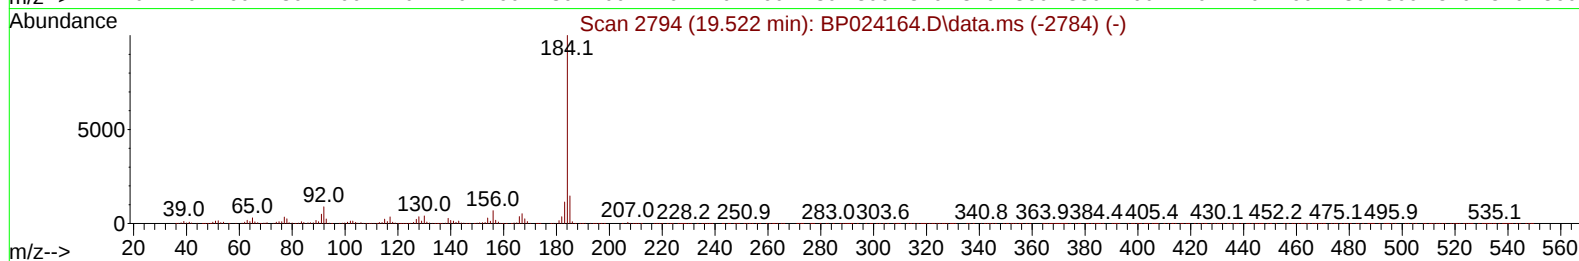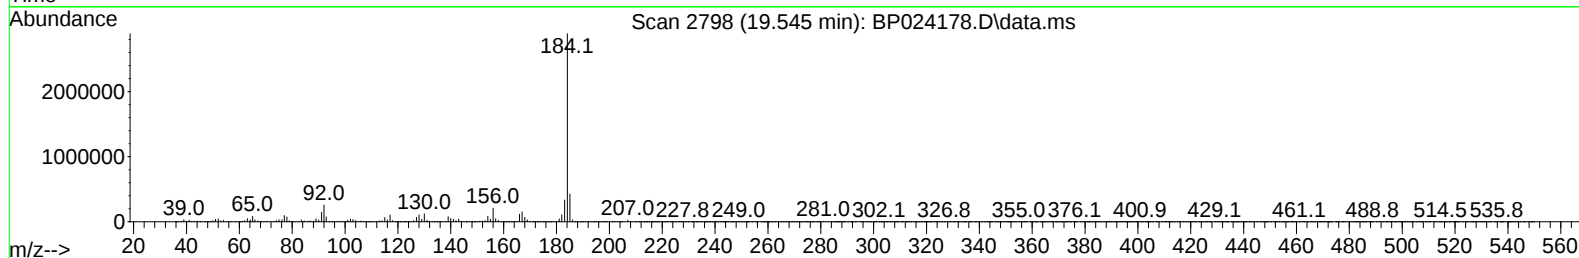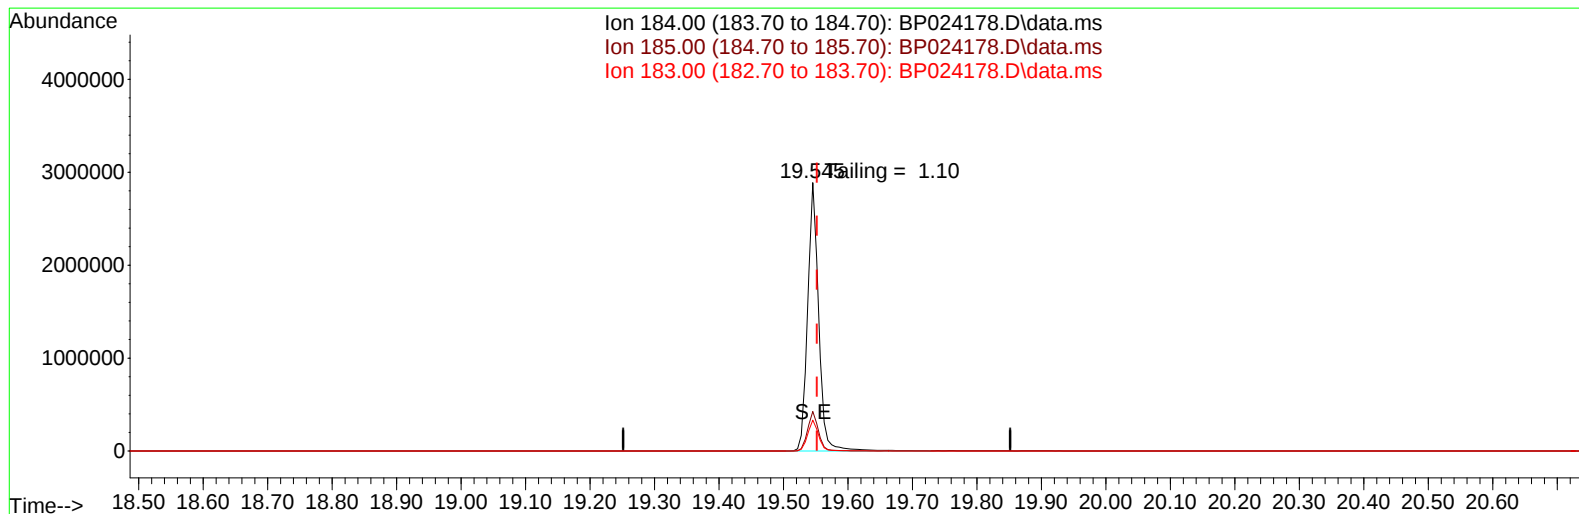

TIC: BP024178.D\data.ms

(77) Benzidine

19.545min (-0.006) 19199.87 ng

response 3449621

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.70	14.74
183.00	11.40	11.55
0.00	0.00	0.00