

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031825\
 Data File : BP024180.D
 Acq On : 18 Mar 2025 10:26
 Operator : RC/JU
 Sample : PB167157BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB167157BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031225.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP024180.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.381	383	390	407	rBV	7311118	9918018	47.31%	10.613%
2	6.946	648	656	675	rBV	6239505	10106661	48.20%	10.815%
3	7.769	788	796	805	rBV	1195498	1873988	8.94%	2.005%
4	8.916	982	991	1010	rBV	3855737	6296564	30.03%	6.738%
5	10.545	1259	1268	1287	rBV	1609048	2635931	12.57%	2.821%
6	13.010	1679	1687	1705	rBV	10358179	15342918	73.18%	16.418%
7	14.404	1917	1924	1945	rBV	2438301	3463550	16.52%	3.706%
8	15.922	2174	2182	2208	rBV	7031691	10863307	51.81%	11.625%
9	17.204	2394	2400	2413	rBV2	2569310	3851215	18.37%	4.121%
10	19.933	2858	2864	2878	rBV	16041623	20966090	100.00%	22.435%
11	21.663	3152	3158	3170	rBV2	2620829	4042822	19.28%	4.326%
12	25.051	3726	3734	3751	rVB	1494967	4090303	19.51%	4.377%




Sum of corrected areas: 93451367

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031825\
Data File : BP024180.D
Acq On : 18 Mar 2025 10:26
Operator : RC/JU
Sample : PB167157BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB167157BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

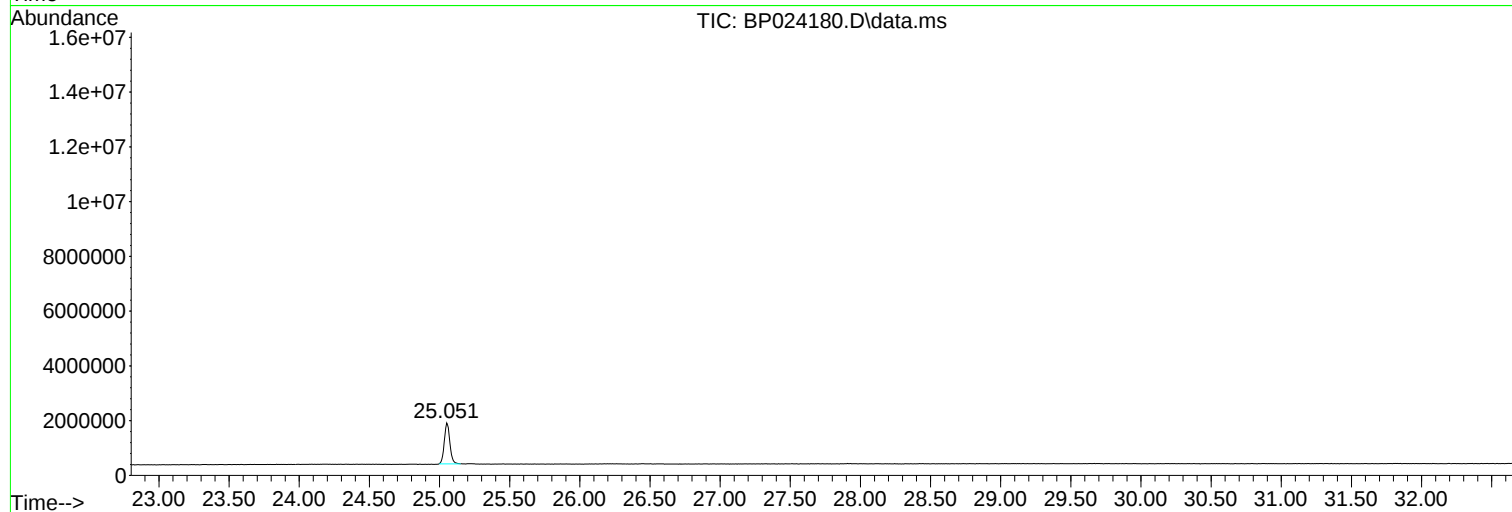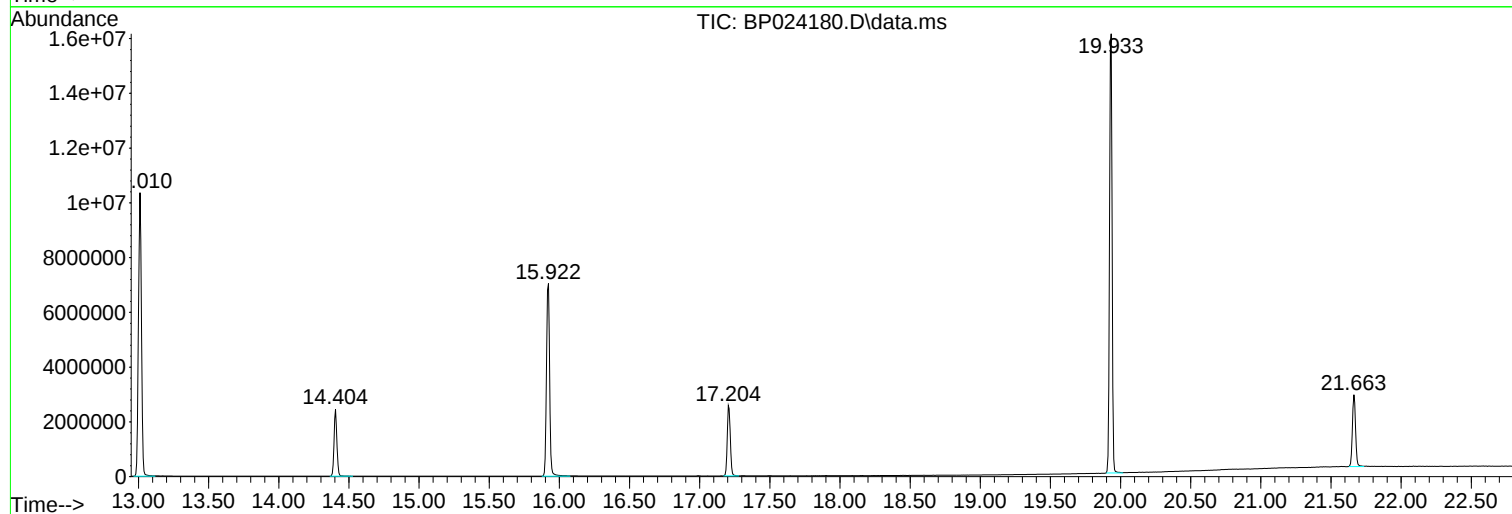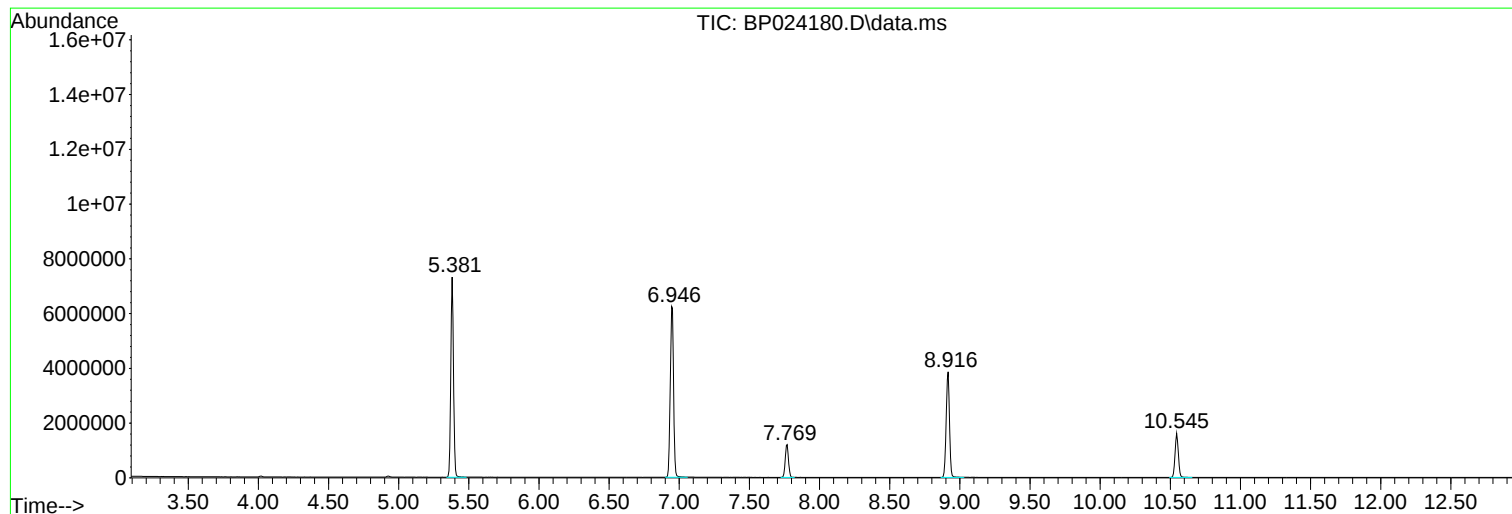

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031825\
Data File : BP024180.D
Acq On : 18 Mar 2025 10:26
Operator : RC/JU
Sample : PB167157BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB167157BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP031825\
Data File : BP024180.D
Acq On : 18 Mar 2025 10:26
Operator : RC/JU
Sample : PB167157BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB167157BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031225.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------