
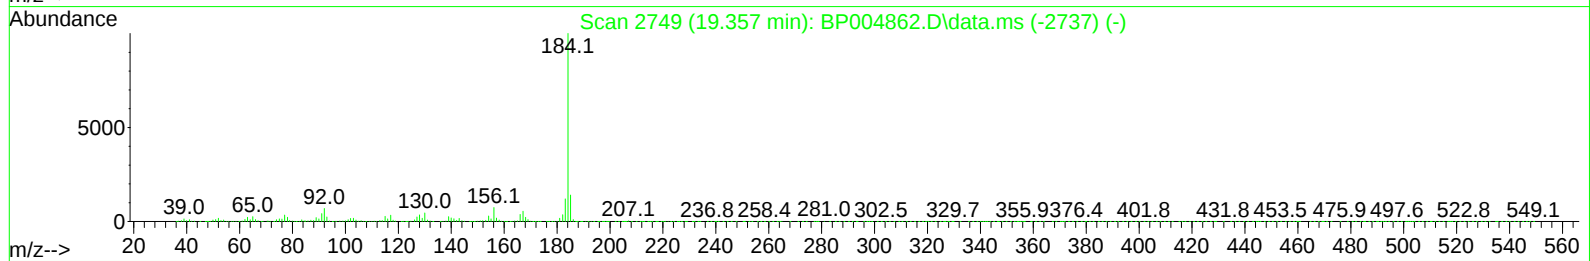
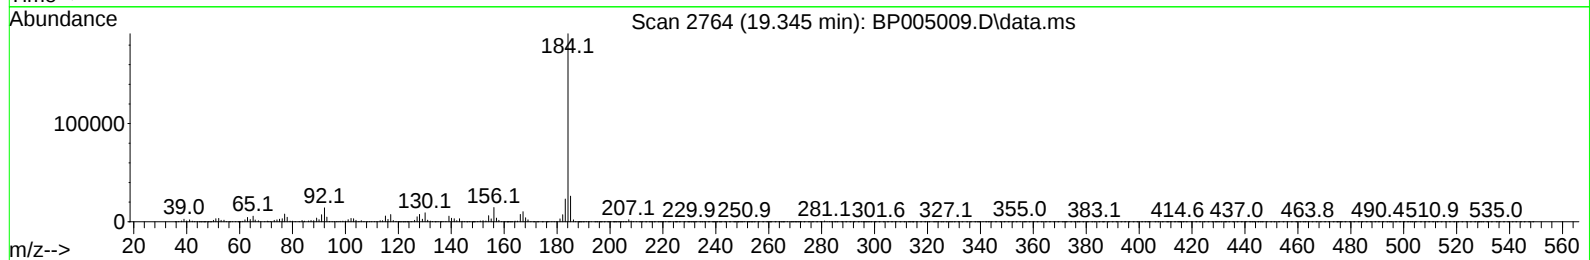


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032221\
Data File : BP005009.D
Acq On : 22 Mar 2021 09:58
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 22 10:48:57 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP032221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 26 17:41:20 2021
Response via : Initial Calibration

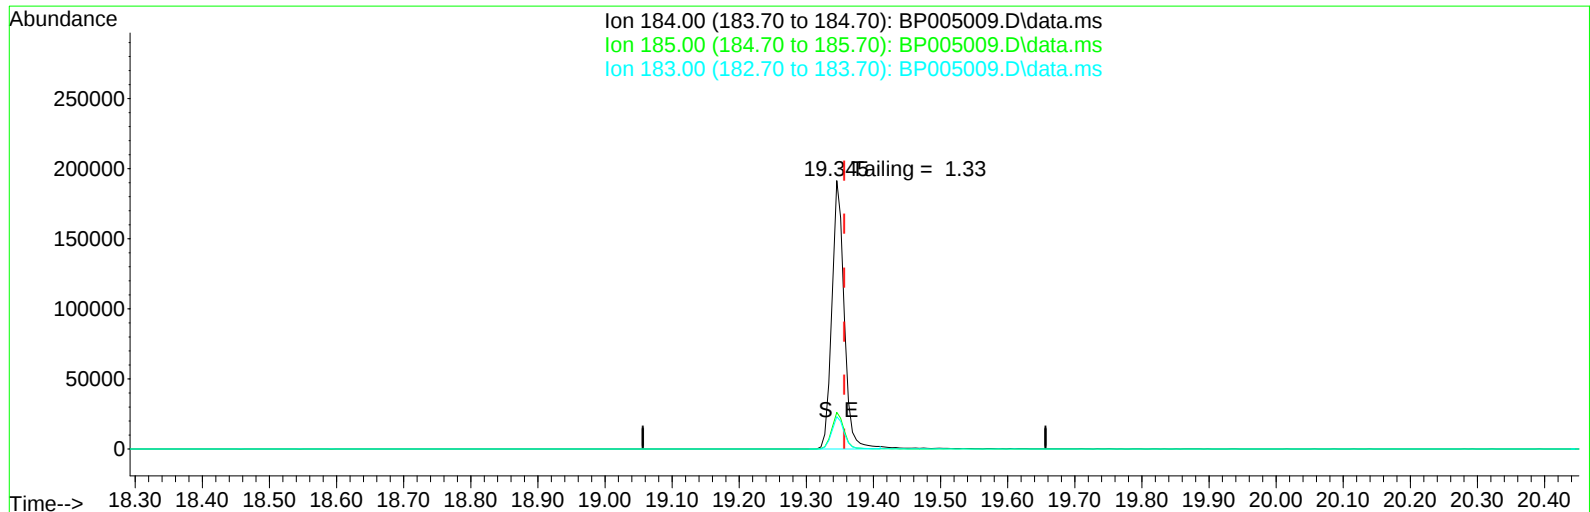

TIC: BP005009.D\data.ms

(77) Benzidine




19.345min (-0.011) 922.70 ng

response 246469

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	13.66
183.00	12.00	12.05
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032221\
Data File : BP005009.D
Acq On : 22 Mar 2021 09:58
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 22 10:48:57 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP032221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Feb 26 17:41:20 2021
Response via : Initial Calibration

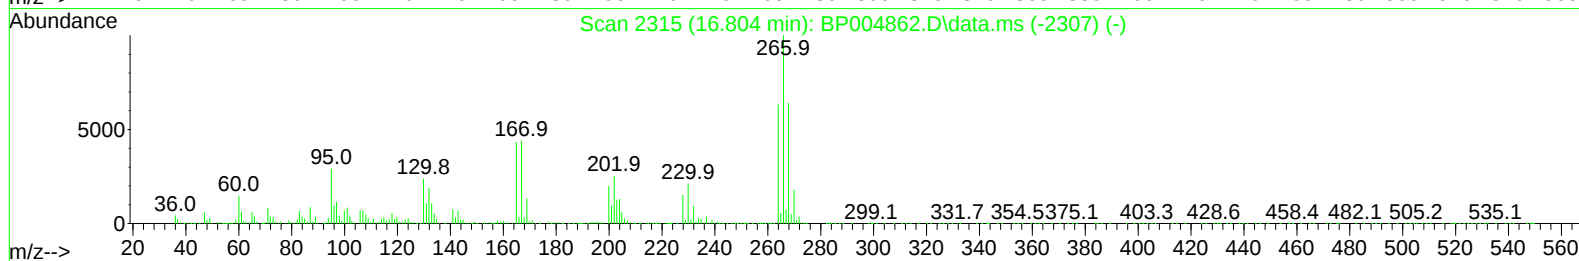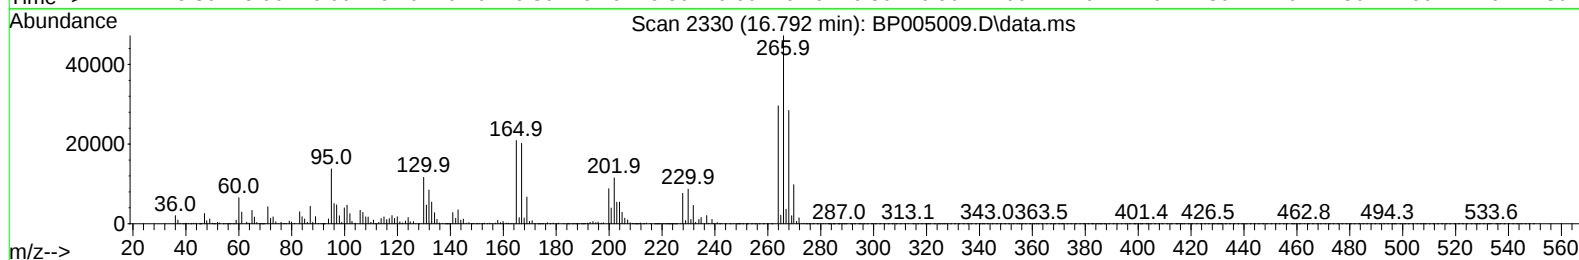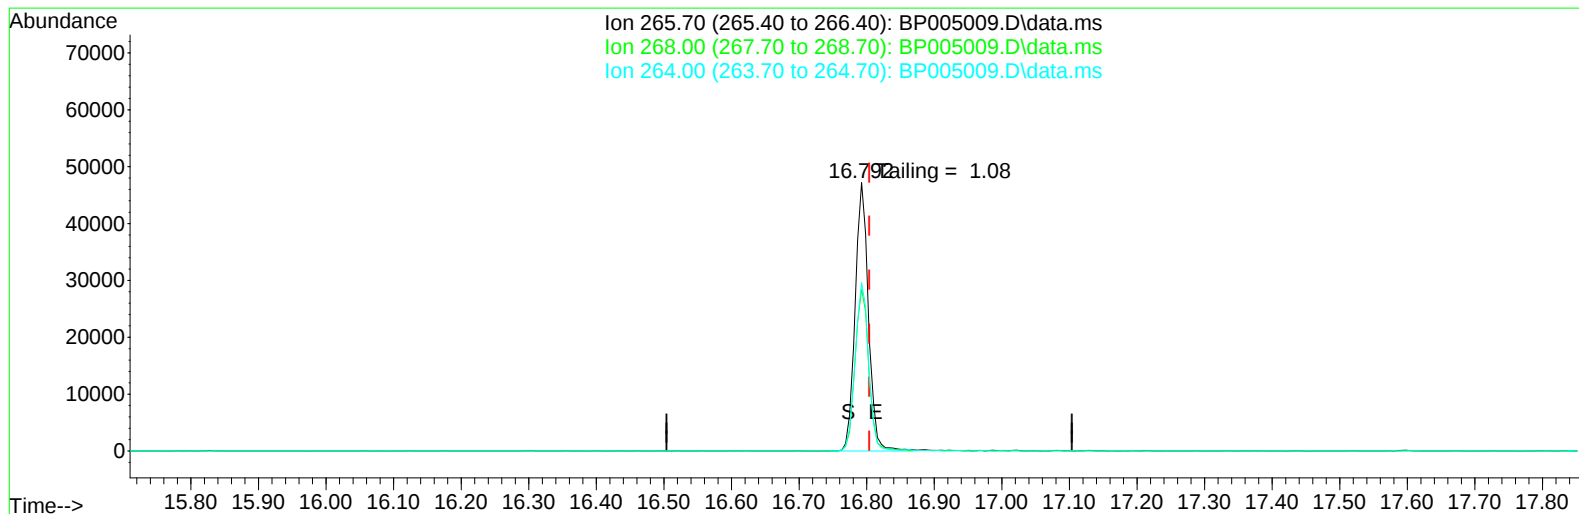

TIC: BP005009.D\data.ms

(70) Pentachlorophenol (C)

16.792min (-0.011) 123211.33 ng m

response 64322

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.90	60.25
264.00	63.30	62.73
0.00	0.00	0.00