

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032221\
 Data File : BP005019.D
 Acq On : 22 Mar 2021 17:40
 Operator : CG/JU
 Sample : PB135220BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB135220BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP032221.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP005019.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.316	372	379	390	rBV	760180	1042845	52.19%	10.988%
2	6.899	641	648	658	rBV	675238	1022323	51.17%	10.771%
3	7.722	781	788	803	rBV	148472	231469	11.58%	2.439%
4	8.881	975	985	998	rBV	410949	668066	33.44%	7.039%
5	10.510	1255	1262	1275	rBV	175352	301164	15.07%	3.173%
6	12.993	1677	1684	1694	rBV	1057142	1514506	75.80%	15.957%
7	14.375	1912	1919	1930	rBV	247427	364657	18.25%	3.842%
8	15.875	2167	2174	2189	rBV	716144	1052642	52.68%	11.091%
9	17.133	2382	2388	2400	rBV	287625	408655	20.45%	4.306%
10	19.704	2820	2825	2835	rBV	1622014	1998064	100.00%	21.052%
11	21.227	3079	3084	3091	rBV	335436	424875	21.26%	4.477%
12	23.515	3466	3473	3487	rVB2	229184	461916	23.12%	4.867%




Sum of corrected areas: 9491182

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032221\
Data File : BP005019.D
Acq On : 22 Mar 2021 17:40
Operator : CG/JU
Sample : PB135220BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB135220BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP032221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

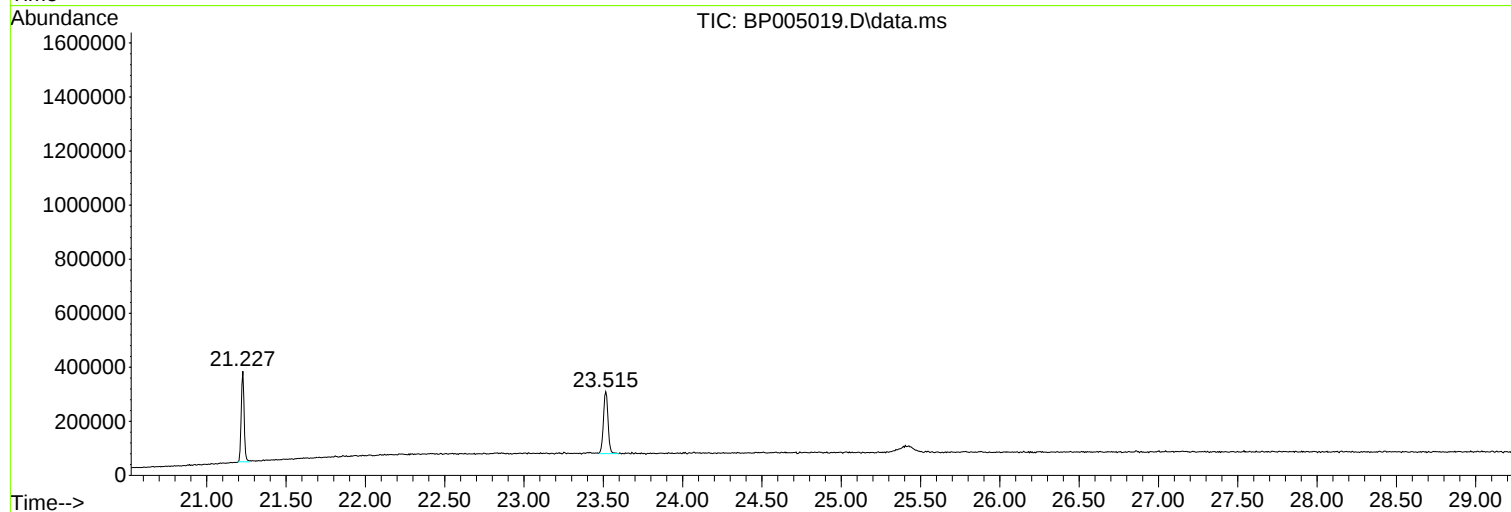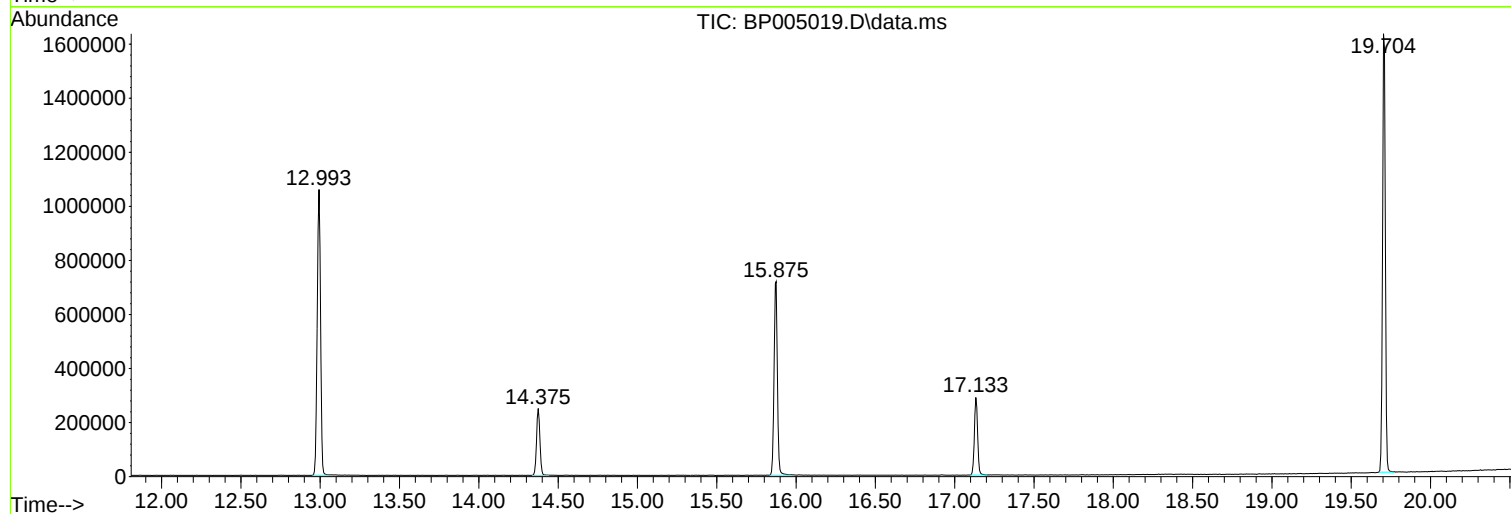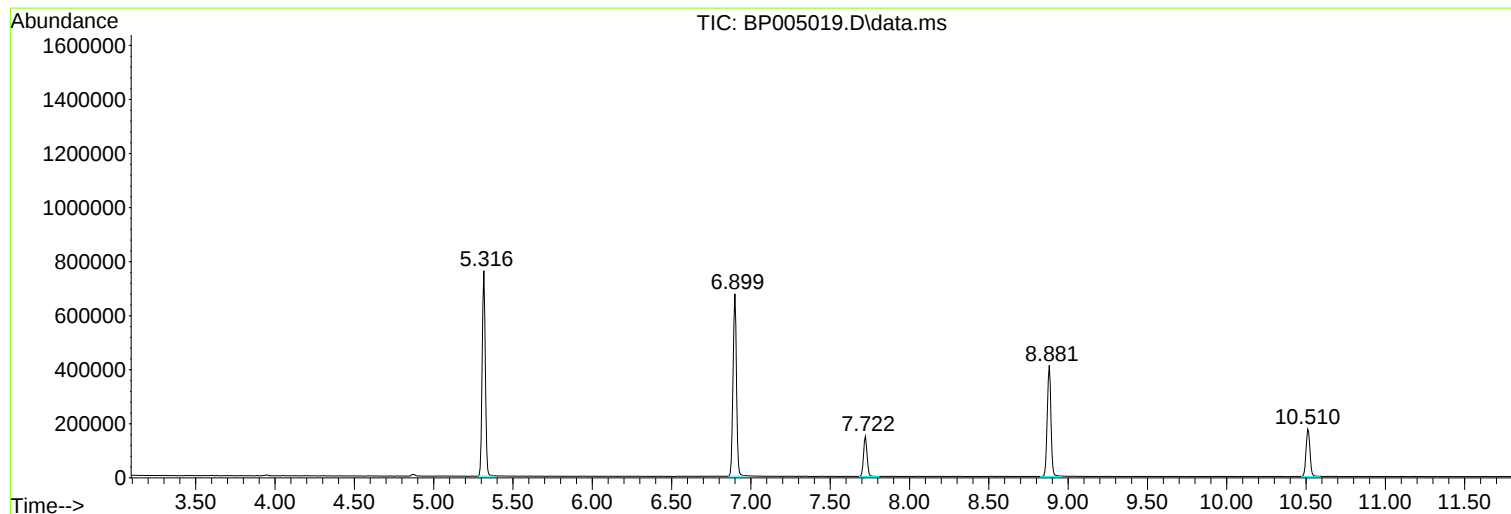

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032221\
Data File : BP005019.D
Acq On : 22 Mar 2021 17:40
Operator : CG/JU
Sample : PB135220BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB135220BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP032221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032221\
Data File : BP005019.D
Acq On : 22 Mar 2021 17:40
Operator : CG/JU
Sample : PB135220BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB135220BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP032221.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------