
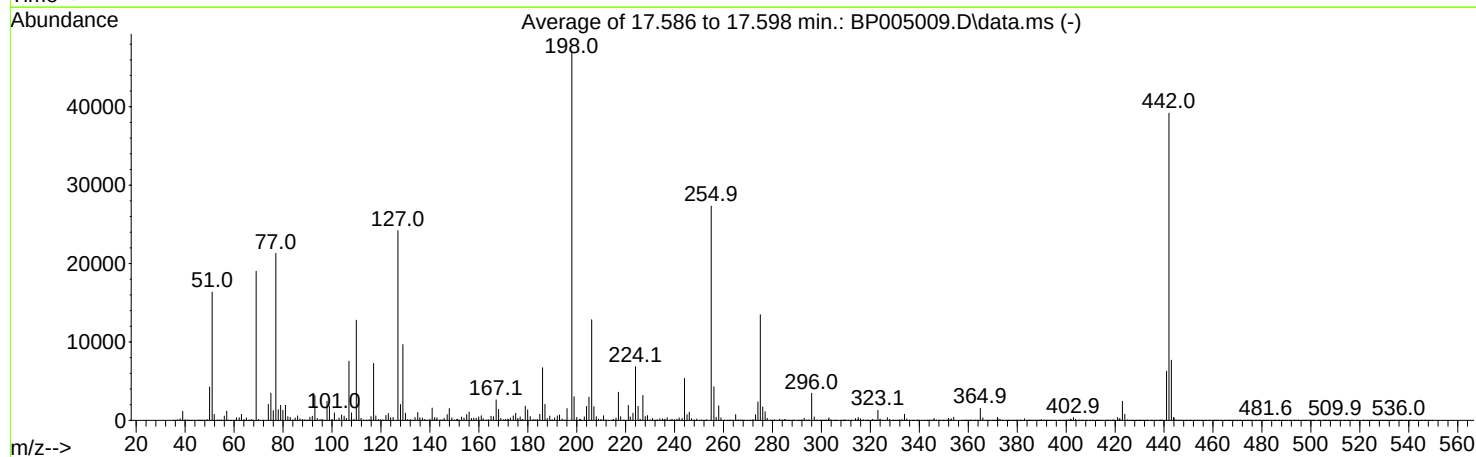


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032221\
 Data File : BP005009.D
 Acq On : 22 Mar 2021 09:58
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP032221.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Mar 22 17:08:54 2021

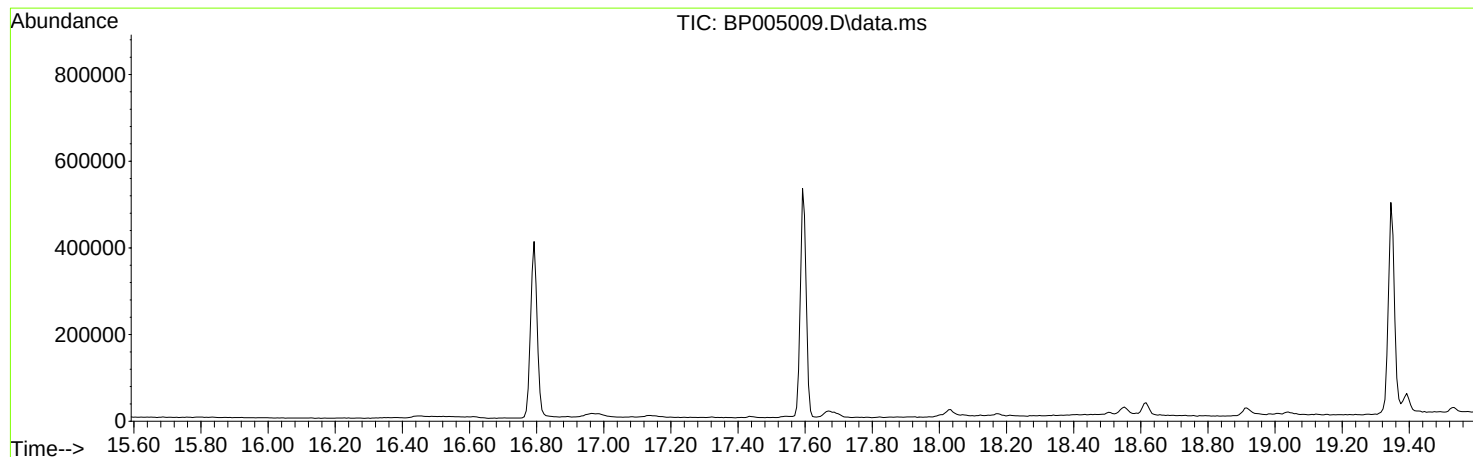

AutoFind: Scans 2465, 2466, 2467; Background Corrected with Scan 2456

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.9	16376	PASS
68	69	0.00	2	0.0	0	PASS
69	198	0.00	100	40.6	19033	PASS
70	69	0.00	2	0.6	115	PASS
127	198	10	80	51.6	24220	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	46930	PASS
199	198	5	9	6.4	3014	PASS
275	198	10	60	28.7	13483	PASS
365	198	1	100	3.3	1534	PASS
441	198	0.01	100	13.4	6275	PASS
442	442	100	100	100.0	39199	PASS
443	442	15	24	19.6	7675	PASS

DDT Breakdown




Date	Instrument Name	DFTPP Data File
3/22/2021	BNA_P	<u>BP005009.D</u>
Compound Name	Response	Retention Time
DDT	178728	20.54
DDD	2285	20.12
DDE	1039	19.62
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
3324	182052	1.83

Instrument :
BNA_P
ClientSampleId :
DFTPP

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032221\
 Data File : BP005009.D
 Acq On : 22 Mar 2021 09:58
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Mar 22 10:48:57 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP032221.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Feb 26 17:41:20 2021
 Response via : Initial Calibration

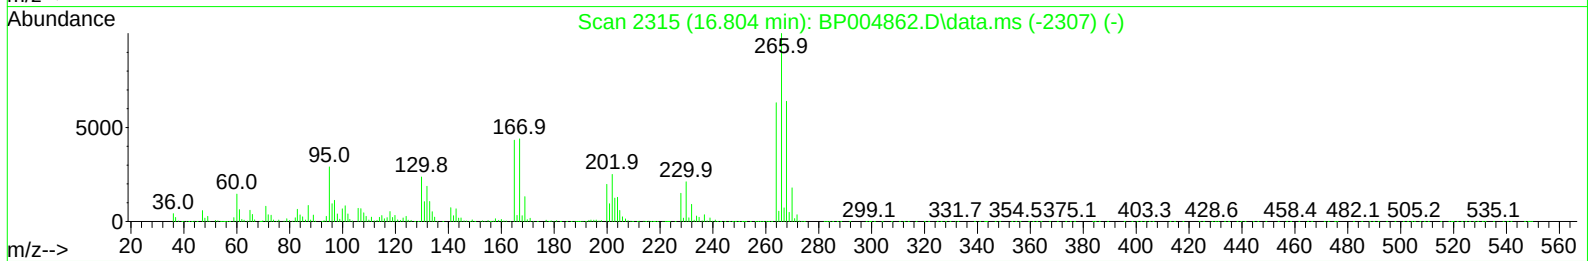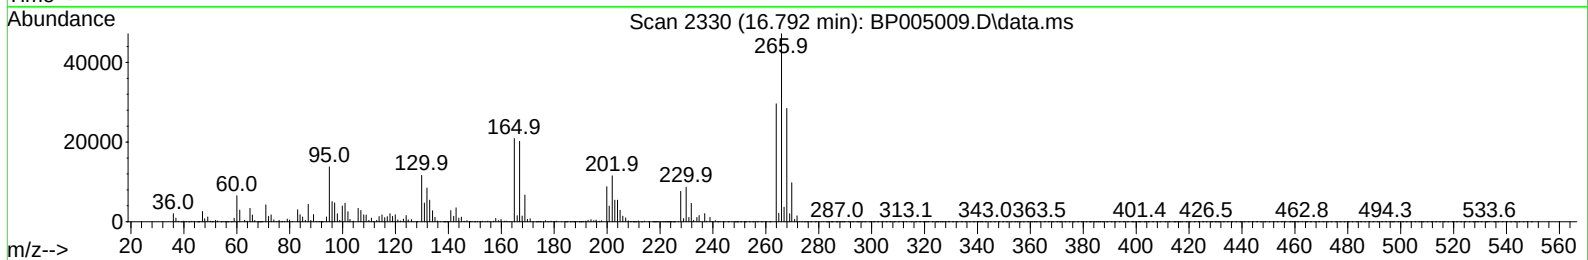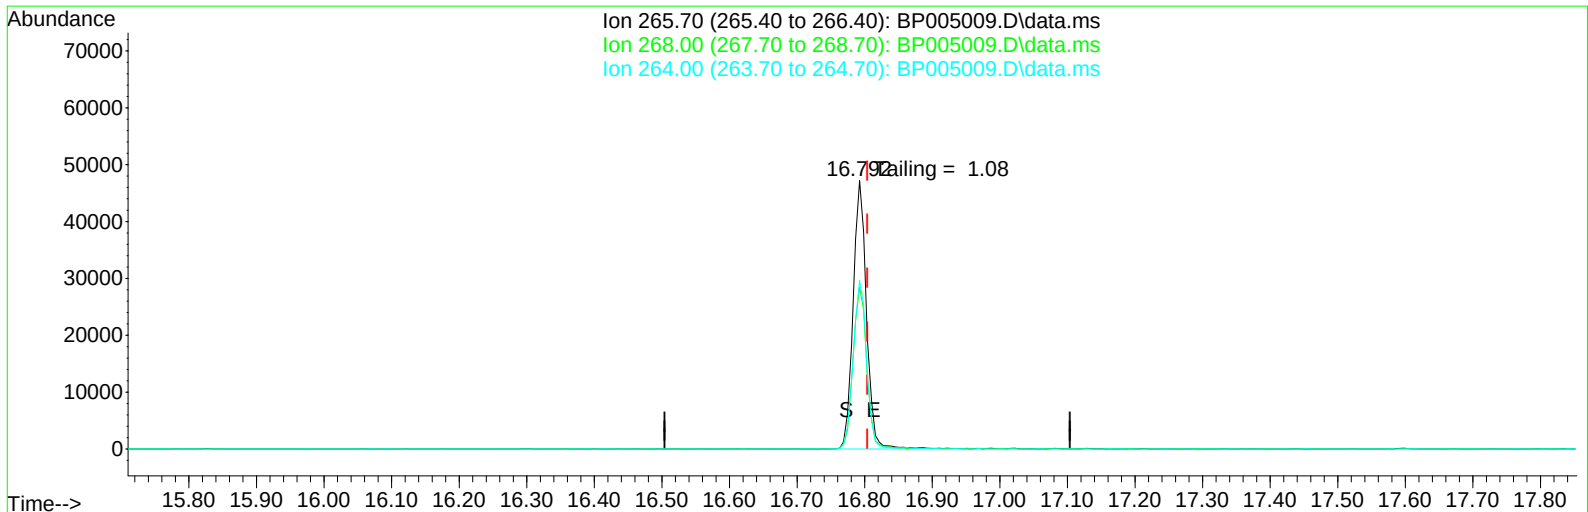

TIC: BP005009.D\data.ms

(70) Pentachlorophenol (C)

16.792min (-0.011) 123211.33 ng m




response 64322

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.90	60.25
264.00	63.30	62.73
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032221\
 Data File : BP005009.D
 Acq On : 22 Mar 2021 09:58
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Mar 22 10:48:57 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP032221.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Feb 26 17:41:20 2021
 Response via : Initial Calibration

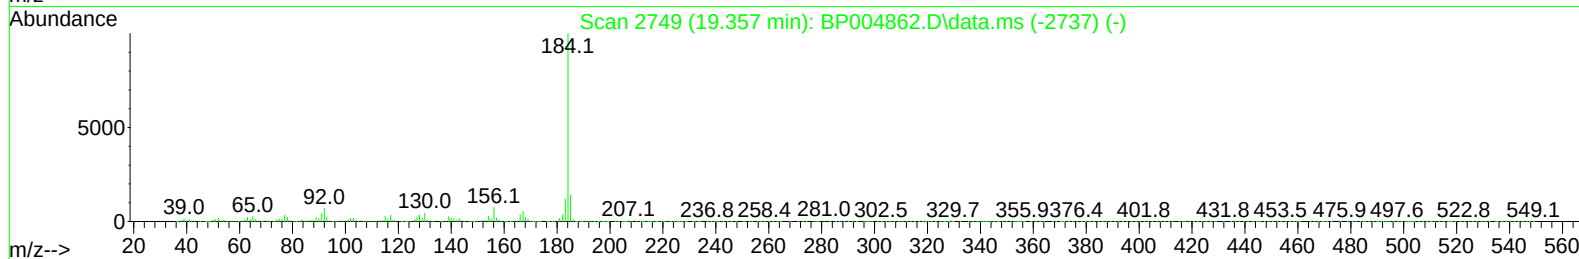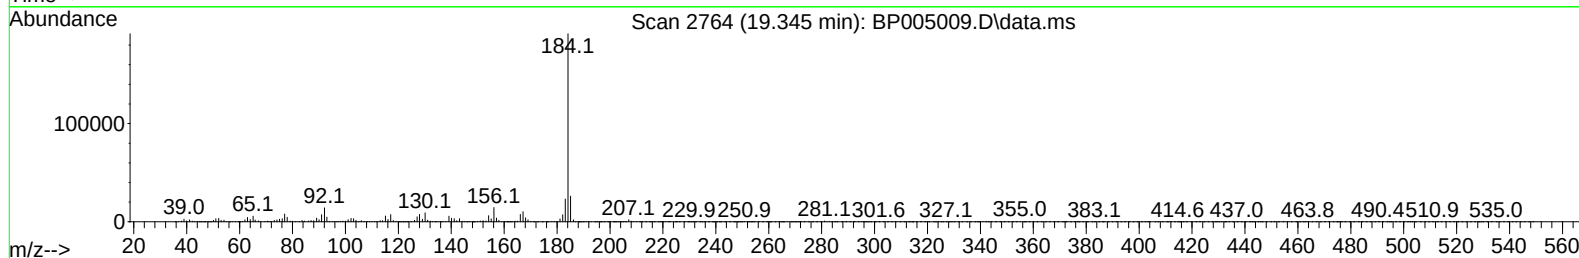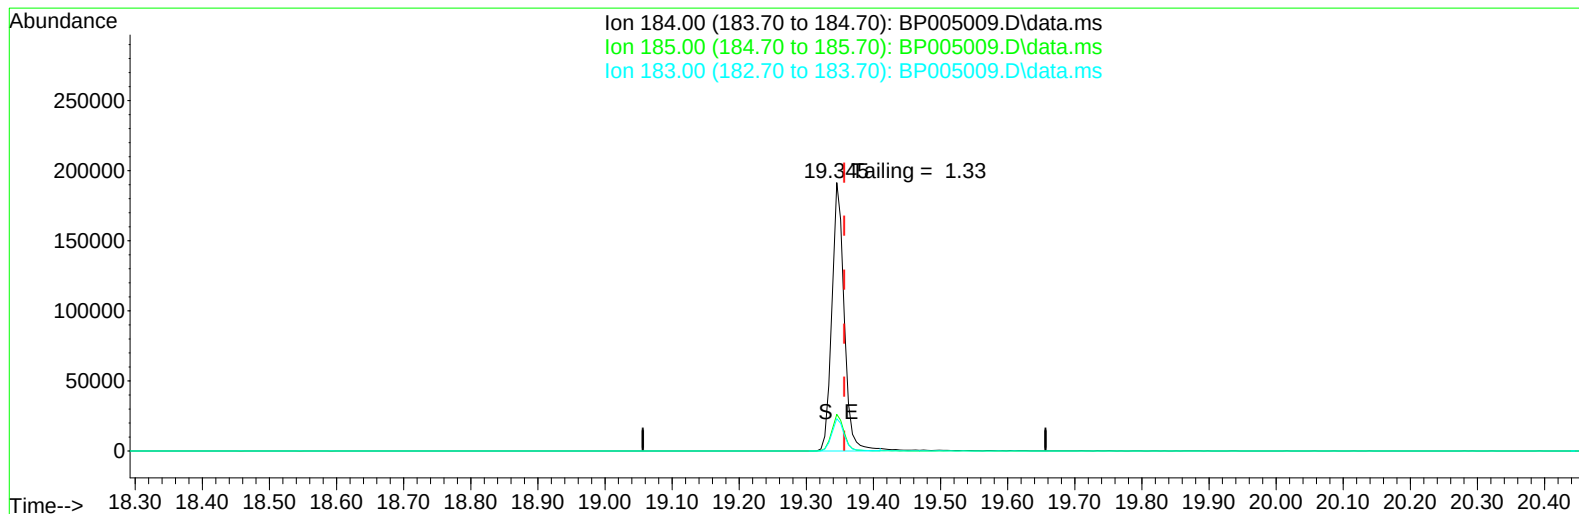

TIC: BP005009.D\data.ms

(77) Benzidine

19.345min (-0.011) 922.70 ng

response 246469

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	13.66
183.00	12.00	12.05
0.00	0.00	0.00