
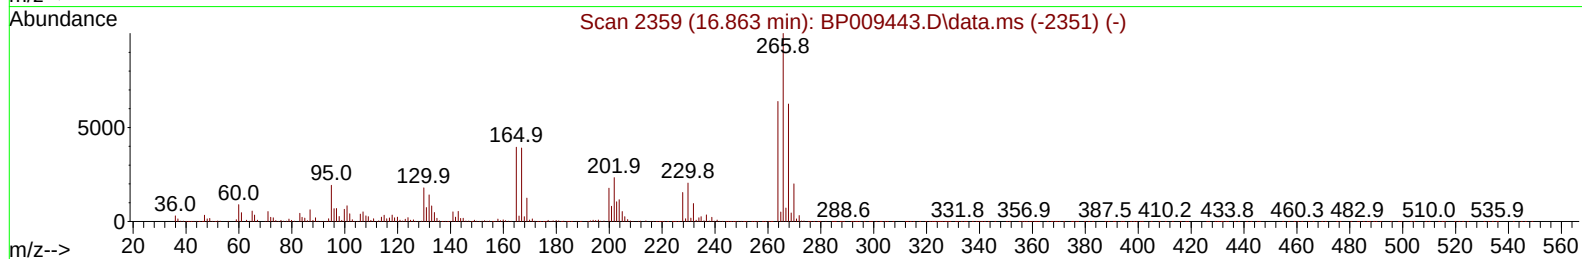
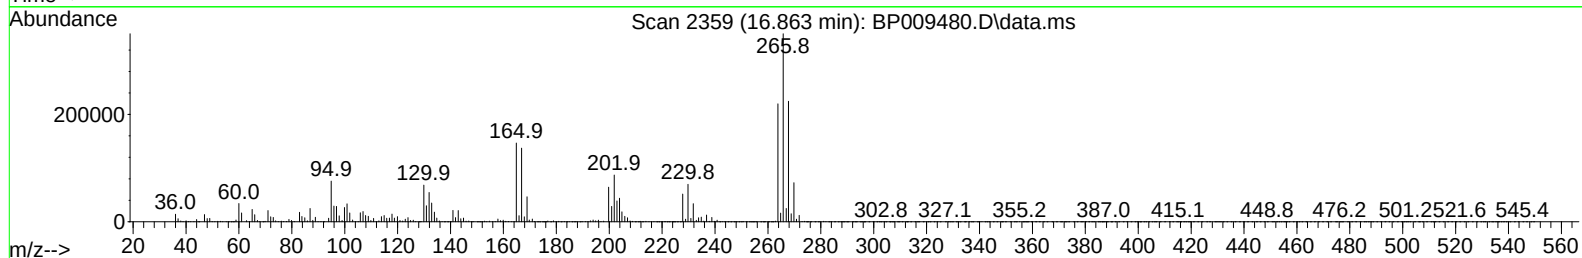


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032222\
Data File : BP009480.D
Acq On : 22 Mar 2022 09:55
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 23 02:18:36 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 17 18:26:53 2022
Response via : Initial Calibration

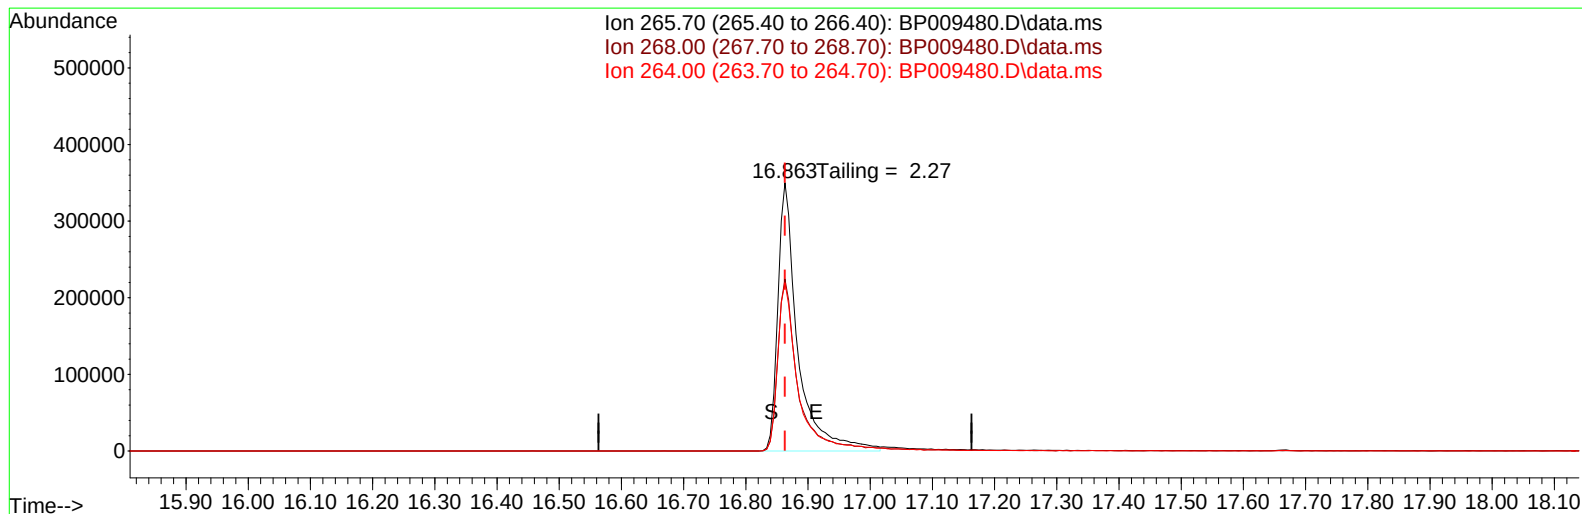

TIC: BP009480.D\data.ms

(70) Pentachlorophenol (C)




16.863min (-0.000) 177968.65 ng

response 802533

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.30	64.06
264.00	63.60	62.74
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032222\
Data File : BP009480.D
Acq On : 22 Mar 2022 09:55
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 23 02:21:40 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 17 18:26:53 2022
Response via : Initial Calibration

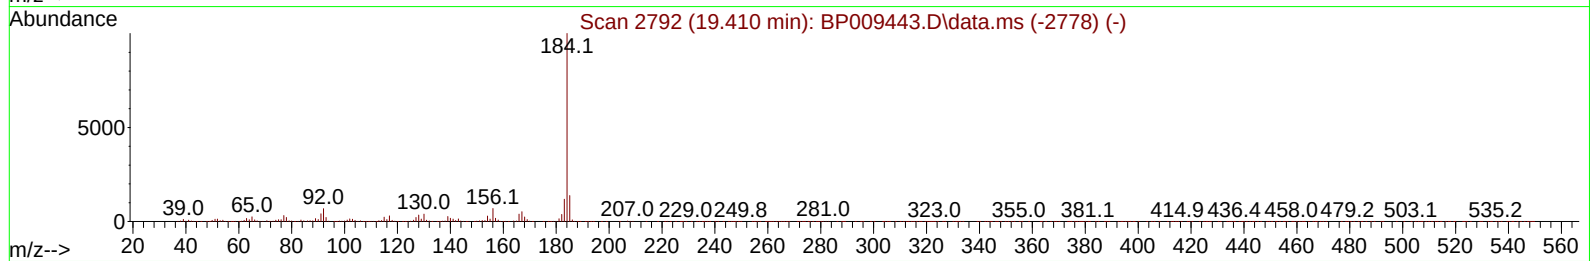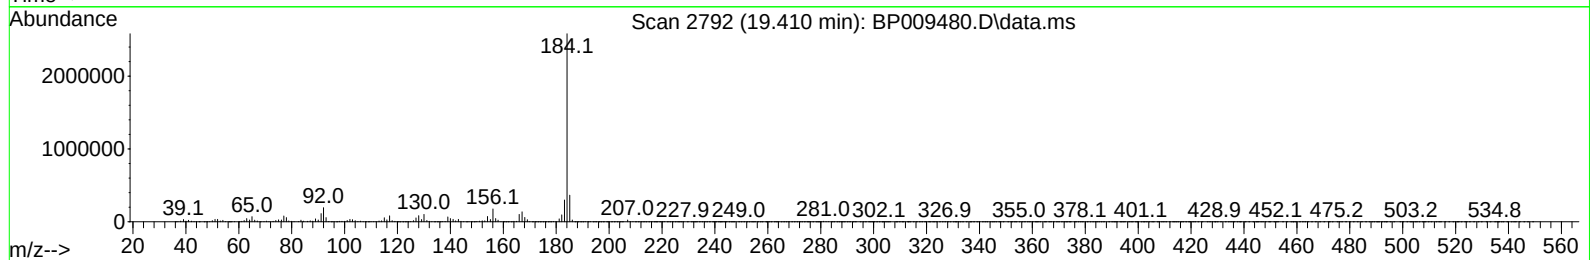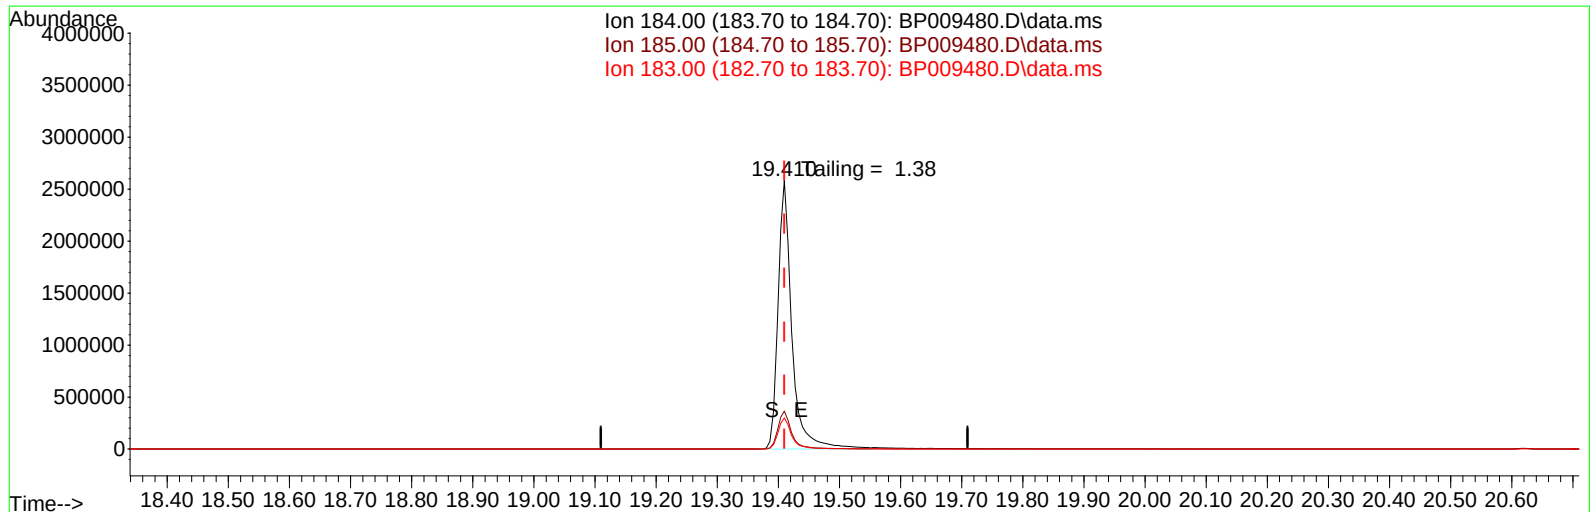

TIC: BP009480.D\data.ms

(77) Benzidine

19.410min (-0.000) 137983.52 ng

response 4126233

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.16
183.00	11.70	11.60
0.00	0.00	0.00