

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032222\
Data File : BP009482.D
Acq On : 22 Mar 2022 11:09
Operator : CG/JU
Sample : PB143421BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB143421BL

Integration Parameters: rteint.p
Integrator: RTE
Smoothing : ON Filtering: 5
Sampling : 1 Min Area: 3 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031722.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP009482.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.399	403	410	437	rBV	6505143	11324187	56.48%	11.426%
2	6.987	672	680	719	rBV	5999785	11248375	56.11%	11.350%
3	7.793	809	817	828	rBV	1299681	2309886	11.52%	2.331%
4	8.951	1006	1014	1034	rBV	3861932	7191894	35.87%	7.257%
5	10.592	1284	1293	1321	rBV	1367113	3056391	15.24%	3.084%
6	13.057	1704	1712	1738	rBV	9636458	16487381	82.24%	16.636%
7	14.439	1939	1947	1972	rBV	2209556	3861799	19.26%	3.897%
8	15.933	2194	2201	2244	rBV	6082603	11177720	55.75%	11.278%
9	17.204	2409	2417	2448	rBV	2303957	4303464	21.47%	4.342%
10	19.780	2849	2855	2868	rBV	14679083	20048636	100.00%	20.229%
11	21.309	3110	3115	3128	rBV	2559289	4187753	20.89%	4.226%
12	23.715	3518	3524	3539	rVB2	1626686	3909018	19.50%	3.944%




Sum of corrected areas: 99106504

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032222\
Data File : BP009482.D
Acq On : 22 Mar 2022 11:09
Operator : CG/JU
Sample : PB143421BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB143421BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

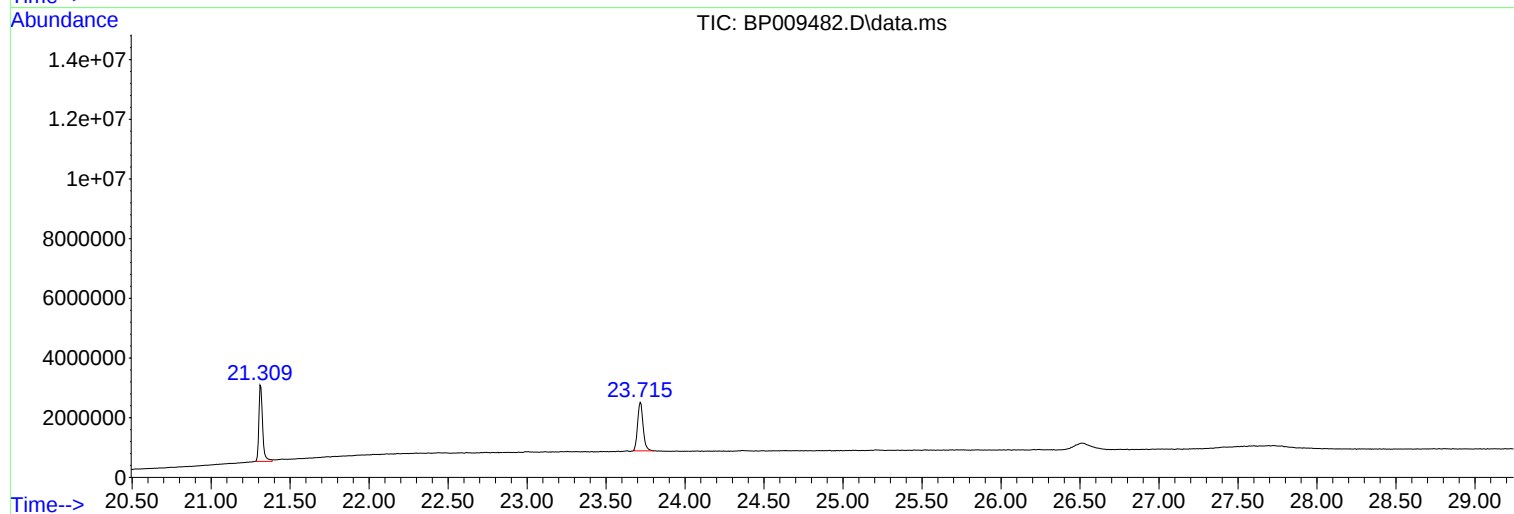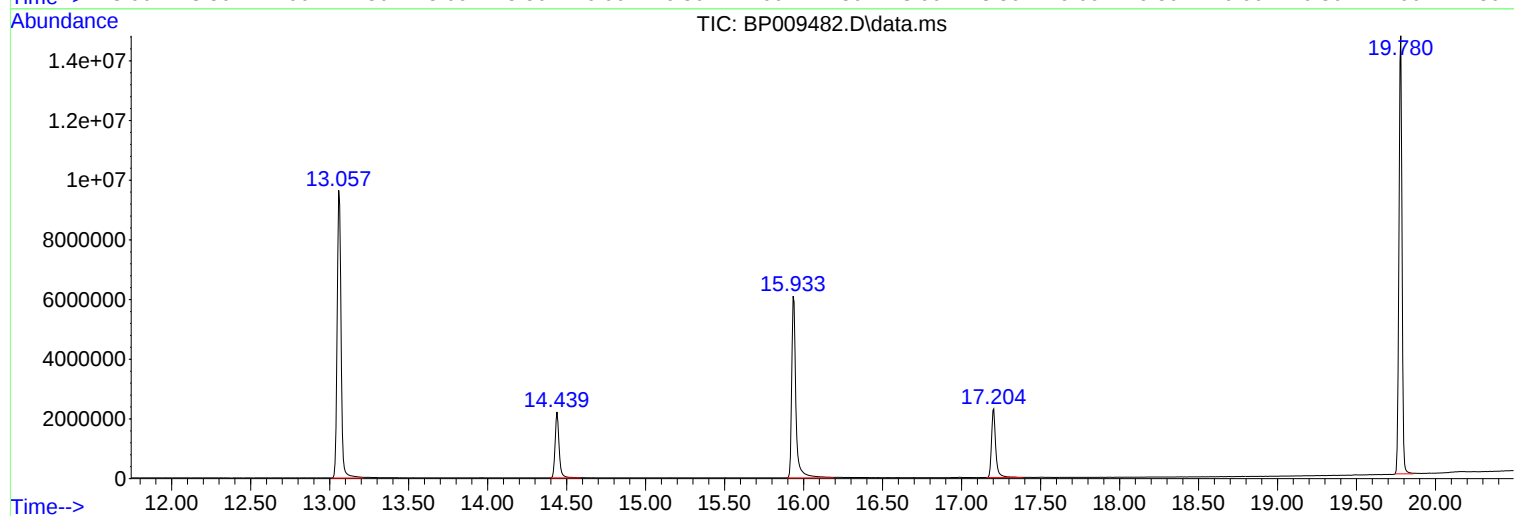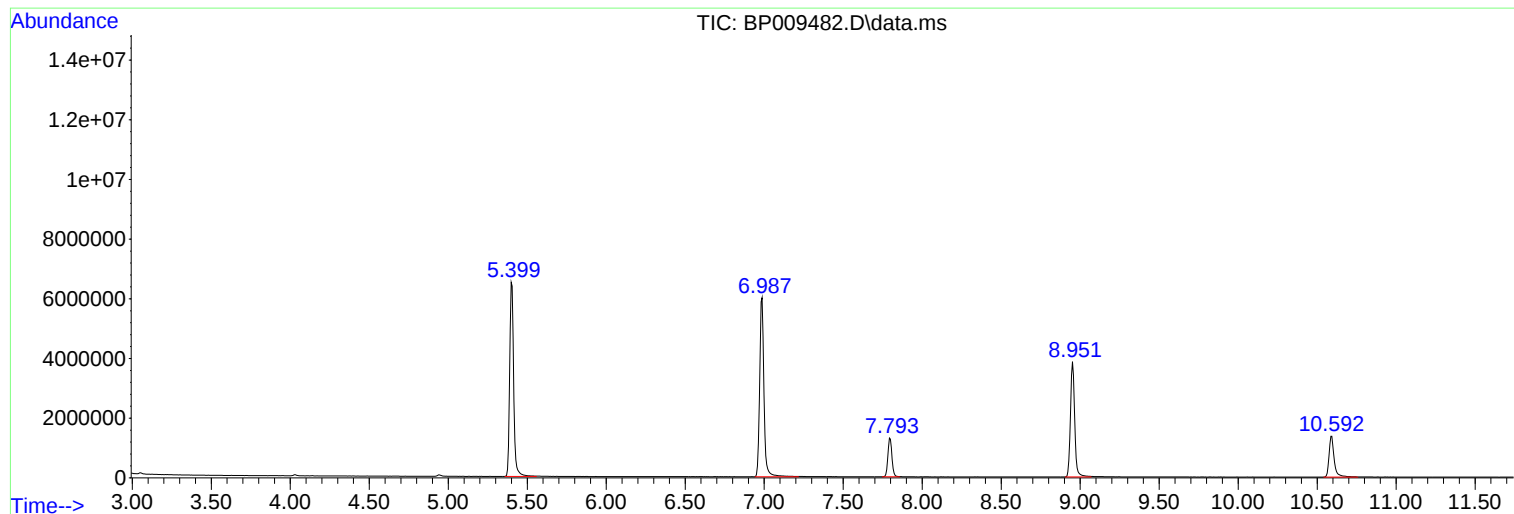

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032222\
Data File : BP009482.D
Acq On : 22 Mar 2022 11:09
Operator : CG/JU
Sample : PB143421BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB143421BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032222\
Data File : BP009482.D
Acq On : 22 Mar 2022 11:09
Operator : CG/JU
Sample : PB143421BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB143421BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------