
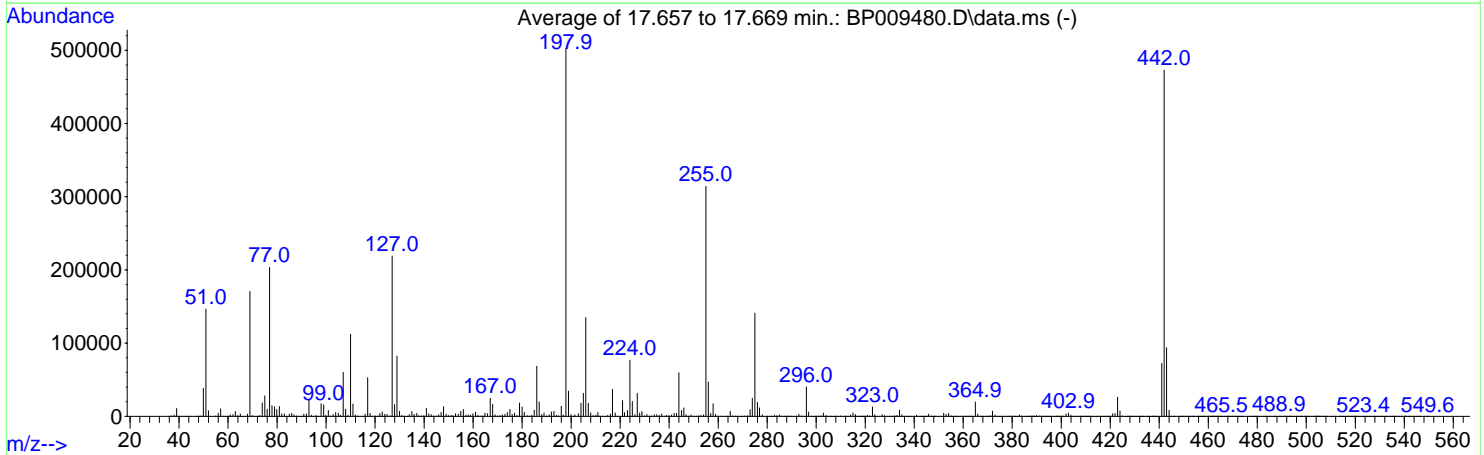


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032222\
 Data File : BP009480.D
 Acq On : 22 Mar 2022 09:55
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031722.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Mar 17 18:26:53 2022

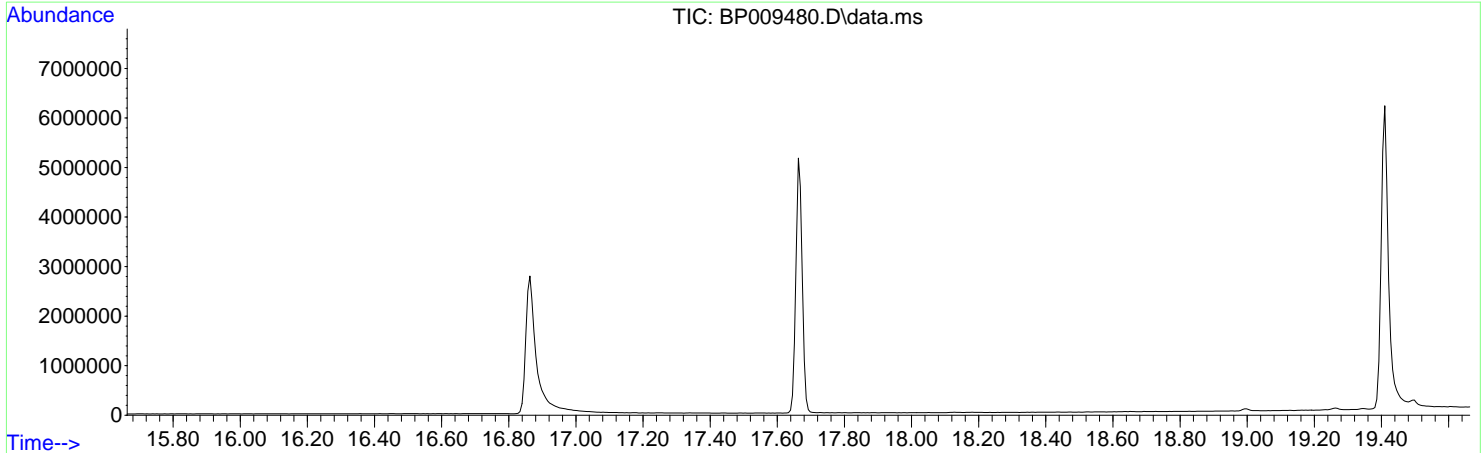




AutoFind: Scans 2494, 2495, 2496; Background Corrected with Scan 2485

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	29.2	146691	PASS
68	69	0.00	2	1.8	3049	PASS
69	198	0.00	100	34.0	170617	PASS
70	69	0.00	2	0.6	1035	PASS
127	198	10	80	43.6	219057	PASS
197	198	0.00	2	0.4	1793	PASS
198	198	100	100	100.0	502469	PASS
199	198	5	9	6.9	34554	PASS
275	198	10	60	28.1	140988	PASS
365	198	1	100	3.9	19607	PASS
441	198	0.01	100	14.4	72331	PASS
442	442	100	100	100.0	472868	PASS
443	442	15	24	19.8	93696	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032222\
 Data File : BP009480.D
 Acq On : 22 Mar 2022 09:55
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Mar 23 02:18:36 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031722.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 17 18:26:53 2022
 Response via : Initial Calibration

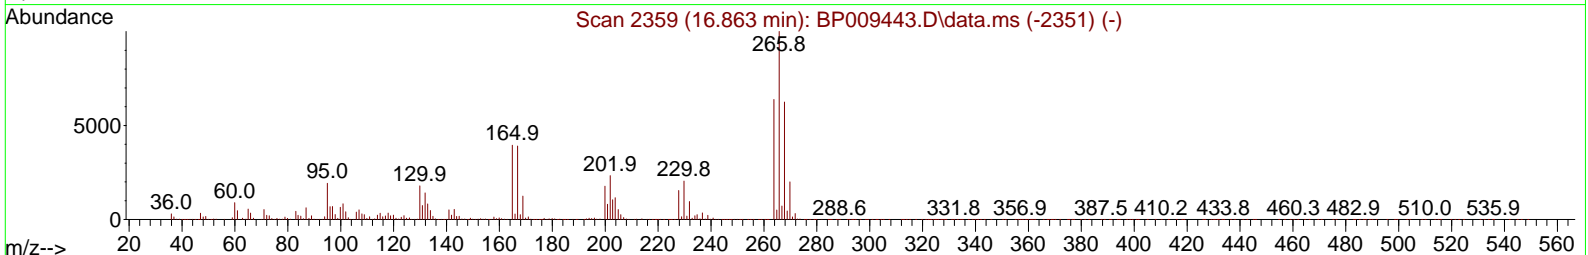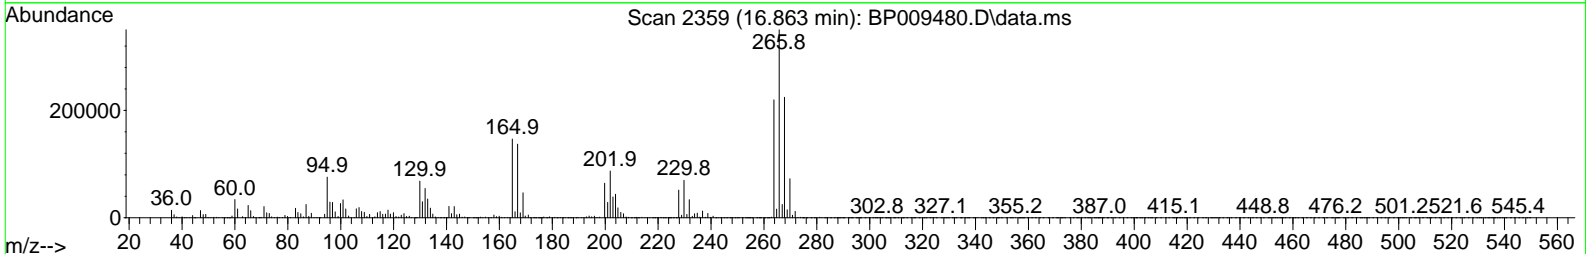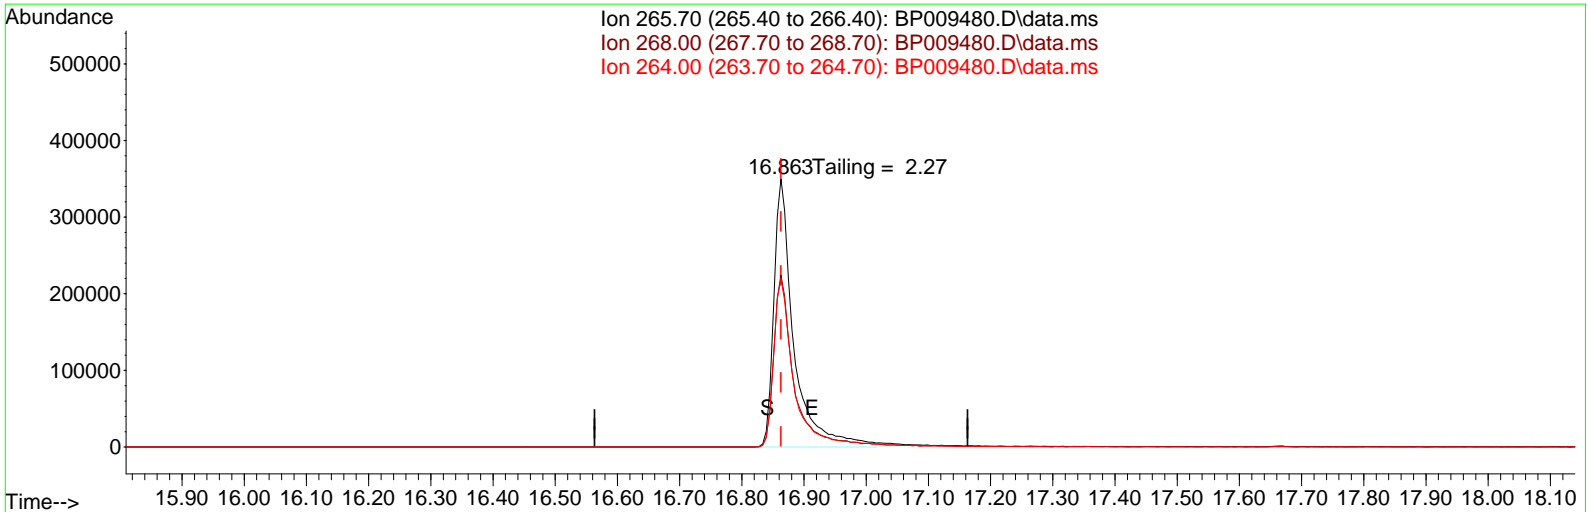

TIC: BP009480.D\data.ms

(70) Pentachlorophenol (C)

16.863min (-0.000) 177968.65 ng




response 802533

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.30	64.06
264.00	63.60	62.74
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032222\
 Data File : BP009480.D
 Acq On : 22 Mar 2022 09:55
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Mar 23 02:21:40 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031722.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 17 18:26:53 2022
 Response via : Initial Calibration

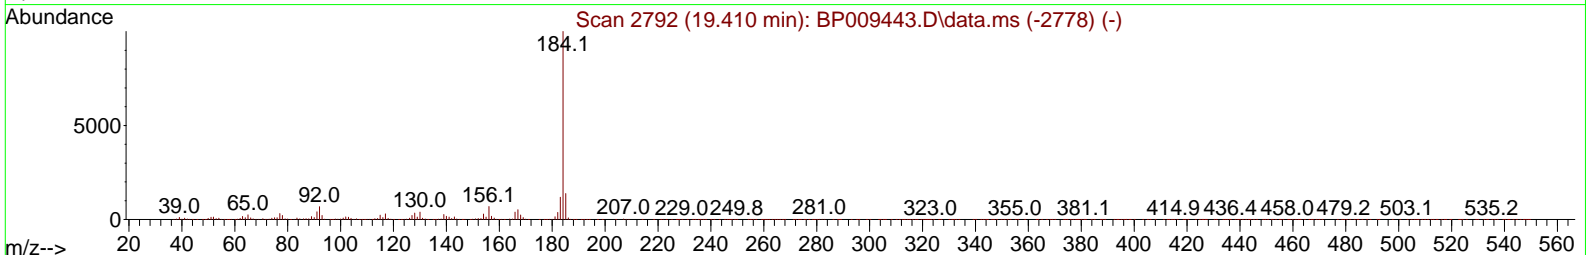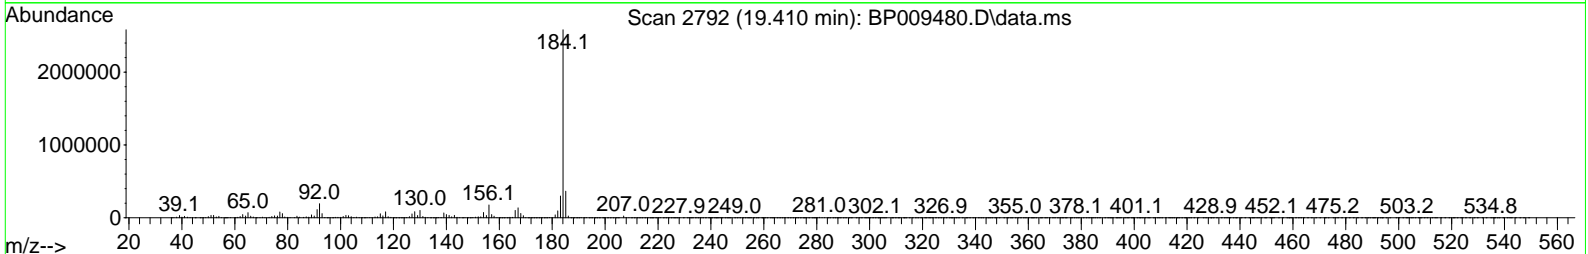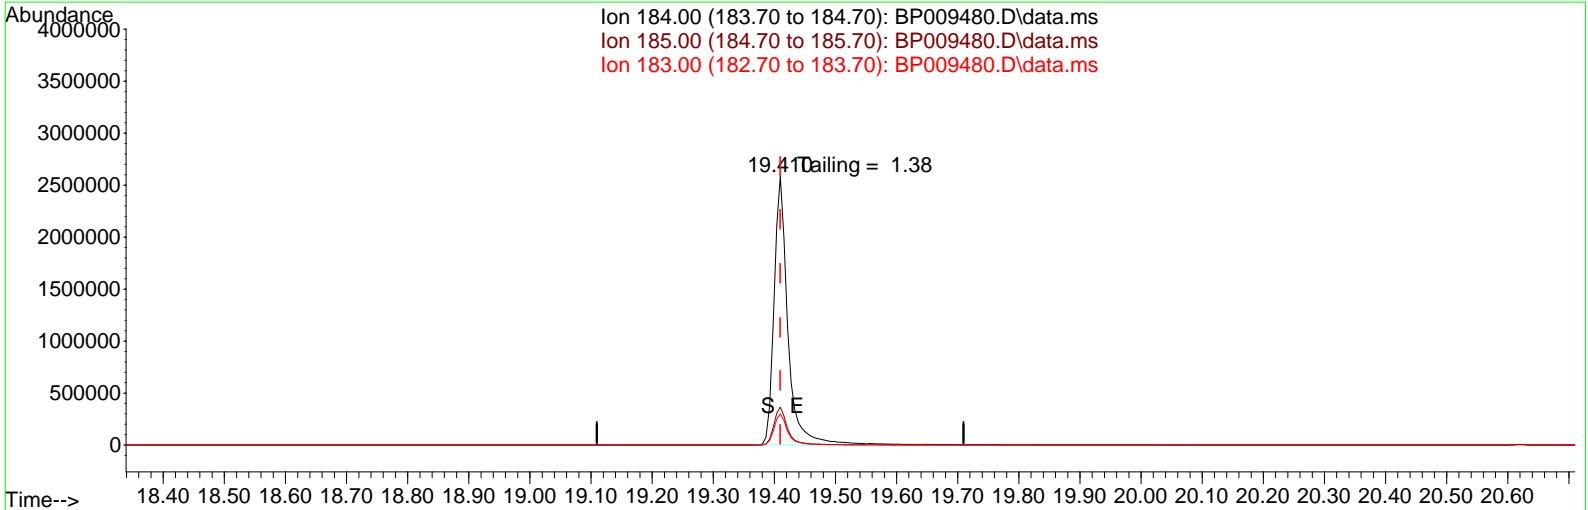

TIC: BP009480.D\data.ms

(77) Benzidine

19.410min (-0.000) 137983.52 ng

response 4126233

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.16
183.00	11.70	11.60
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/22/2022	BNA_P	<u>BP009480.D</u>
Compound Name	Response	Retention Time
DDT	1935403	20.621
DDD	21989	20.192
DDE	2650	19.692
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
24639	1960042	1.26

Instrument :
 BNA_P
 ClientSampled :
 DFTPP