




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032223\
 Data File : BP014248.D
 Acq On : 23 Mar 2023 09:34
 Operator : CG/JU
 Sample : 01977-18
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EYGA3

Manual IntegrationsAPPROVED

Quant Time: Mar 24 01:44:01 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Mar 23 04:56:06 2023
 Response via : Initial Calibration

Reviewed By :Christian Giraldo 03/24/2023
 Supervised By :Jagrut Upadhyay 03/24/2023

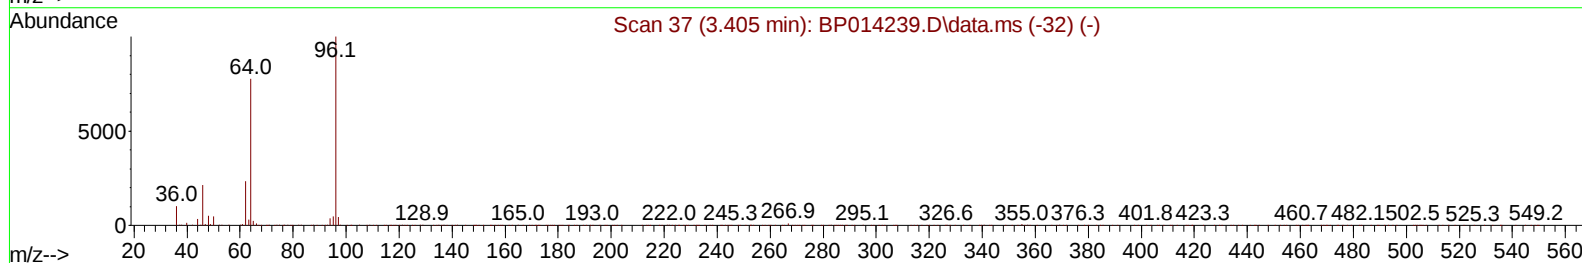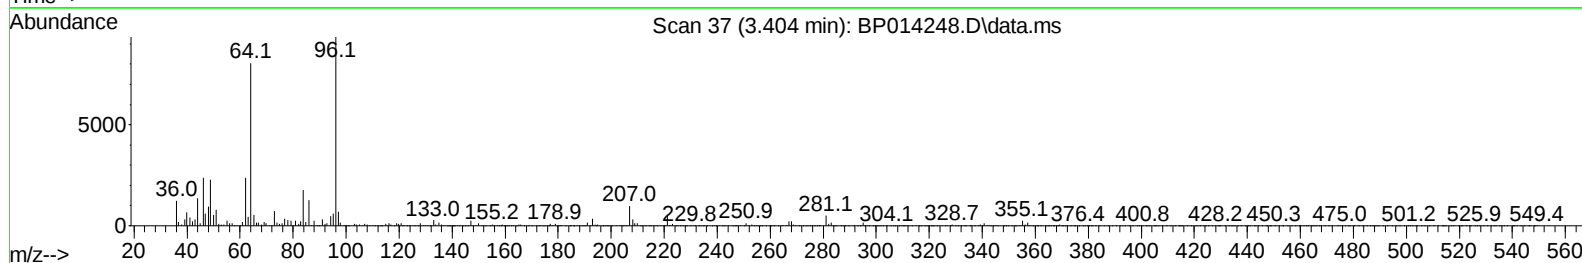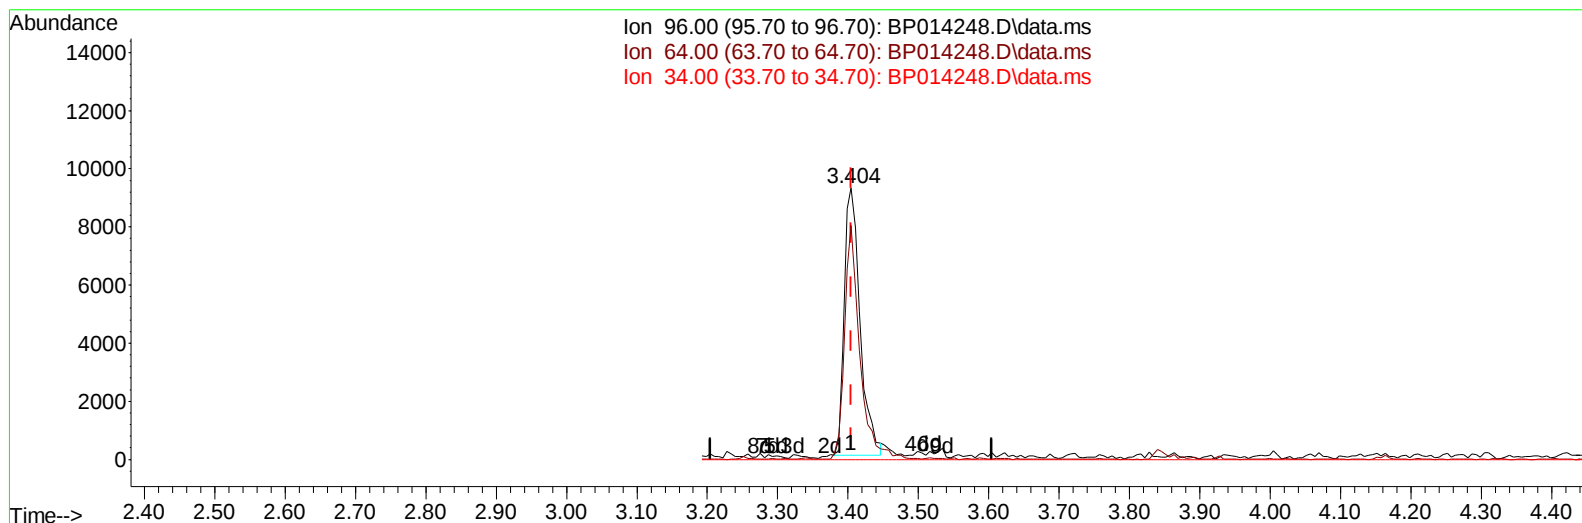

TIC: BP014248.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.404min (-0.000) 3.57 ng/uL

response 14247

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	66.60	86.12#
34.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032223\
 Data File : BP014248.D
 Acq On : 23 Mar 2023 09:34
 Operator : CG/JU
 Sample : 01977-18
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EYGA3

Manual IntegrationsAPPROVED

Quant Time: Mar 24 01:44:01 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Mar 23 04:56:06 2023
 Response via : Initial Calibration

Reviewed By :Christian Giraldo 03/24/2023
 Supervised By :Jagrut Upadhyay 03/24/2023

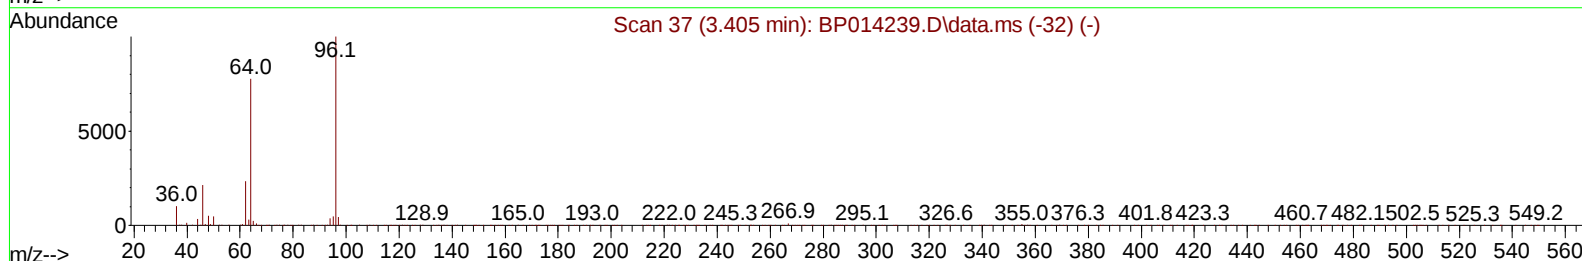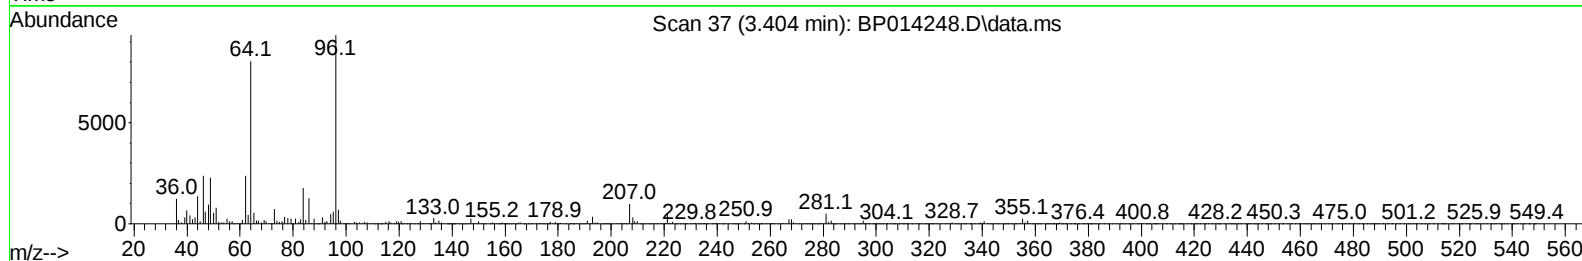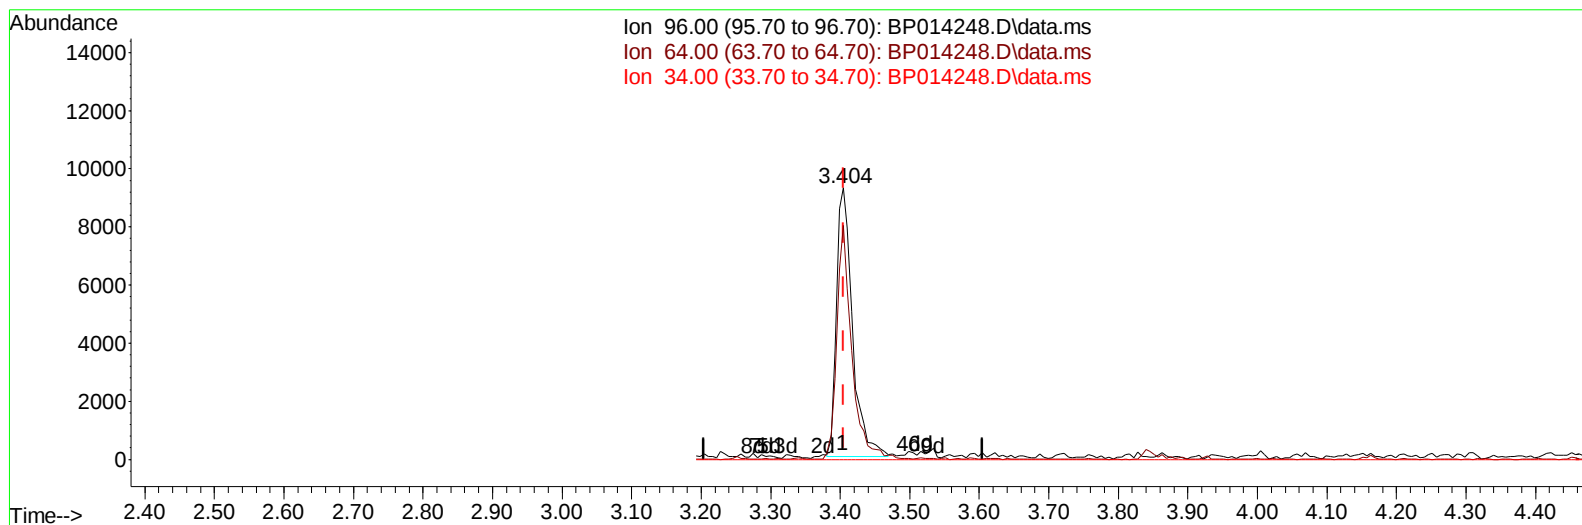

TIC: BP014248.D\data.ms

(3) 1,4-Dioxane-d8 (S)

3.404min (-0.000) 3.71 ng/uL m

response 14808

Ion	Exp%	Act%
96.00	100.00	100.00
64.00	66.60	86.12#
34.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032223\
 Data File : BP014248.D
 Acq On : 23 Mar 2023 09:34
 Operator : CG/JU
 Sample : 01977-18
 Misc :
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EYGA3

Manual IntegrationsAPPROVED

Quant Time: Mar 24 01:44:01 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Mar 23 04:56:06 2023
 Response via : Initial Calibration

Reviewed By :Christian Giraldo 03/24/2023
 Supervised By :Jagrut Upadhyay 03/24/2023

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.034	152	150699	20.000	ng/ul	0.00
20) Naphthalene-d8	10.857	136	685205	20.000	ng/ul	# 0.00
38) Acenaphthene-d10	14.680	164	497635	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.439	188	1184473	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.521	240	1192400	20.000	ng/ul	# 0.00
88) Perylene-d12	24.045	264	1226074	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.404	96	14808m	3.713	ng/uL	0.00
4) Pyridine-d5	3.840	84	194860	17.645	ng/ul	0.00
7) Phenol-d5	7.198	99	290354	21.833	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.357	67	187421	24.165	ng/ul	0.00
11) 2-Chlorophenol-d4	7.563	132	216026	21.321	ng/ul	0.00
15) 4-Methylphenol-d8	8.751	113	239280	22.027	ng/ul	0.00
21) Nitrobenzene-d5	9.210	128	116853	21.373	ng/ul	0.00
24) 2-Nitrophenol-d4	9.939	143	136674	20.884	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.481	165	239360	19.438	ng/ul	0.00
31) 4-Chloroaniline-d4	11.004	131	318777	19.561	ng/ul	0.00
46) Dimethylphthalate-d6	14.086	166	941430	22.291	ng/ul	0.00
49) Acenaphthylene-d8	14.374	160	996986	22.285	ng/ul	0.00
54) 4-Nitrophenol-d4	14.898	143	131973	17.732	ng/ul	0.00
60) Fluorene-d10	15.674	176	806712	22.539	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.798	200	147689	16.497	ng/ul	0.00
73) Anthracene-d10	17.539	188	1317640	22.915	ng/ul	0.00
81) Pyrene-d10	19.768	212	1602851	24.373	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.880	264	1518029	23.276	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032223\
Data File : BP014248.D
Acq On : 23 Mar 2023 09:34
Operator : CG/JU
Sample : 01977-18
Misc :
ALS Vial : 28 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EYGA3

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 03/24/2023
Supervised By :Jagrut Upadhyay 03/24/2023

Quant Time: Mar 24 01:44:01 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Mar 23 04:56:06 2023
Response via : Initial Calibration

