




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032223\
Data File : BP014251.D
Acq On : 23 Mar 2023 11:17
Operator : CG/JU
Sample : 01977-21
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EYGA6

Manual IntegrationsAPPROVED

Quant Time: Mar 24 01:51:05 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Mar 23 04:56:06 2023
Response via : Initial Calibration

Reviewed By :Christian Giraldo 03/24/2023
Supervised By :Jagrut Upadhyay 03/24/2023

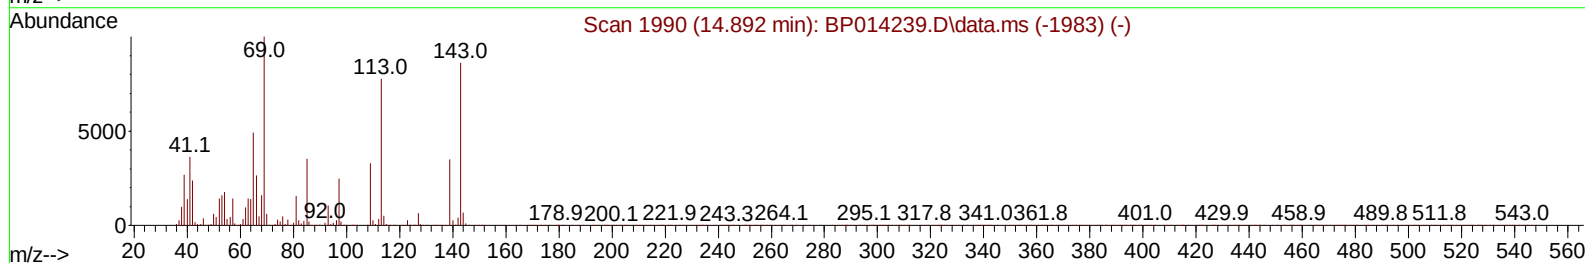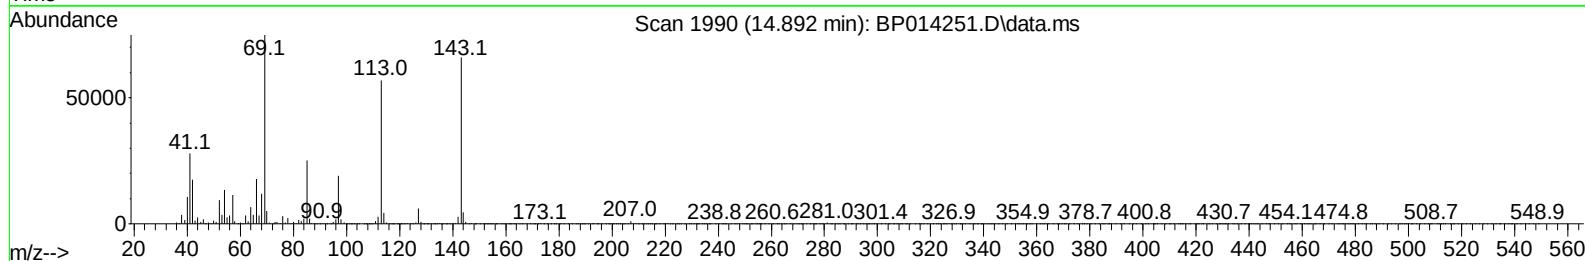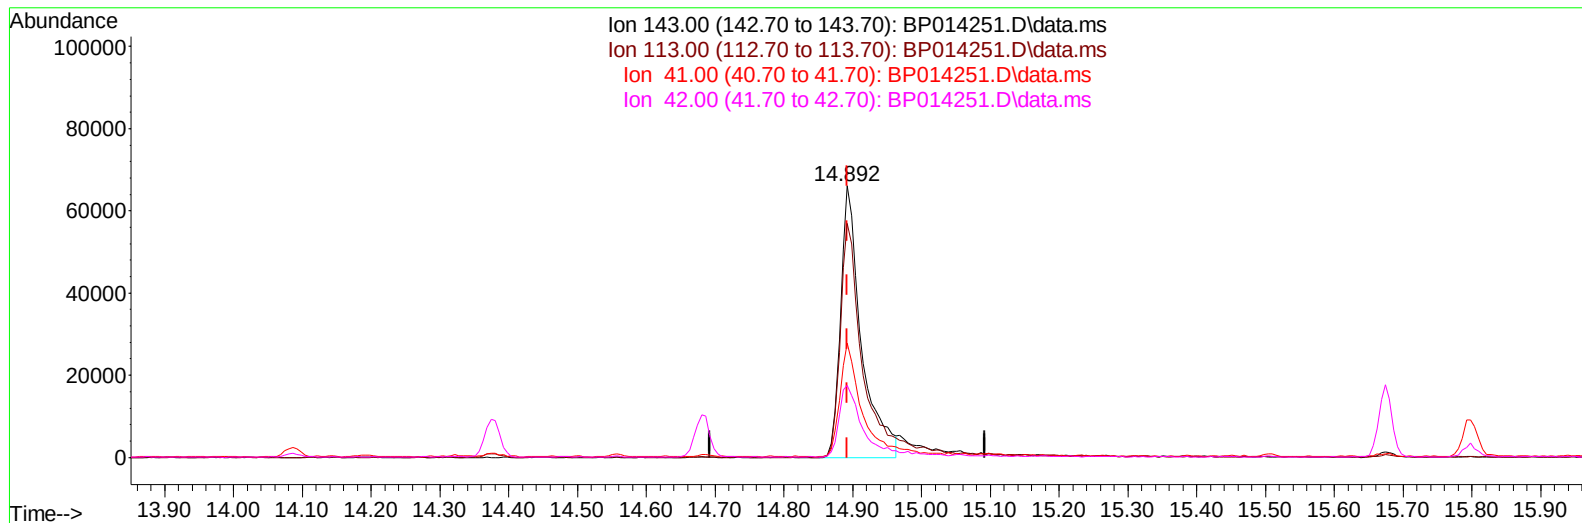

TIC: BP014251.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.892min (-0.000) 19.00 ng/ul

response 139343

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	103.10	86.13
41.00	40.20	42.20
42.00	28.50	26.60




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032223\
 Data File : BP014251.D
 Acq On : 23 Mar 2023 11:17
 Operator : CG/JU
 Sample : 01977-21
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EYGA6

Manual IntegrationsAPPROVED

Quant Time: Mar 24 01:51:05 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Mar 23 04:56:06 2023
 Response via : Initial Calibration

Reviewed By :Christian Giraldo 03/24/2023
 Supervised By :Jagrut Upadhyay 03/24/2023

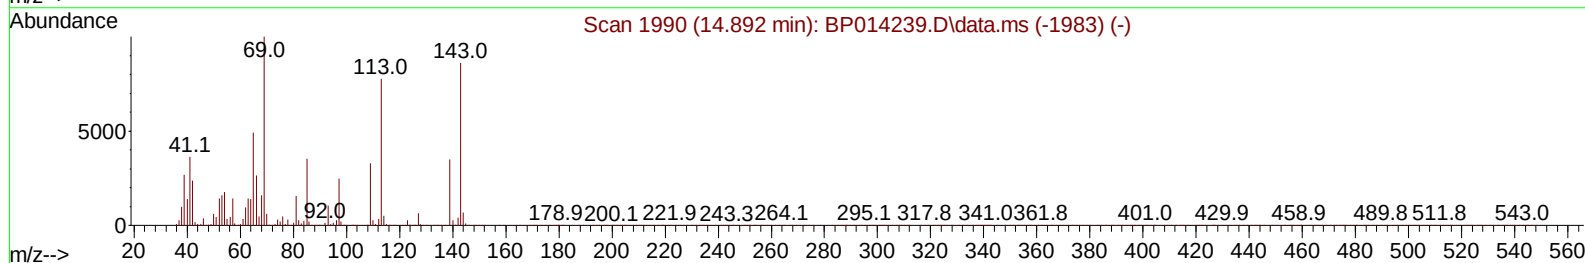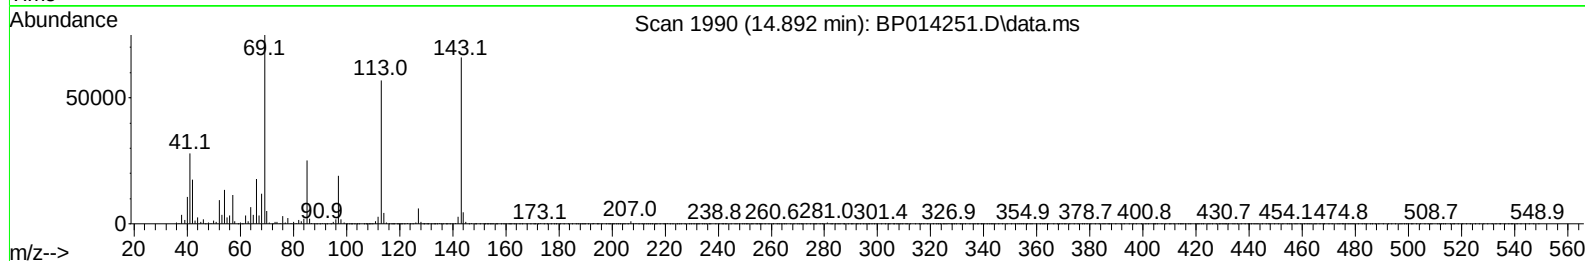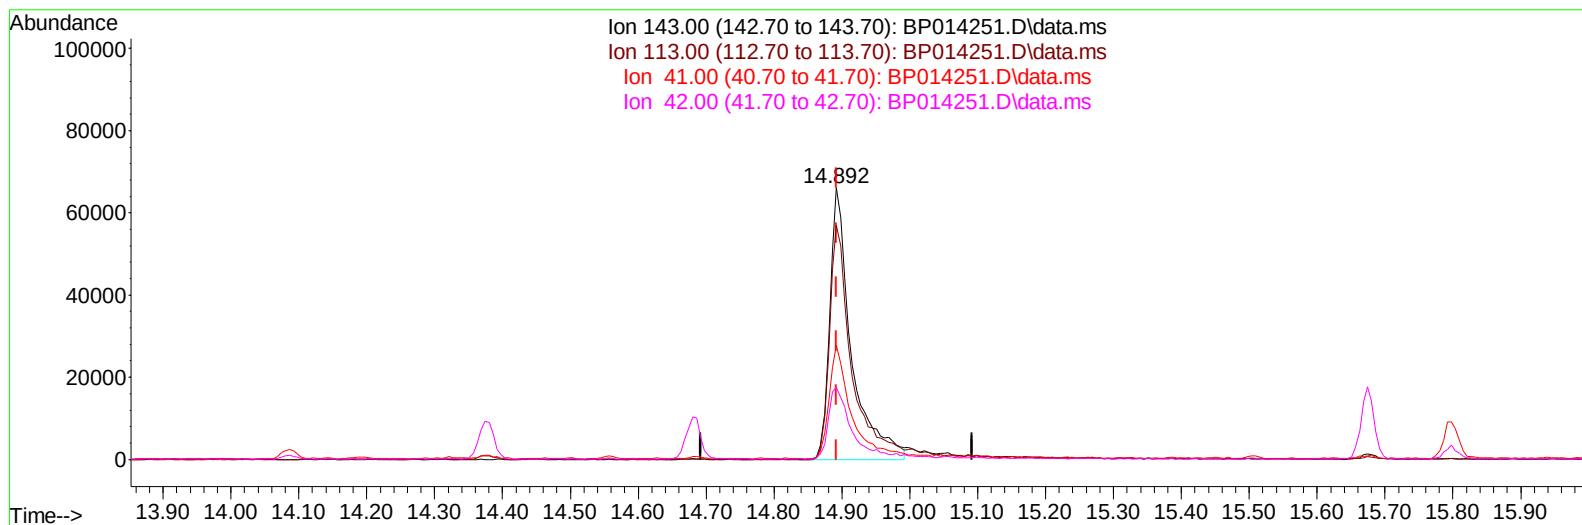

TIC: BP014251.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.892min (-0.000) 19.94 ng/ul m

response 146262

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	103.10	86.13
41.00	40.20	42.20
42.00	28.50	26.60

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032223\
 Data File : BP014251.D
 Acq On : 23 Mar 2023 11:17
 Operator : CG/JU
 Sample : 01977-21
 Misc :
 ALS Vial : 31 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EYGA6

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 03/24/2023
 Supervised By :Jagrut Upadhyay 03/24/2023

Quant Time: Mar 24 01:51:05 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Mar 23 04:56:06 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.034	152	146387	20.000	ng/ul	0.00
20) Naphthalene-d8	10.857	136	667651	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.680	164	490435	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.439	188	1146183	20.000	ng/ul	# 0.00
79) Chrysene-d12	21.521	240	1141766	20.000	ng/ul	# 0.00
88) Perylene-d12	24.039	264	1158315	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.404	96	18096	4.671	ng/uL	0.00
4) Pyridine-d5	3.840	84	234977	21.904	ng/ul	0.00
7) Phenol-d5	7.192	99	337549	26.130	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	7.357	67	220713	29.296	ng/ul	0.00
11) 2-Chlorophenol-d4	7.563	132	251153	25.518	ng/ul	0.00
15) 4-Methylphenol-d8	8.751	113	284706	26.981	ng/ul	0.00
21) Nitrobenzene-d5	9.210	128	132862	24.940	ng/ul	0.00
24) 2-Nitrophenol-d4	9.939	143	155688	24.414	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.481	165	279230	23.272	ng/ul	0.00
31) 4-Chloroaniline-d4	11.004	131	375774	23.665	ng/ul	0.00
46) Dimethylphthalate-d6	14.086	166	1073421	25.790	ng/ul	0.00
49) Acenaphthylene-d8	14.374	160	1127459	25.571	ng/ul	0.00
54) 4-Nitrophenol-d4	14.892	143	146262m	19.941	ng/ul	0.00
60) Fluorene-d10	15.674	176	905643	25.674	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.798	200	169723	19.592	ng/ul	0.00
73) Anthracene-d10	17.539	188	1449608	26.053	ng/ul	0.00
81) Pyrene-d10	19.768	212	1758833	27.930	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.880	264	1627518	26.415	ng/ul	0.00

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032223\
Data File : BP014251.D
Acq On : 23 Mar 2023 11:17
Operator : CG/JU
Sample : 01977-21
Misc :
ALS Vial : 31 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EYGA6

Manual IntegrationsAPPROVED

Reviewed By :Christian Giraldo 03/24/2023
Supervised By :Jagrut Upadhyay 03/24/2023

Quant Time: Mar 24 01:51:05 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Mar 23 04:56:06 2023
Response via : Initial Calibration

