

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032223\
 Data File : BP014225.D
 Acq On : 22 Mar 2023 19:54
 Operator : CG/JU
 Sample : 01977-02
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EYG88

Quant Time: Mar 23 02:35:36 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Mar 23 02:31:48 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.040	152	130912	20.000	ng/u1	0.00
20) Naphthalene-d8	10.863	136	591986	20.000	ng/u1	0.00
38) Acenaphthene-d10	14.687	164	433944	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.445	188	1035413	20.000	ng/u1	# 0.00
79) Chrysene-d12	21.527	240	1054319	20.000	ng/u1	# 0.00
88) Perylene-d12	24.051	264	1107185	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.405	96	26015	7.508	ng/uL	0.00
4) Pyridine-d5	3.840	84	357235	37.238	ng/u1	0.00
7) Phenol-d5	7.199	99	518020	44.840	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.364	67	334865	49.701	ng/u1	0.00
11) 2-Chlorophenol-d4	7.569	132	383694	43.593	ng/u1	0.00
15) 4-Methylphenol-d8	8.758	113	426891	45.238	ng/u1	0.00
21) Nitrobenzene-d5	9.216	128	210249	44.512	ng/u1	0.00
24) 2-Nitrophenol-d4	9.946	143	245996	43.507	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.487	165	427383	40.172	ng/u1	0.00
31) 4-Chloroaniline-d4	11.005	131	505882	35.931	ng/u1	0.00
46) Dimethylphthalate-d6	14.093	166	1603913	43.552	ng/u1	0.00
49) Acenaphthylene-d8	14.381	160	1715079	43.962	ng/u1	0.00
54) 4-Nitrophenol-d4	14.898	143	251706	38.784	ng/u1	0.00
60) Fluorene-d10	15.681	176	1357057	43.479	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.804	200	286514	36.612	ng/u1	0.00
73) Anthracene-d10	17.545	188	2227749	44.321	ng/u1	0.00
81) Pyrene-d10	19.769	212	2696448	46.371	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.886	264	2659139	45.151	ng/u1	0.00
Target Compounds						
86) Bis(2-ethylhexyl)phtha...	21.404	149	68694	1.648	ng/u1#	Qvalue 98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032223\
Data File : BP014225.D
Acq On : 22 Mar 2023 19:54
Operator : CG/JU
Sample : 01977-02
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EYG88

Quant Time: Mar 23 02:35:36 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Mar 23 02:31:48 2023
Response via : Initial Calibration

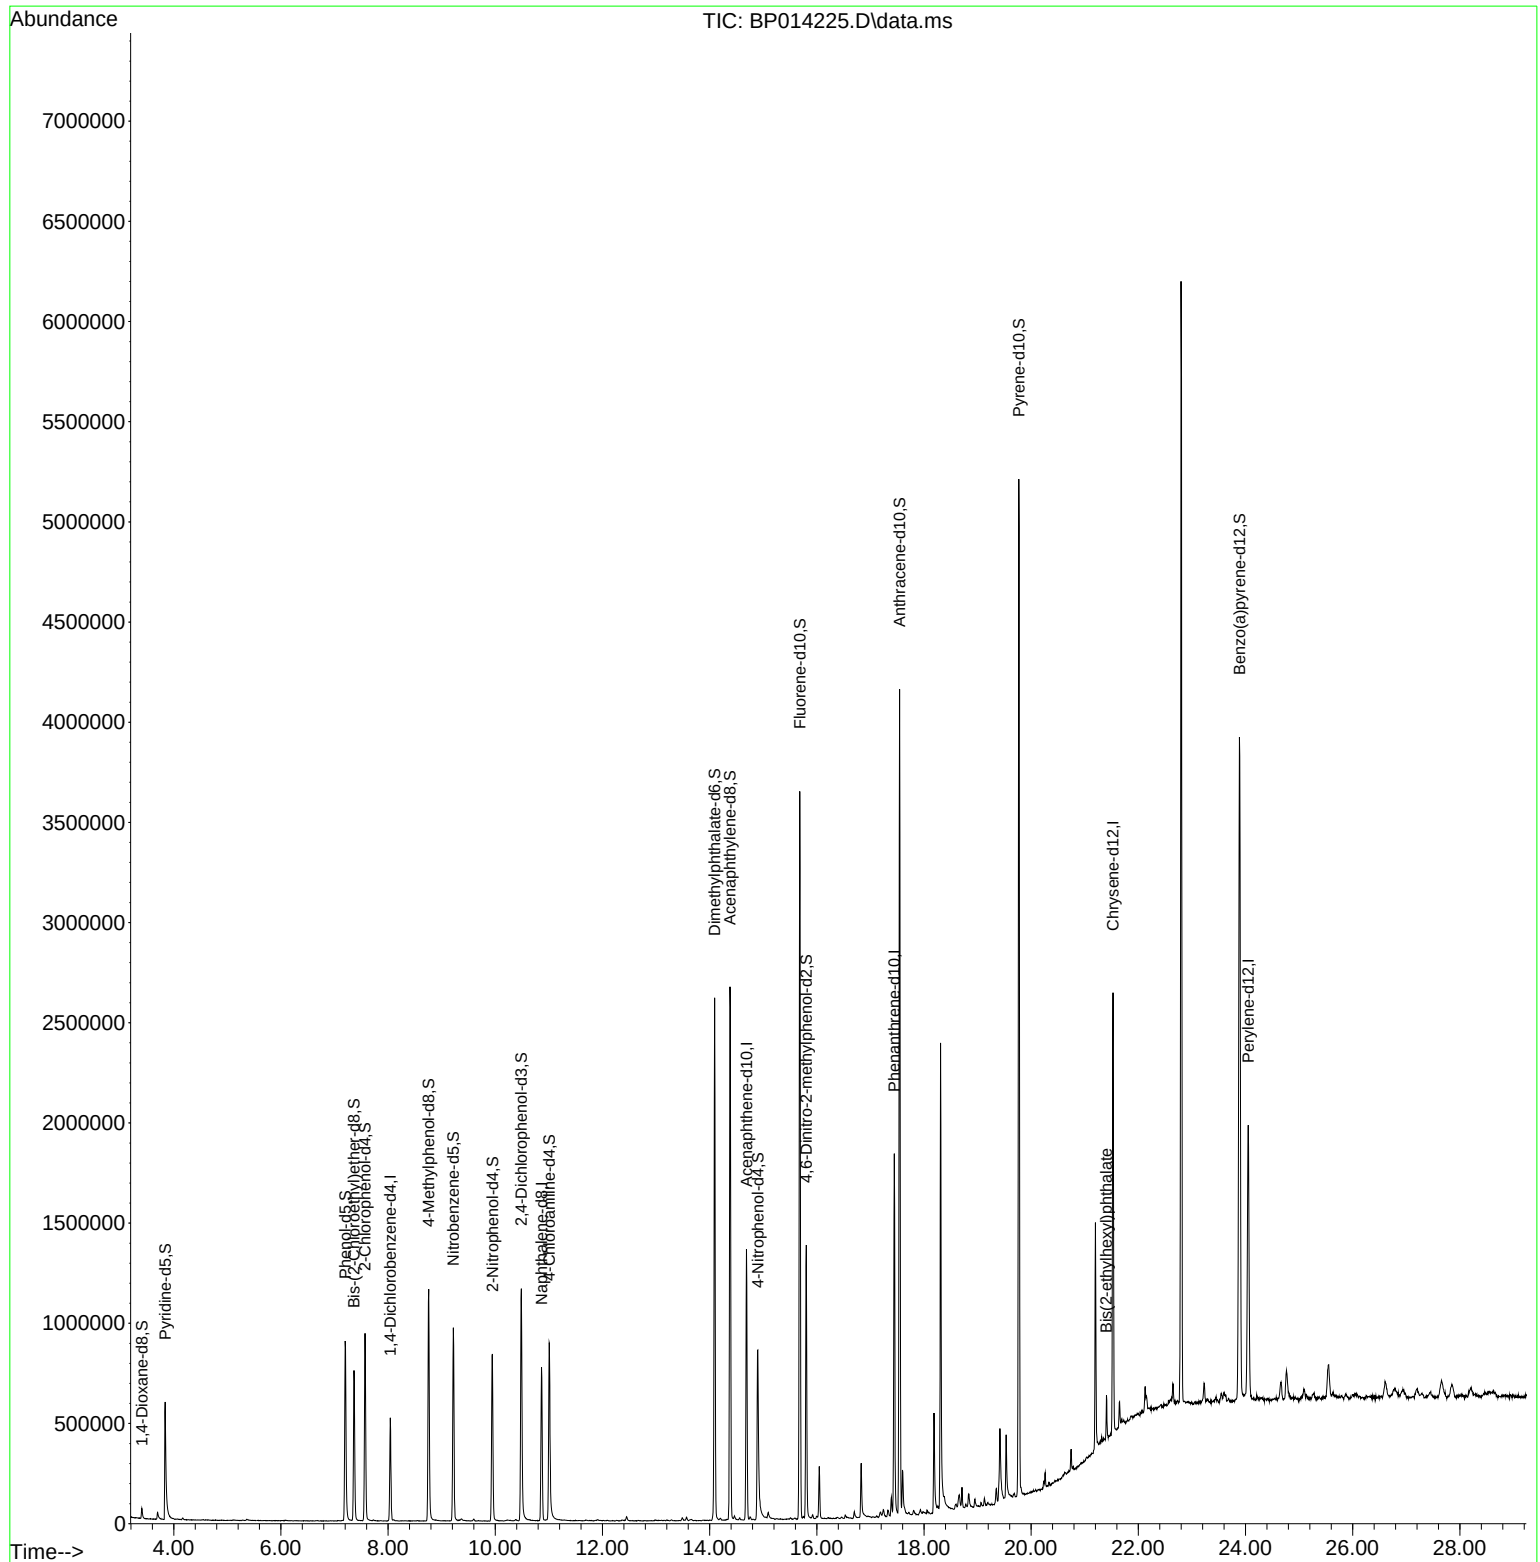

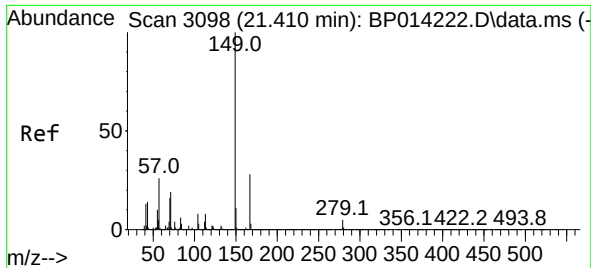

#86
 Bis(2-ethylhexyl)phthalate
 Concen: 1.648 ng/ul
 RT: 21.404 min Scan# 30
 Delta R.T. -0.006 min
 Lab File: BP014225.D
 Acq: 22 Mar 2023 19:54

Instrument :
 BNA_P
 ClientSampleId :
 EYG88

Tgt Ion:149 Resp: 68694
 Ion Ratio Lower Upper
 149 100
 167 27.1 22.3 33.5
 279 3.8 4.3 6.5#

