

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032223\
 Data File : BP014237.D
 Acq On : 23 Mar 2023 02:45
 Operator : CG/JU
 Sample : 01977-14
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EYGA1

Quant Time: Mar 23 03:12:03 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Mar 23 02:31:48 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.040	152	137452	20.000	ng/u1	0.00
20) Naphthalene-d8	10.863	136	625425	20.000	ng/u1	# 0.00
38) Acenaphthene-d10	14.681	164	466716	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.439	188	1113810	20.000	ng/u1	# 0.00
79) Chrysene-d12	21.522	240	1133736	20.000	ng/u1	#-0.01
88) Perylene-d12	24.039	264	1199486	20.000	ng/u1	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.405	96	16782	4.613	ng/uL	0.00
4) Pyridine-d5	3.840	84	217102	21.554	ng/u1	0.00
7) Phenol-d5	7.199	99	306424	25.262	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.364	67	203522	28.770	ng/u1	0.00
11) 2-Chlorophenol-d4	7.569	132	233237	25.238	ng/u1	0.00
15) 4-Methylphenol-d8	8.752	113	259383	26.179	ng/u1	0.00
21) Nitrobenzene-d5	9.210	128	123054	24.659	ng/u1	0.00
24) 2-Nitrophenol-d4	9.940	143	143649	24.047	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.481	165	247685	22.036	ng/u1	0.00
31) 4-Chloroaniline-d4	11.004	131	347944	23.392	ng/u1	0.00
46) Dimethylphthalate-d6	14.087	166	990232	25.000	ng/u1	0.00
49) Acenaphthylene-d8	14.381	160	1045592	24.919	ng/u1	0.00
54) 4-Nitrophenol-d4	14.898	143	141462	20.267	ng/u1	0.00
60) Fluorene-d10	15.675	176	849890	25.318	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.798	200	162008	19.245	ng/u1	0.00
73) Anthracene-d10	17.539	188	1367035	25.283	ng/u1	0.00
81) Pyrene-d10	19.763	212	1676589	26.813	ng/u1	-0.01
92) Benzo(a)pyrene-d12	23.874	264	1633699	25.605	ng/u1	-0.02
Target Compounds						
86) Bis(2-ethylhexyl)phtha...	21.404	149	48349	1.079	ng/u1	Qvalue 100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032223\
Data File : BP014237.D
Acq On : 23 Mar 2023 02:45
Operator : CG/JU
Sample : 01977-14
Misc :
ALS Vial : 17 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EYGA1

Quant Time: Mar 23 03:12:03 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Mar 23 02:31:48 2023
Response via : Initial Calibration

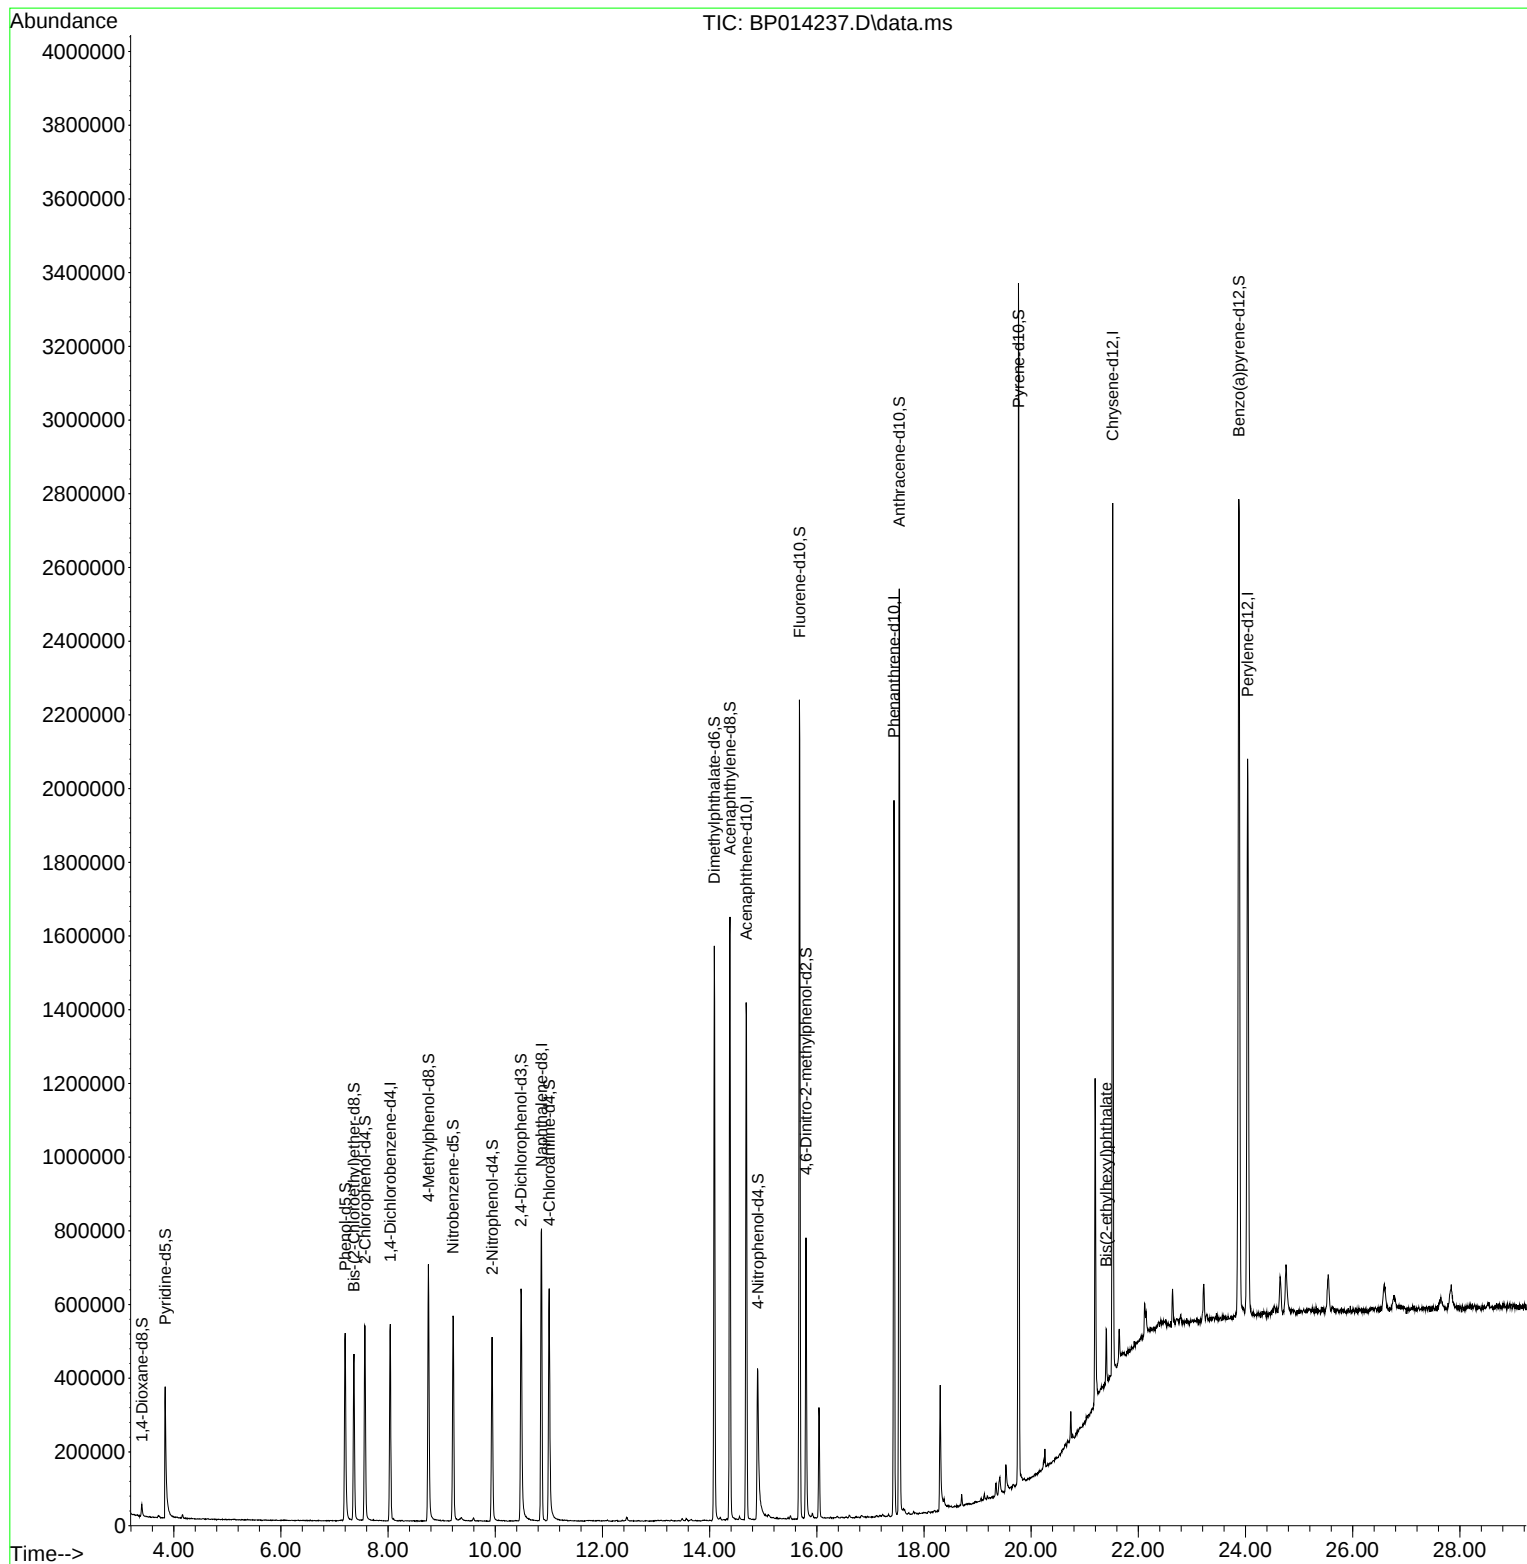

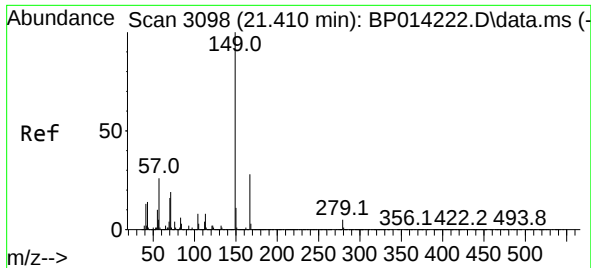

#86
 Bis(2-ethylhexyl)phthalate
 Concen: 1.079 ng/ul
 RT: 21.404 min Scan# 3097
 Delta R.T. -0.006 min
 Lab File: BP014237.D
 Acq: 23 Mar 2023 02:45

Instrument :
 BNA_P
 ClientSampleId :
 EYGA1

Tgt Ion:149	Resp:	48349
Ion Ratio	Lower	Upper
149	100	
167	27.7	22.3 33.5
279	5.1	4.3 6.5

