

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032223\
 Data File : BP014277.D
 Acq On : 24 Mar 2023 02:42
 Operator : CG/JU
 Sample : 01960-13
 Misc :
 ALS Vial : 57 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 EYFG1

Quant Time: Mar 24 03:24:33 2023
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Mar 23 04:56:06 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	8.034	152	143169	20.000	ng/ul	0.00
20) Naphthalene-d8	10.857	136	566794	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.680	164	407298	20.000	ng/ul	0.00
64) Phenanthrene-d10	17.433	188	1030518	20.000	ng/ul	#-0.01
79) Chrysene-d12	21.515	240	948728	20.000	ng/ul	# 0.00
88) Perylene-d12	24.039	264	902499	20.000	ng/ul	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	0.000	96	0d	0.000	ng/uL	
4) Pyridine-d5	0.000	84	0d	0.000	ng/ul	
7) Phenol-d5	0.000	99	0d	0.000	ng/ul	
9) Bis-(2-Chloroethyl)eth...	0.000	67	0d	0.000	ng/ul	
11) 2-Chlorophenol-d4	0.000	132	0d	0.000	ng/ul	
15) 4-Methylphenol-d8	0.000	113	0d	0.000	ng/ul	
21) Nitrobenzene-d5	0.000	128	0d	0.000	ng/ul	
24) 2-Nitrophenol-d4	0.000	143	0d	0.000	ng/ul	
28) 2,4-Dichlorophenol-d3	0.000	165	0d	0.000	ng/ul	
31) 4-Chloroaniline-d4	0.000	131	0d	0.000	ng/ul	
46) Dimethylphthalate-d6	0.000	166	0d	0.000	ng/ul	
49) Acenaphthylene-d8	0.000	160	0d	0.000	ng/ul	
54) 4-Nitrophenol-d4	0.000	143	0d	0.000	ng/ul	
60) Fluorene-d10	0.000	176	0d	0.000	ng/ul	
65) 4,6-Dinitro-2-methylph...	0.000	200	0d	0.000	ng/ul	
73) Anthracene-d10	0.000	188	0d	0.000	ng/ul	
81) Pyrene-d10	0.000	212	0d	0.000	ng/ul	
92) Benzo(a)pyrene-d12	0.000	264	0d	0.000	ng/ul	


Target Compounds					Qvalue
30) Naphthalene	10.904	128	54479	1.750 ng/ul	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032223\
Data File : BP014277.D
Acq On : 24 Mar 2023 02:42
Operator : CG/JU
Sample : 01960-13
Misc :
ALS Vial : 57 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EYFG1

Quant Time: Mar 24 03:24:33 2023
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Mar 23 04:56:06 2023
Response via : Initial Calibration

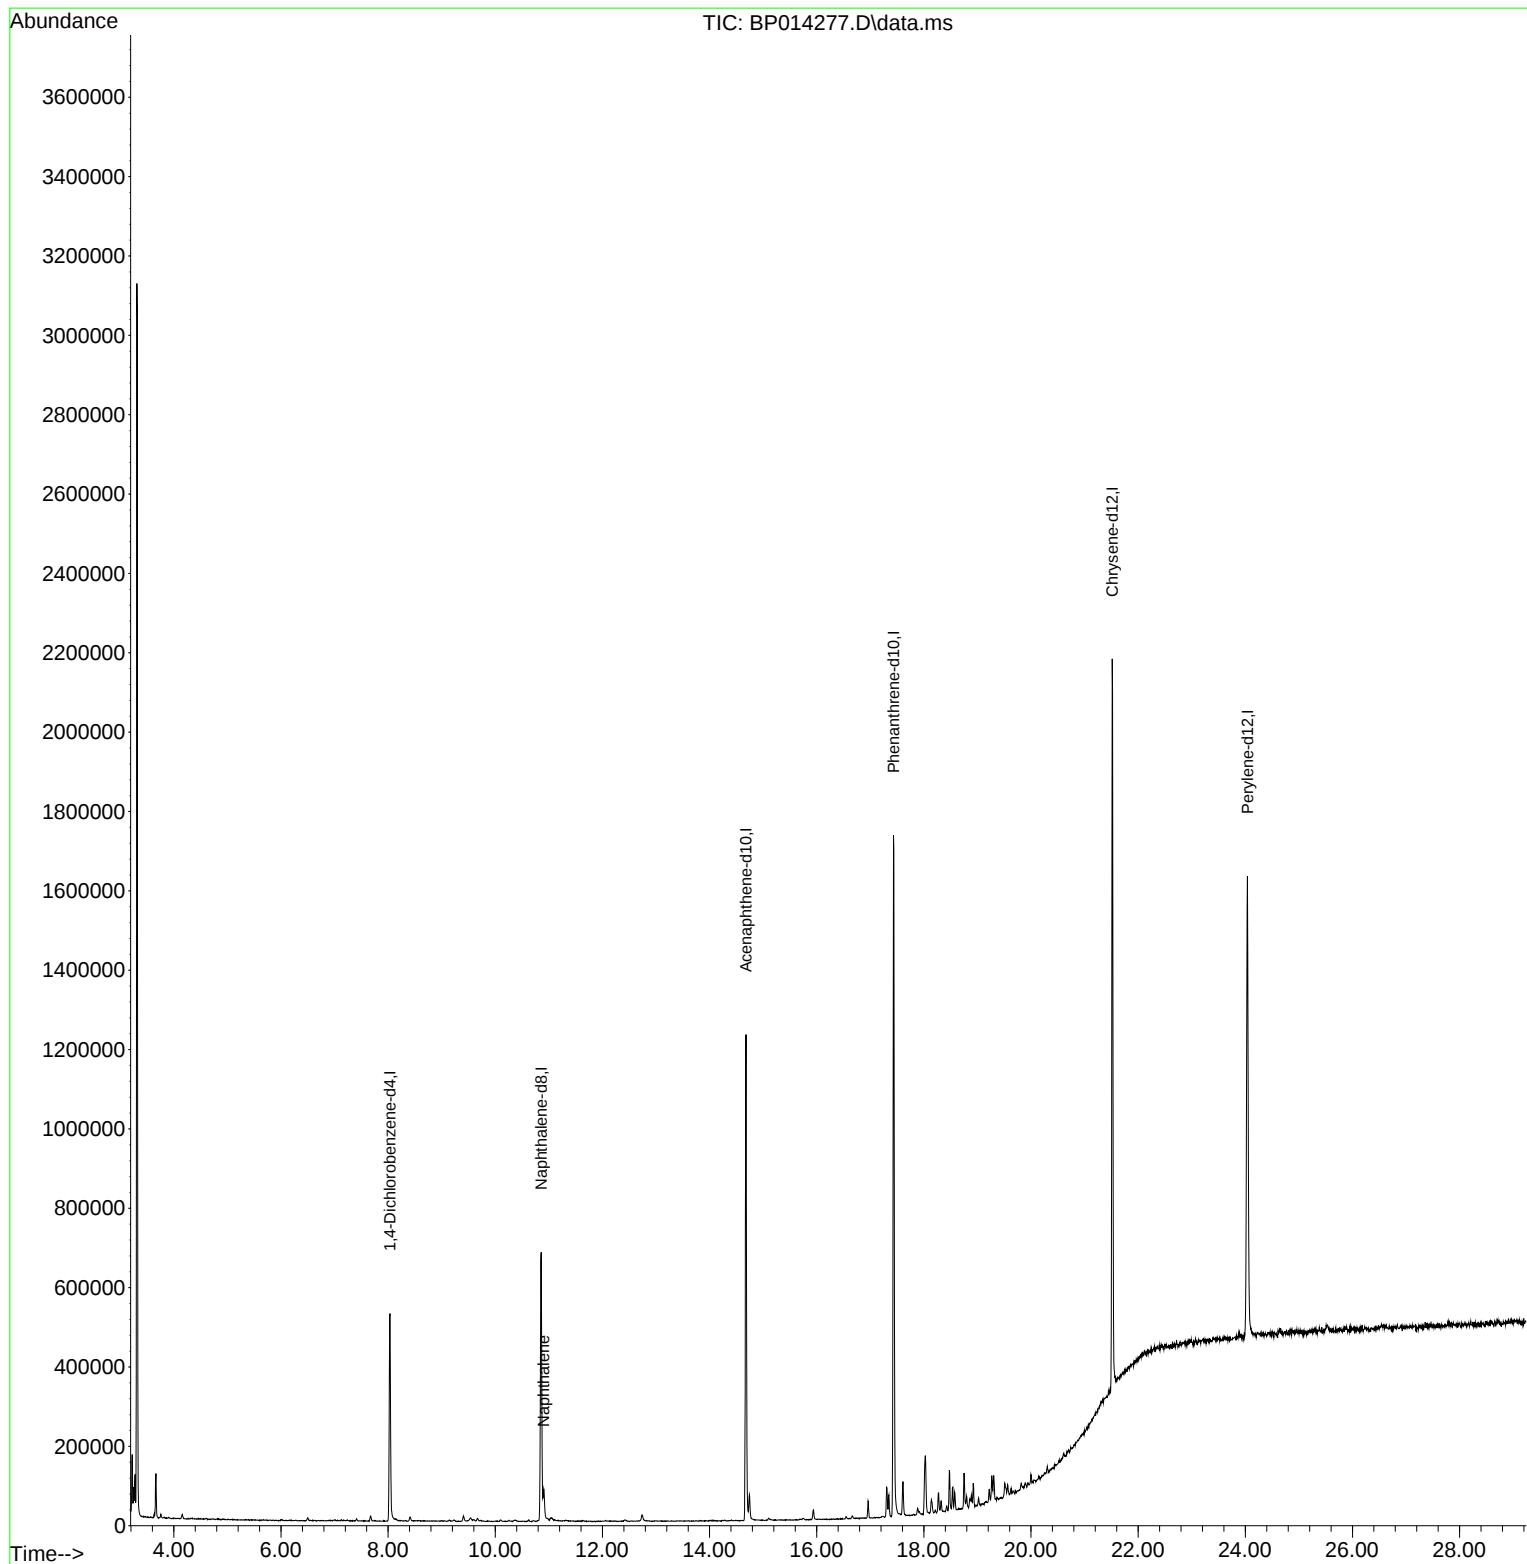

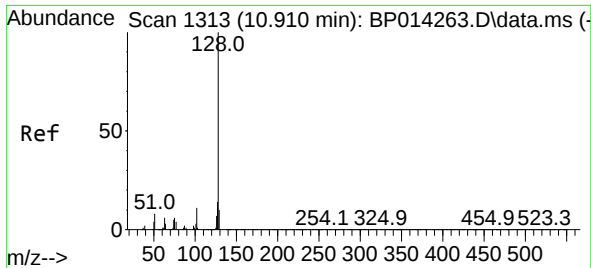

#30

Naphthalene

Concen: 1.750 ng/ul

RT: 10.904 min Scan# 11

Delta R.T. -0.006 min

Lab File: BP014277.D

Acq: 24 Mar 2023 02:42

Instrument :

BNA_P

ClientSampleId :

EYFG1

Tgt Ion:128 Resp: 54479

Ion Ratio Lower Upper

128 100

129 11.7 8.5 12.7

127 15.0 11.0 16.4

