

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032223\
 Data File : BP014243.D
 Acq On : 23 Mar 2023 06:44
 Operator : CG/JU
 Sample : 01996-09DL 5X
 Misc :
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 H0A30DL

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
 Title : SVOA CALIBRATION

Signal : TIC: BP014243.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.370	26	31	39	rBV	246850	410891	4.79%	1.052%
2	3.440	39	43	55	rVB	144868	211984	2.47%	0.543%
3	3.870	113	116	132	rVB	23423	54386	0.63%	0.139%
4	4.164	162	166	174	rVB2	12493	19267	0.22%	0.049%
5	4.705	251	258	273	rBV	5520587	8586582	100.00%	21.980%
6	7.205	677	683	693	rBV	31208	68811	0.80%	0.176%
7	7.364	704	710	722	rBV	142759	238439	2.78%	0.610%
8	7.569	737	745	759	rBV	129943	245447	2.86%	0.628%
9	8.034	817	824	838	rBV	682409	1161663	13.53%	2.974%
10	8.758	941	947	961	rBV	94982	201486	2.35%	0.516%
11	9.216	1017	1025	1036	rBV	171341	313011	3.65%	0.801%
12	9.346	1041	1047	1048	rBV6	6737	8626	0.10%	0.022%
13	9.940	1139	1148	1157	rBV	141934	267004	3.11%	0.683%
14	10.493	1235	1242	1261	rBV	158092	387484	4.51%	0.992%
15	10.857	1297	1304	1315	rBV	1040401	1803611	21.00%	4.617%
16	11.010	1323	1330	1346	rBV	98351	233999	2.73%	0.599%
17	11.828	1463	1469	1480	rBV2	24177	71687	0.83%	0.184%
18	12.387	1559	1564	1571	rVB7	6337	14808	0.17%	0.038%
19	12.452	1571	1575	1581	rBV9	4745	10218	0.12%	0.026%
20	13.563	1756	1764	1771	rVB3	17066	29681	0.35%	0.076%
21	14.087	1845	1853	1866	rBV	579511	844683	9.84%	2.162%
22	14.375	1896	1902	1917	rBV	566227	868594	10.12%	2.223%
23	14.681	1947	1954	1966	rBV	1935566	2916744	33.97%	7.466%
24	14.951	1995	2000	2007	rBV10	12101	37322	0.43%	0.096%
25	15.675	2116	2123	2139	rBV	824645	1246093	14.51%	3.190%
26	15.804	2139	2145	2156	rBV	197887	358369	4.17%	0.917%
27	16.045	2181	2186	2192	rVB2	21450	30358	0.35%	0.078%
28	17.222	2384	2386	2397	rBV5	6173	13214	0.15%	0.034%
29	17.439	2417	2423	2434	rBV	2751098	3824562	44.54%	9.790%
30	17.539	2434	2440	2450	rVV	1016827	1449239	16.88%	3.710%
31	18.304	2566	2570	2578	rBV2	56099	107116	1.25%	0.274%
32	18.398	2582	2586	2593	rVB	86730	134120	1.56%	0.343%
33	19.533	2776	2779	2782	rBV4	25491	34743	0.40%	0.089%
34	19.763	2813	2818	2824	rBV	1338266	1840819	21.44%	4.712%
35	21.522	3112	3117	3124	rBV	3326297	4406027	51.31%	11.278%
36	22.792	3329	3333	3337	rVB	286741	389284	4.53%	0.996%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032223\
Data File : BP014243.D
Acq On : 23 Mar 2023 06:44
Operator : CG/JU
Sample : 01996-09DL 5X
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
H0A30DL

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Title : SVOA CALIBRATION

37	23.874	3512	3517	3527	rVB2	895299	1781634	20.75%	4.561%
38	24.045	3539	3546	3558	rVB2	2042361	4444185	51.76%	11.376%




Sum of corrected areas: 39066191

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032223\
Data File : BP014243.D
Acq On : 23 Mar 2023 06:44
Operator : CG/JU
Sample : 01996-09DL 5X
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
H0A30DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

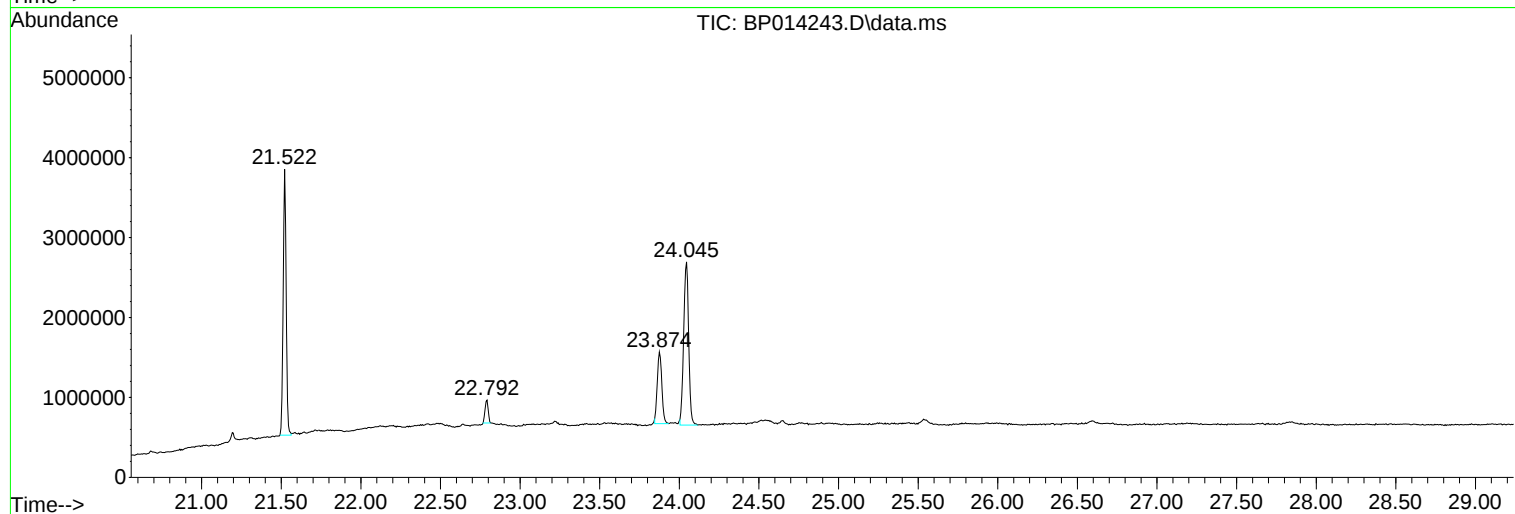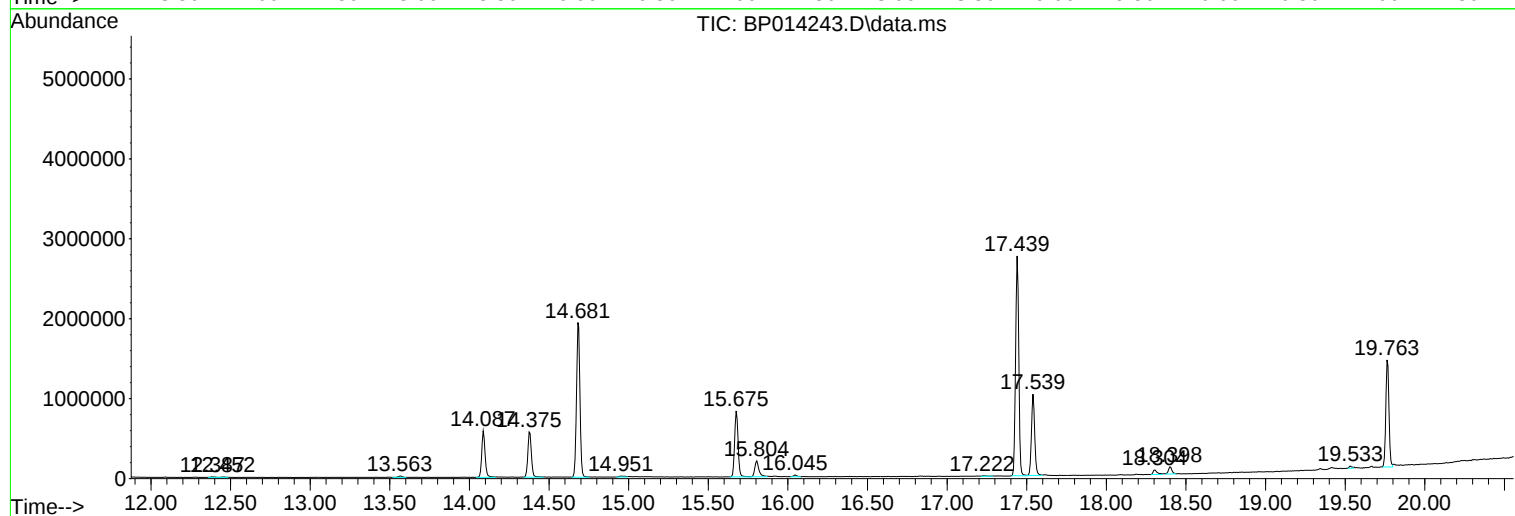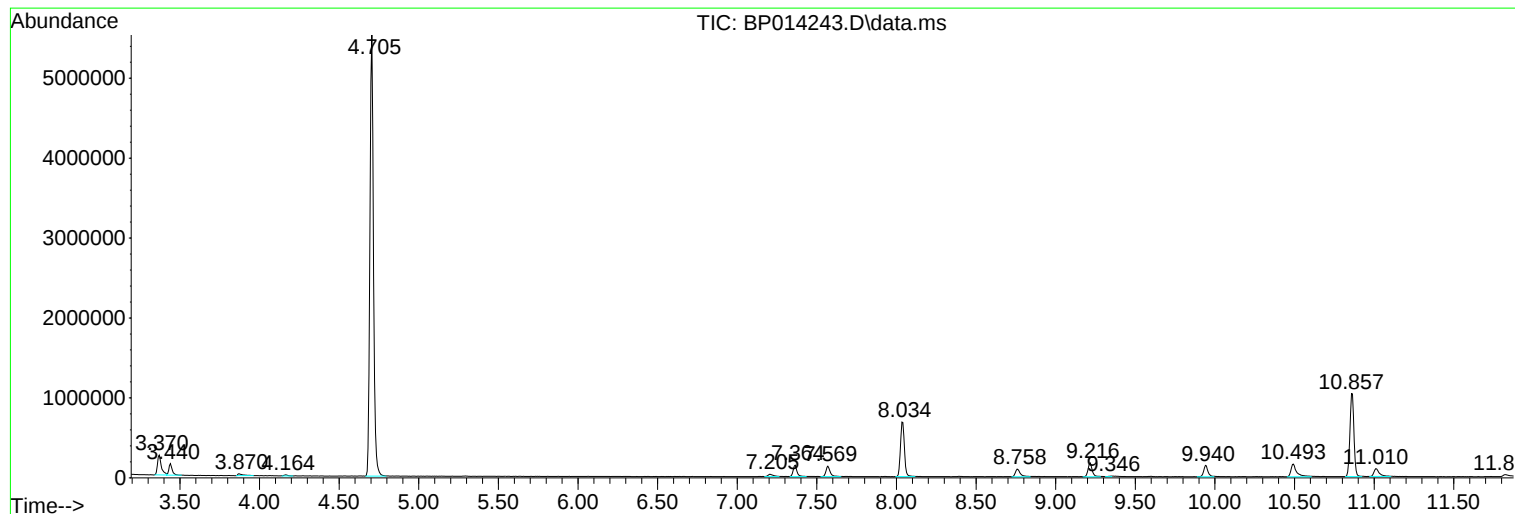

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032223\
Data File : BP014243.D
Acq On : 23 Mar 2023 06:44
Operator : CG/JU
Sample : 01996-09DL 5X
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
H0A30DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032223\
Data File : BP014243.D
Acq On : 23 Mar 2023 06:44
Operator : CG/JU
Sample : 01996-09DL 5X
Misc :
ALS Vial : 23 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
H0A30DL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
					# RT Resp Conc