

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032223\
 Data File : BP014255.D
 Acq On : 23 Mar 2023 13:34
 Operator : CG/JU
 Sample : PB151603BL
 Misc :
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK603

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
 Title : SVOA CALIBRATION

Signal : TIC: BP014255.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.405	33	37	45	rVB	39234	60503	1.17%	0.125%
2	3.834	107	110	130	rBV	438944	784525	15.11%	1.625%
3	4.164	162	166	172	rVB	10036	16193	0.31%	0.034%
4	7.193	674	681	696	rBV	603943	1037782	19.99%	2.150%
5	7.358	703	709	722	rBV	513224	816811	15.73%	1.692%
6	7.564	738	744	759	rBV	631037	1039660	20.02%	2.154%
7	8.034	816	824	836	rBV	482002	785622	15.13%	1.627%
8	8.752	936	946	964	rBV	765384	1377819	26.53%	2.854%
9	9.210	1017	1024	1037	rBV	647417	1097253	21.13%	2.273%
10	9.934	1136	1147	1161	rBV	545269	984127	18.95%	2.039%
11	10.481	1232	1240	1260	rBV	737174	1414944	27.25%	2.931%
12	10.857	1296	1304	1314	rBV	727707	1208206	23.27%	2.503%
13	10.999	1320	1328	1344	rBV	757219	1484332	28.59%	3.075%
14	12.452	1568	1575	1586	rBV4	11818	27432	0.53%	0.057%
15	13.569	1759	1765	1769	rBV8	6031	9846	0.19%	0.020%
16	13.663	1776	1781	1784	rBV6	2633	5440	0.10%	0.011%
17	14.087	1846	1853	1867	rBV	1840212	2553612	49.18%	5.290%
18	14.375	1895	1902	1918	rBV	1937846	2827057	54.44%	5.856%
19	14.681	1947	1954	1966	rBV	1275856	1906630	36.72%	3.949%
20	14.893	1983	1990	2020	rBV	480393	1193433	22.98%	2.472%
21	15.675	2116	2123	2138	rBV	2594406	3692495	71.11%	7.649%
22	15.798	2138	2144	2157	rVV	883753	1328459	25.58%	2.752%
23	15.916	2160	2164	2171	rVB3	13631	27577	0.53%	0.057%
24	16.463	2250	2257	2261	rVB10	4760	10057	0.19%	0.021%
25	17.234	2382	2388	2390	rBV7	5509	8108	0.16%	0.017%
26	17.439	2416	2423	2432	rBV	1765836	2493493	48.02%	5.165%
27	17.539	2433	2440	2452	rVV	3017479	4287317	82.57%	8.881%
28	19.345	2743	2747	2752	rVB3	39502	48940	0.94%	0.101%
29	19.416	2755	2759	2763	rBV2	31505	45563	0.88%	0.094%
30	19.763	2813	2818	2832	rBV	3825812	5192643	100.00%	10.756%
31	21.522	3112	3117	3127	rBV	2072045	2908093	56.00%	6.024%
32	23.880	3511	3518	3529	rVB2	2491538	4886218	94.10%	10.121%
33	24.045	3539	3546	3557	rVB2	1253291	2716708	52.32%	5.627%




Sum of corrected areas: 48276898

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032223\
Data File : BP014255.D
Acq On : 23 Mar 2023 13:34
Operator : CG/JU
Sample : PB151603BL
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK603

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

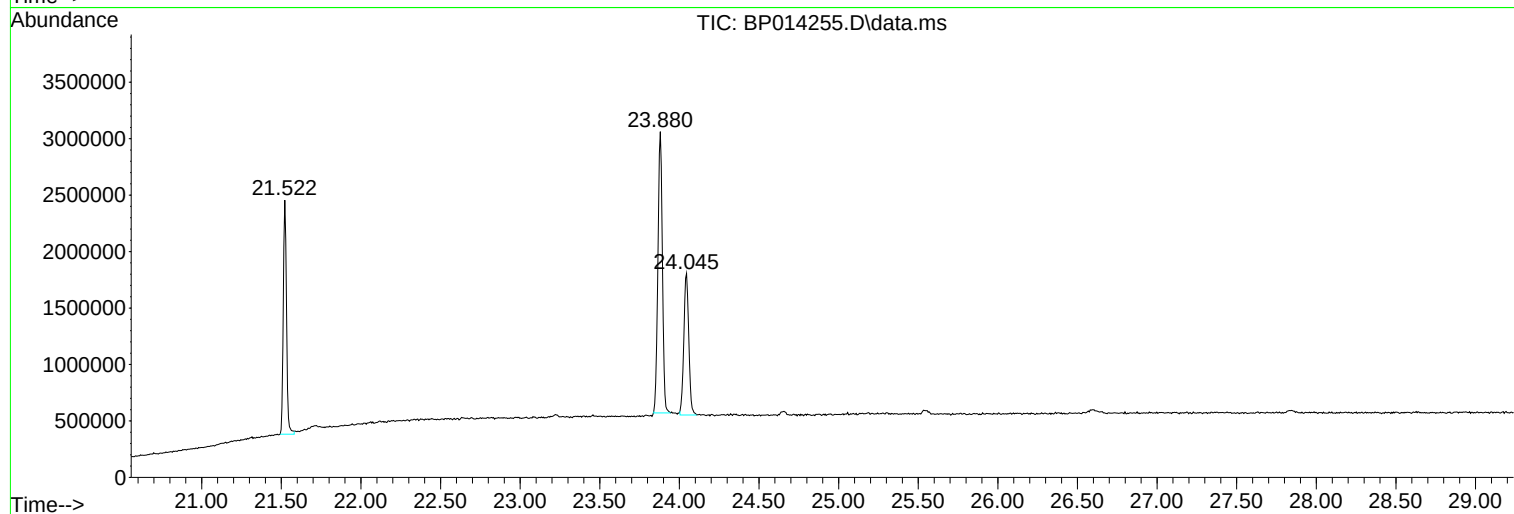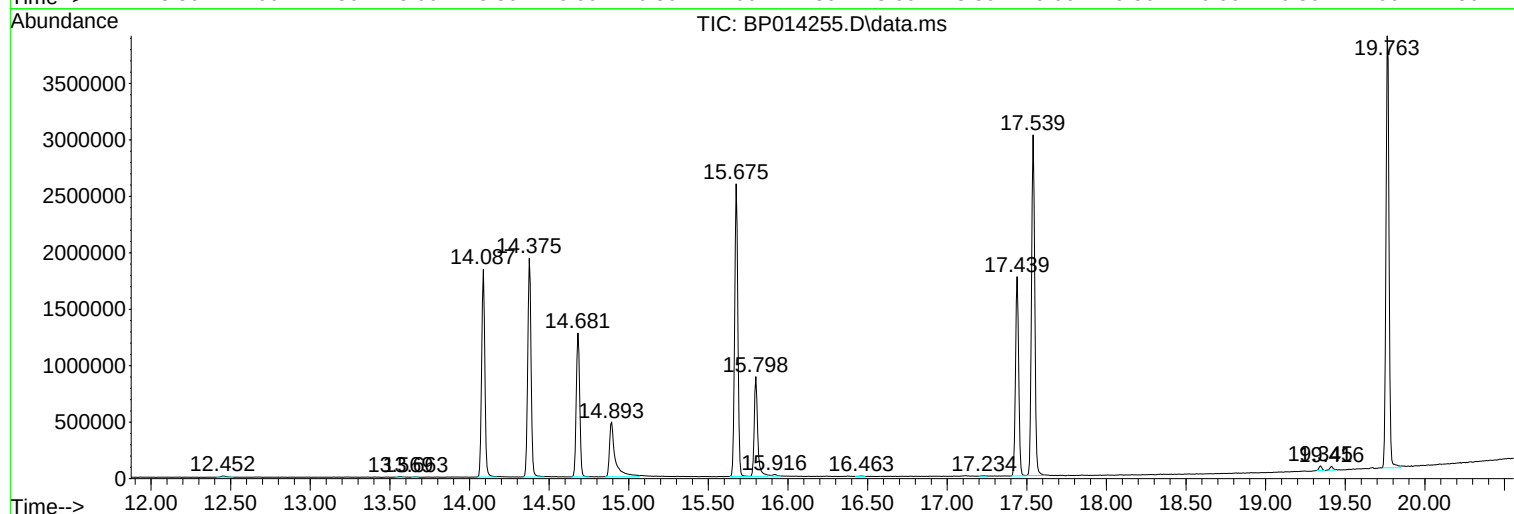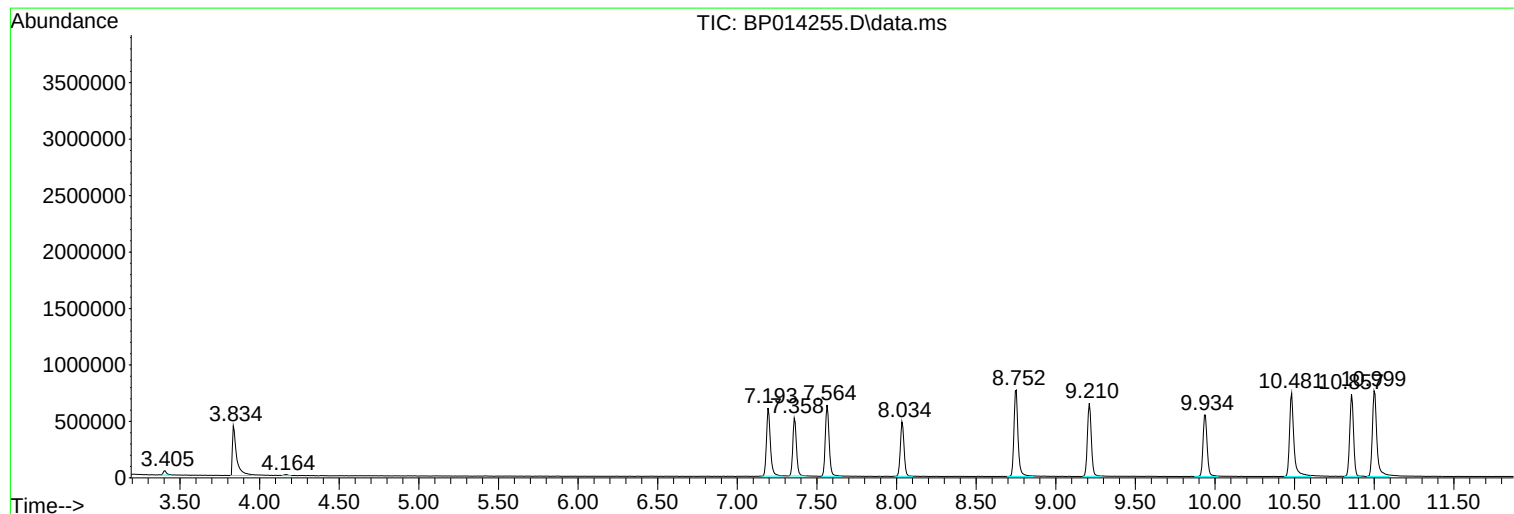

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032223\
Data File : BP014255.D
Acq On : 23 Mar 2023 13:34
Operator : CG/JU
Sample : PB151603BL
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK603

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032223\
Data File : BP014255.D
Acq On : 23 Mar 2023 13:34
Operator : CG/JU
Sample : PB151603BL
Misc :
ALS Vial : 35 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK603

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc