

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032223\
 Data File : BP014260.D
 Acq On : 23 Mar 2023 16:25
 Operator : CG/JU
 Sample : 02010-02
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CB945

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
 Title : SVOA CALIBRATION

Signal : TIC: BP014260.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.405	33	37	43	rBV	21982	32960	0.50%	0.066%
2	3.846	110	112	131	rBV	105265	196361	2.97%	0.396%
3	4.058	145	148	155	rVB5	4841	8826	0.13%	0.018%
4	4.164	161	166	171	rBV3	10355	17608	0.27%	0.036%
5	5.128	326	330	333	rVB5	4603	7008	0.11%	0.014%
6	5.440	379	383	389	rBV4	6820	10099	0.15%	0.020%
7	5.781	436	441	449	rBV4	5653	13982	0.21%	0.028%
8	7.199	676	682	692	rBV	84780	168789	2.55%	0.340%
9	7.357	703	709	722	rBV	456044	727783	11.00%	1.468%
10	7.563	737	744	754	rBV	391637	668004	10.09%	1.347%
11	8.034	817	824	832	rBV	510565	835841	12.63%	1.686%
12	8.752	938	946	958	rBV	310706	562142	8.49%	1.134%
13	9.210	1017	1024	1037	rBV	592835	1002983	15.15%	2.023%
14	9.369	1047	1051	1058	rVB10	3853	8117	0.12%	0.016%
15	9.593	1082	1089	1095	rVB3	12020	20365	0.31%	0.041%
16	9.934	1140	1147	1160	rBV	471770	821410	12.41%	1.657%
17	10.246	1194	1200	1201	rBV6	5223	7986	0.12%	0.016%
18	10.369	1214	1221	1226	rBV8	7649	16312	0.25%	0.033%
19	10.481	1231	1240	1263	rBV	628653	1220185	18.44%	2.461%
20	10.857	1295	1304	1317	rBV	793270	1333338	20.15%	2.689%
21	10.998	1321	1328	1345	rBV	556141	1110785	16.78%	2.240%
22	12.093	1511	1514	1518	rVB6	4706	6926	0.10%	0.014%
23	12.204	1527	1533	1537	rBV3	9101	18136	0.27%	0.037%
24	12.445	1569	1574	1579	rBV4	11261	19947	0.30%	0.040%
25	12.675	1606	1613	1616	rBV2	6142	10242	0.15%	0.021%
26	13.487	1747	1751	1754	rBV5	5523	9889	0.15%	0.020%
27	13.563	1759	1764	1770	rVB3	23260	36106	0.55%	0.073%
28	14.087	1846	1853	1864	rBV	1797784	2541478	38.40%	5.126%
29	14.375	1895	1902	1912	rBV	1850282	2672489	40.38%	5.390%
30	14.681	1947	1954	1962	rBV	1395827	2130693	32.19%	4.297%
31	14.798	1971	1974	1981	rVB6	9974	15855	0.24%	0.032%
32	14.916	1989	1994	2012	rBV2	48545	172048	2.60%	0.347%
33	15.175	2035	2038	2047	rVB4	10554	16373	0.25%	0.033%
34	15.492	2089	2092	2097	rVB4	8181	12228	0.18%	0.025%
35	15.675	2116	2123	2137	rBV	4787159	6618554	100.00%	13.349%
36	15.798	2138	2144	2154	rVV	919492	1309998	19.79%	2.642%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032223\
 Data File : BP014260.D
 Acq On : 23 Mar 2023 16:25
 Operator : CG/JU
 Sample : 02010-02
 Misc :
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 CB945

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
 Title : SVOA CALIBRATION

37	15.881	2155	2158	2162	rVV	31893	49863	0.75%	0.101%
38	15.934	2162	2167	2174	rVV6	31840	64421	0.97%	0.130%
39	16.039	2177	2185	2192	rBV2	107235	188386	2.85%	0.380%
40	16.186	2205	2210	2217	rVB	70438	92022	1.39%	0.186%
41	16.410	2244	2248	2255	rBV2	18168	26868	0.41%	0.054%
42	16.504	2259	2264	2268	rBV	48839	64261	0.97%	0.130%
43	16.557	2268	2273	2280	rBV2	56438	105987	1.60%	0.214%
44	16.622	2280	2284	2288	rBV2	51464	71118	1.07%	0.143%
45	16.669	2288	2292	2296	rVB2	27327	34681	0.52%	0.070%
46	16.722	2297	2301	2307	rBV4	21529	50448	0.76%	0.102%
47	16.828	2314	2319	2326	rBV4	40469	73867	1.12%	0.149%
48	16.892	2326	2330	2334	rBV	41731	56281	0.85%	0.114%
49	16.969	2339	2343	2349	rVB2	28326	43793	0.66%	0.088%
50	17.022	2350	2352	2358	rVB7	5752	8680	0.13%	0.018%
51	17.345	2405	2407	2410	rVB4	7441	6901	0.10%	0.014%
52	17.439	2416	2423	2433	rBV	1921673	2647963	40.01%	5.341%
53	17.539	2433	2440	2450	rBV	3054570	4311070	65.14%	8.695%
54	18.298	2565	2569	2578	rBV	149325	236545	3.57%	0.477%
55	18.375	2579	2582	2591	rVB	26498	43225	0.65%	0.087%
56	19.339	2743	2746	2752	rVB3	43386	56858	0.86%	0.115%
57	19.410	2755	2758	2765	rVB2	39357	64184	0.97%	0.129%
58	19.527	2775	2778	2783	rBV3	66311	95862	1.45%	0.193%
59	19.763	2812	2818	2824	rBV	3987449	5238850	79.15%	10.566%
60	21.192	3058	3061	3069	rBV2	233130	315950	4.77%	0.637%
61	21.521	3112	3117	3126	rVB	2244857	3039125	45.92%	6.129%
62	23.874	3510	3517	3529	rVB2	2604852	5212456	78.76%	10.513%
63	24.039	3539	3545	3555	rVB2	1463232	3000834	45.34%	6.052%




Sum of corrected areas: 49582345

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032223\
Data File : BP014260.D
Acq On : 23 Mar 2023 16:25
Operator : CG/JU
Sample : 02010-02
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB945

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

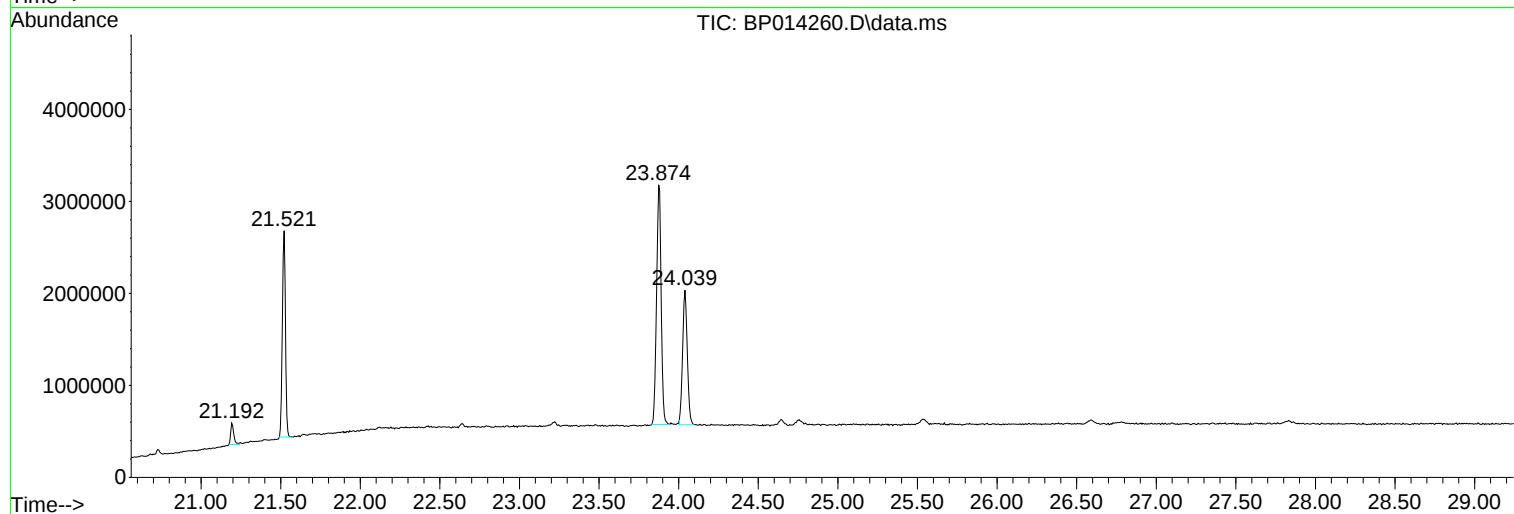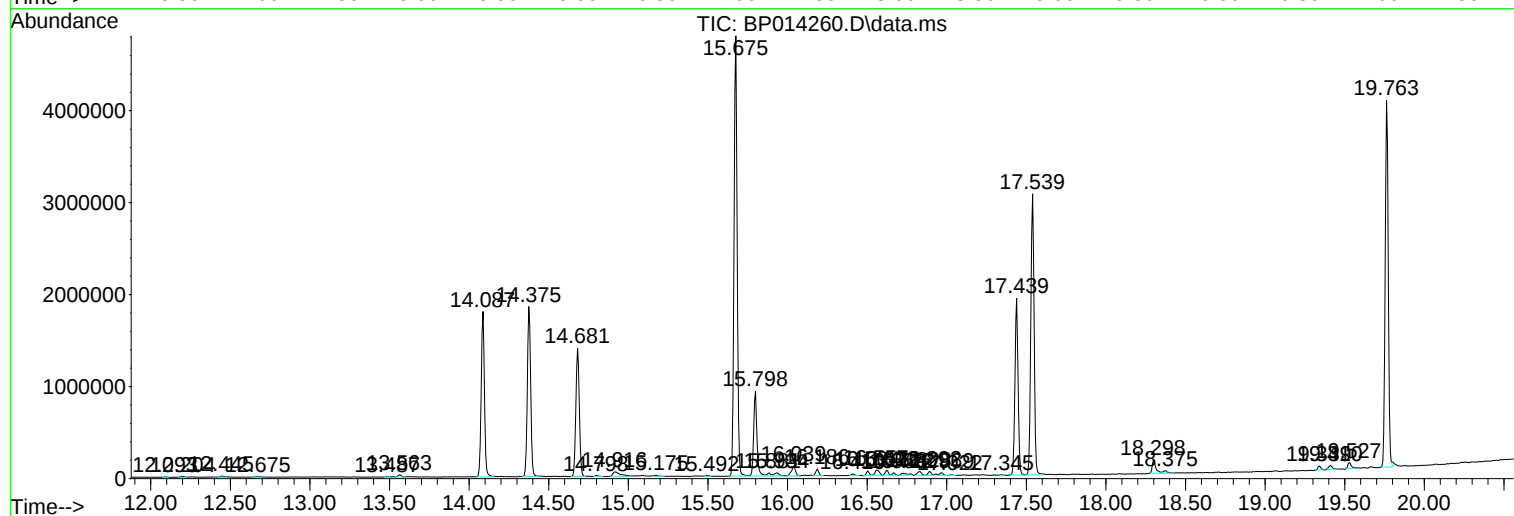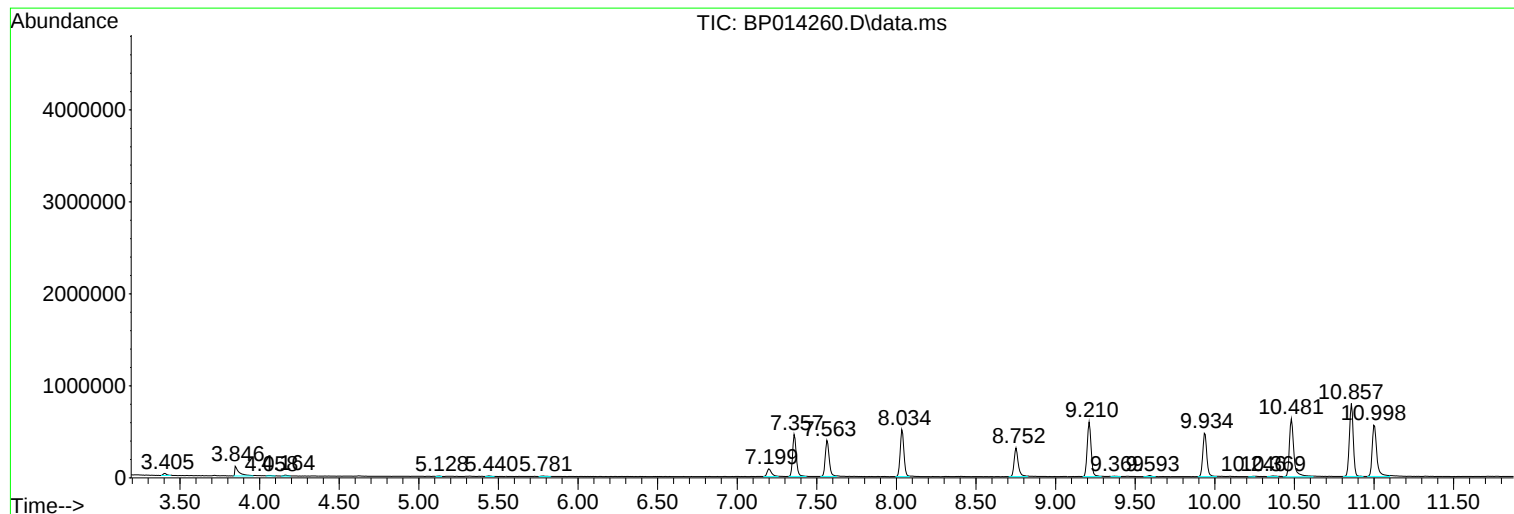

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032223\
Data File : BP014260.D
Acq On : 23 Mar 2023 16:25
Operator : CG/JU
Sample : 02010-02
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB945










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Trichloroacetic acid, hexad... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
21.192	2.08 ng/ul	315950	Chrysene-d12	21.522

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Trichloroacetic acid, hexadecyl ...	386	C18H33Cl3O2	074339-54-1	94
2			Pentafluoropropionic acid, penta...	374	C18H31F5O2	959092-08-1	94
3			Heptafluorobutyric acid, pentade...	424	C19H31F7O2	959261-23-5	94
4			E-14-Hexadecenal	238	C16H30O	330207-53-9	92
5			1-Hexacosene	364	C26H52	018835-33-1	91

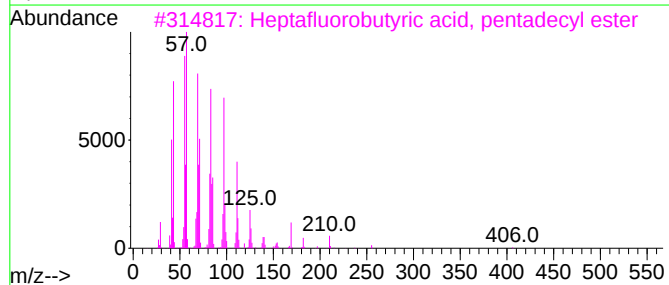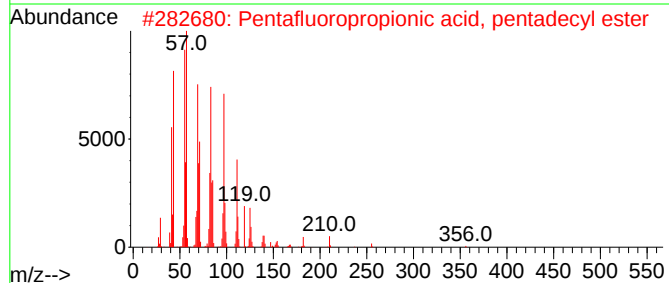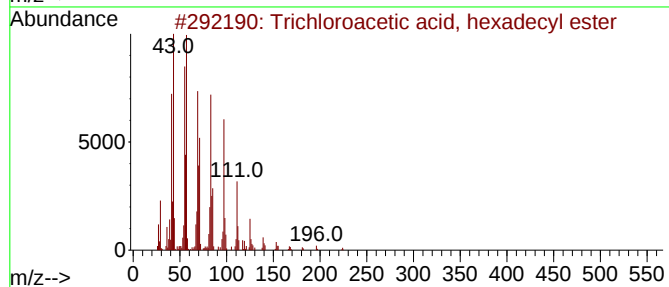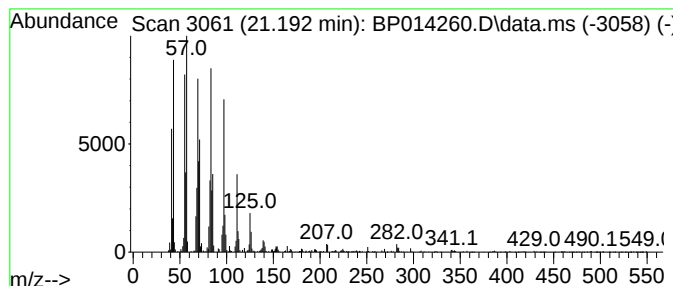

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032223\
Data File : BP014260.D
Acq On : 23 Mar 2023 16:25
Operator : CG/JU
Sample : 02010-02
Misc :
ALS Vial : 40 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
CB945

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Trichloroacetic...	21.192	2.1	ng/ul	315950	5	21.522	3039130	20.0