

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032223\
 Data File : BP014264.D
 Acq On : 23 Mar 2023 19:17
 Operator : CG/JU
 Sample : PB151603BL
 Misc :
 ALS Vial : 44 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK603

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
 Title : SVOA CALIBRATION

Signal : TIC: BP014264.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.405	33	37	46	rVB	47410	67334	1.10%	0.118%
2	3.834	108	110	125	rBV	574527	976963	15.99%	1.709%
3	4.164	162	166	172	rVB2	10163	17691	0.29%	0.031%
4	7.193	674	681	700	rBV	787812	1337894	21.90%	2.341%
5	7.357	703	709	719	rBV	639958	1021003	16.71%	1.786%
6	7.563	737	744	762	rBV	791732	1302177	21.32%	2.278%
7	8.034	814	824	838	rBV	598809	976886	15.99%	1.709%
8	8.746	938	945	961	rBV	988590	1714389	28.07%	2.999%
9	9.210	1015	1024	1041	rBV	835724	1387723	22.72%	2.428%
10	9.934	1139	1147	1160	rBV	707643	1218268	19.94%	2.131%
11	10.481	1232	1240	1268	rBV	907952	1802235	29.50%	3.153%
12	10.857	1296	1304	1316	rBV	885352	1493189	24.44%	2.612%
13	10.998	1319	1328	1344	rBV	941686	1839620	30.12%	3.218%
14	12.451	1569	1575	1583	rBV2	15293	31559	0.52%	0.055%
15	13.563	1759	1764	1768	rBV5	9880	15231	0.25%	0.027%
16	13.657	1775	1780	1786	rBV6	4276	8760	0.14%	0.015%
17	14.087	1846	1853	1868	rBV	2199537	3090465	50.59%	5.407%
18	14.375	1893	1902	1918	rBV	2398987	3445703	56.41%	6.028%
19	14.681	1947	1954	1965	rBV	1567722	2304524	37.73%	4.032%
20	14.887	1982	1989	2017	rBV	668505	1490875	24.41%	2.608%
21	15.675	2116	2123	2135	rBV	3232024	4464325	73.08%	7.810%
22	15.798	2138	2144	2161	rVV	1049275	1589662	26.02%	2.781%
23	15.916	2161	2164	2169	rVB4	15047	23912	0.39%	0.042%
24	17.439	2416	2423	2432	rBV	2078727	2941406	48.15%	5.146%
25	17.539	2433	2440	2455	rVV	3591811	5130641	83.99%	8.976%
26	18.080	2528	2532	2537	rBV8	4095	8090	0.13%	0.014%
27	19.339	2742	2746	2752	rBV2	49349	80628	1.32%	0.141%
28	19.410	2755	2758	2762	rVV	39088	51289	0.84%	0.090%
29	19.763	2812	2818	2829	rBV	4631965	6108607	100.00%	10.687%
30	21.521	3112	3117	3125	rBV	2291927	3191223	52.24%	5.583%
31	23.874	3510	3517	3533	rBV2	2539691	5265598	86.20%	9.212%
32	24.039	3539	3545	3554	rVB2	1371991	2761457	45.21%	4.831%




Sum of corrected areas: 57159327

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032223\
Data File : BP014264.D
Acq On : 23 Mar 2023 19:17
Operator : CG/JU
Sample : PB151603BL
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK603

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

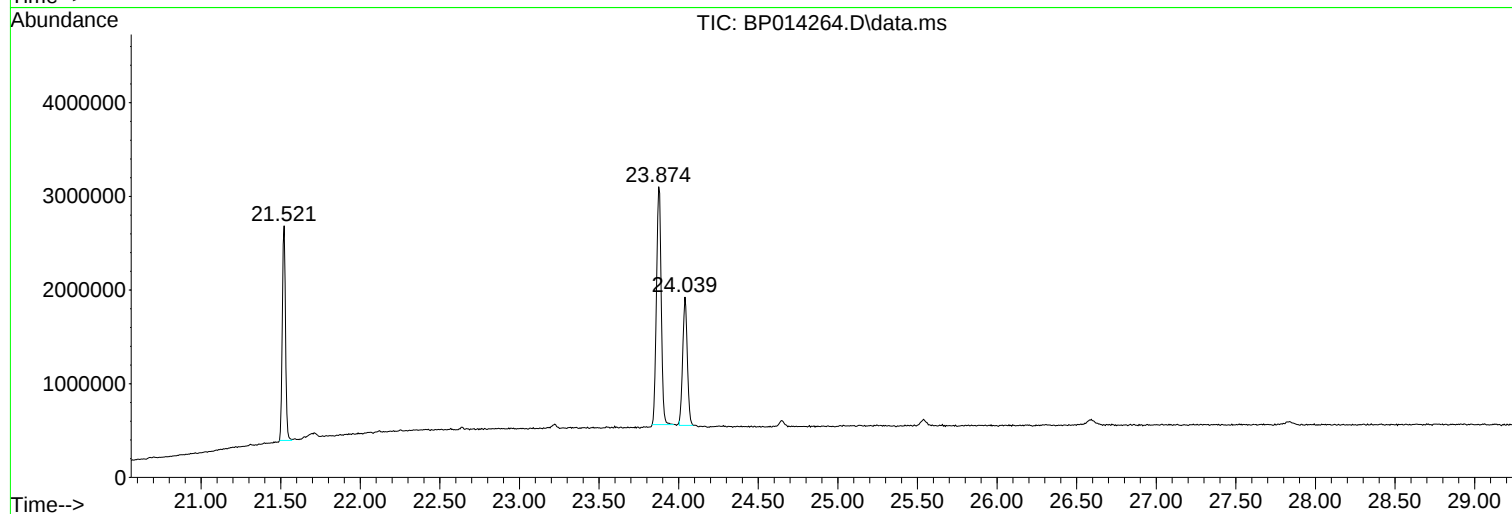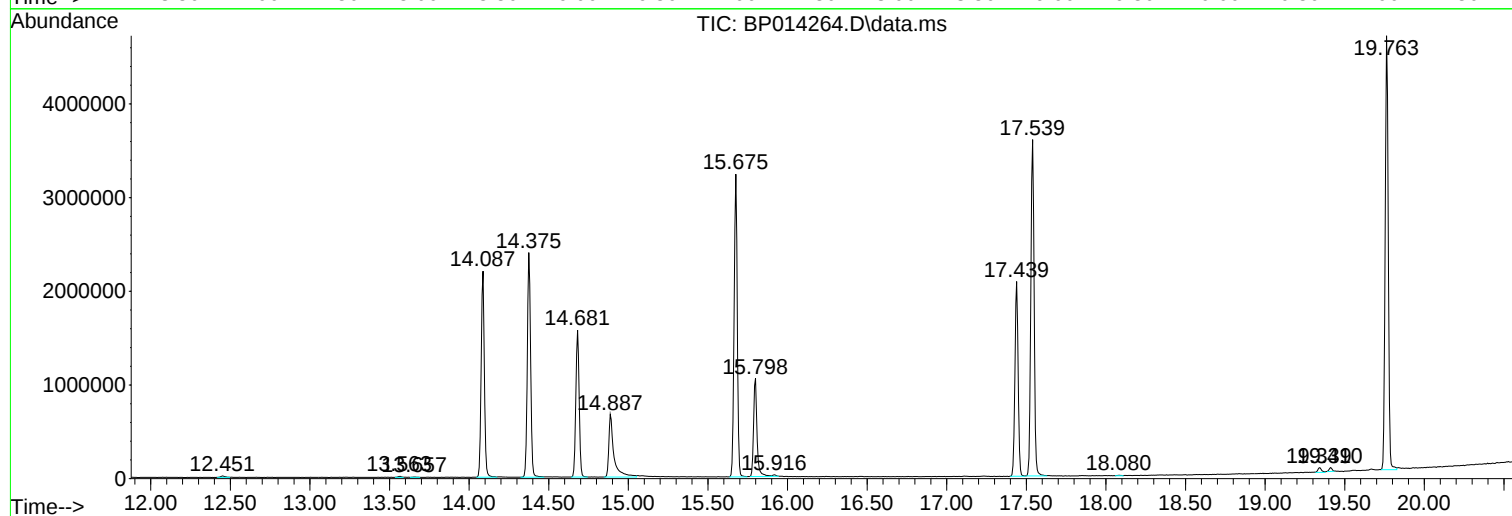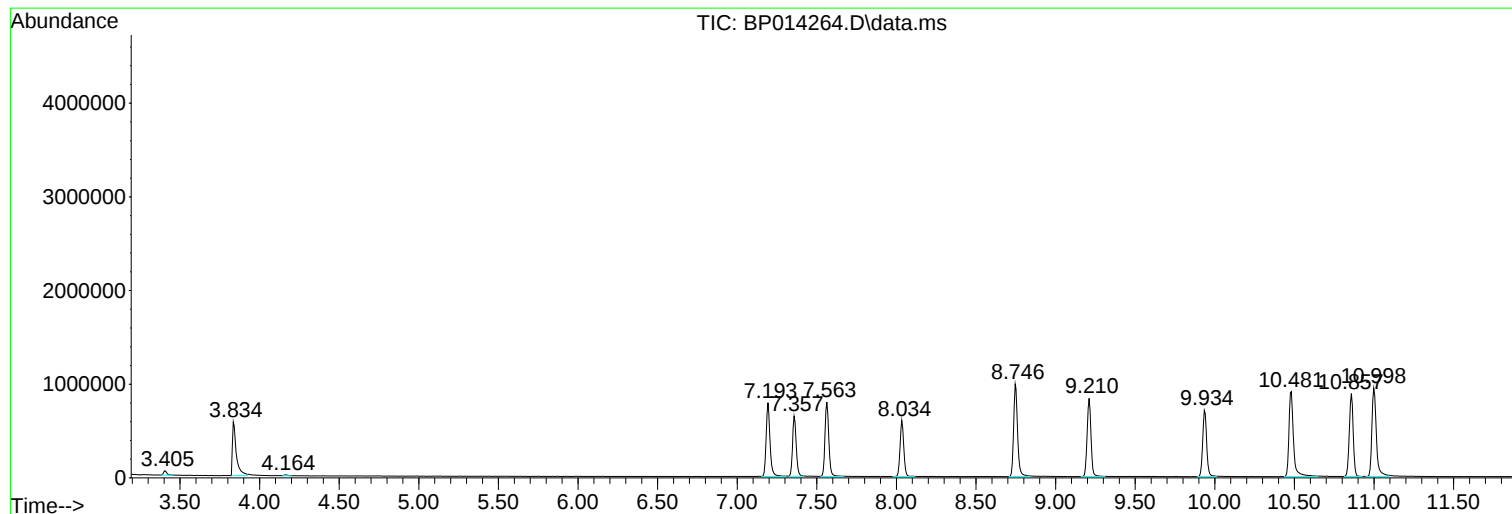

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032223\
Data File : BP014264.D
Acq On : 23 Mar 2023 19:17
Operator : CG/JU
Sample : PB151603BL
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK603

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032223\
Data File : BP014264.D
Acq On : 23 Mar 2023 19:17
Operator : CG/JU
Sample : PB151603BL
Misc :
ALS Vial : 44 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK603

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------