

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032223\
 Data File : BP014270.D
 Acq On : 23 Mar 2023 22:42
 Operator : CG/JU
 Sample : PB151571BL
 Misc :
 ALS Vial : 50 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK571

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
 Title : SVOA CALIBRATION

Signal : TIC: BP014270.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.222	3	6	8	rBV	48192	48927	1.83%	0.365%
2	3.252	8	11	13	rVV	20427	22289	0.83%	0.166%
3	3.275	13	15	17	rVV	32601	29888	1.12%	0.223%
4	3.311	17	21	31	rVB	1080859	1174009	43.83%	8.766%
5	3.664	77	81	87	rVB	37773	43616	1.63%	0.326%
6	3.758	95	97	102	rVB6	2904	3512	0.13%	0.026%
7	4.158	161	165	170	rVB	13539	16928	0.63%	0.126%
8	5.681	419	424	428	rVB8	1458	2867	0.11%	0.021%
9	8.034	817	824	846	rBV	575604	1013462	37.84%	7.568%
10	8.175	846	848	858	rVB	2359	4981	0.19%	0.037%
11	8.557	905	913	916	rBV9	1364	3458	0.13%	0.026%
12	10.857	1296	1304	1328	rBV	718332	1356567	50.65%	10.130%
13	14.045	1841	1846	1849	rBV7	1663	3429	0.13%	0.026%
14	14.410	1904	1908	1909	rBV4	2272	2909	0.11%	0.022%
15	14.681	1946	1954	1972	rBV	1240468	1960798	73.21%	14.641%
16	15.051	2012	2017	2021	rBV7	1569	3768	0.14%	0.028%
17	16.151	2199	2204	2205	rBV4	2068	2796	0.10%	0.021%
18	17.222	2383	2386	2389	rBV5	4593	7204	0.27%	0.054%
19	17.439	2416	2423	2445	rBV	1698932	2609525	97.43%	19.485%
20	21.515	3111	3116	3127	rBV	1962009	2678249	100.00%	19.999%
21	24.033	3538	3544	3560	rVB2	1129494	2402972	89.72%	17.943%




Sum of corrected areas: 13392154

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032223\
Data File : BP014270.D
Acq On : 23 Mar 2023 22:42
Operator : CG/JU
Sample : PB151571BL
Misc :
ALS Vial : 50 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK571

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

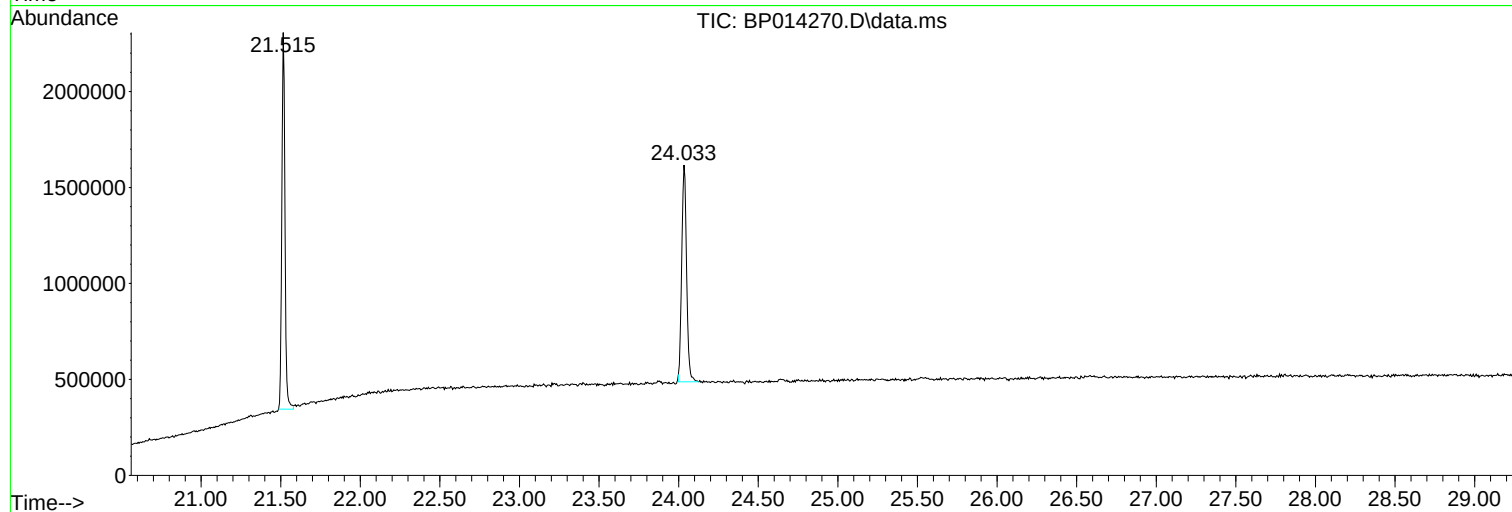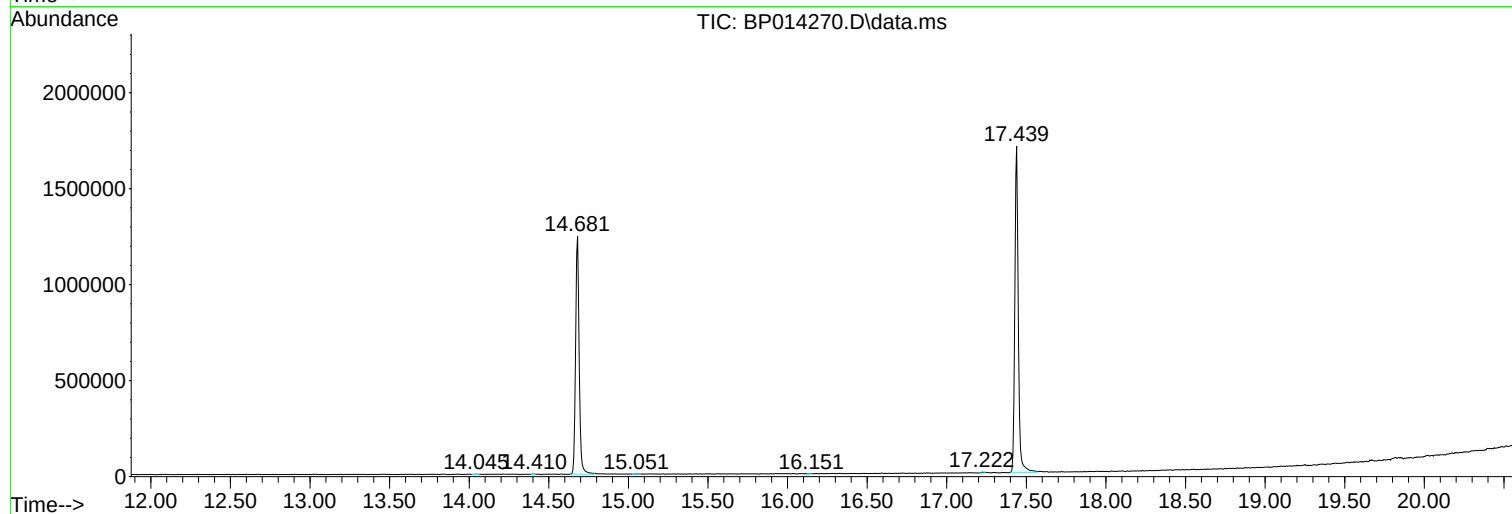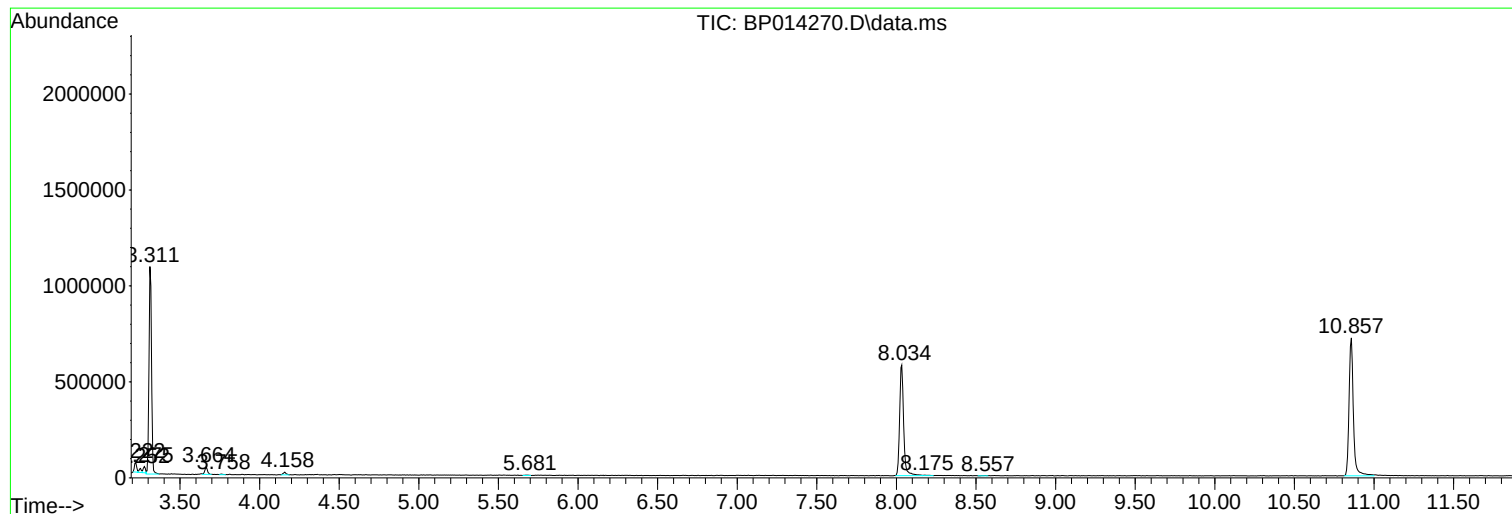

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032223\
Data File : BP014270.D
Acq On : 23 Mar 2023 22:42
Operator : CG/JU
Sample : PB151571BL
Misc :
ALS Vial : 50 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK571










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Straight-Chai... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.311	23.17 ng/ul	1174010	1,4-Dichlorobenzene-d4	8.034

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	Heptane			100	C7H16	000142-82-5	94
2	Heptane			100	C7H16	000142-82-5	94
3	Heptane			100	C7H16	000142-82-5	91
4	Heptane			100	C7H16	000142-82-5	87
5	Pentane, 2-methyl-			86	C6H14	000107-83-5	47

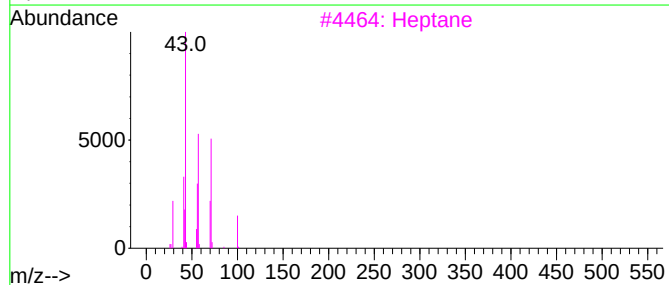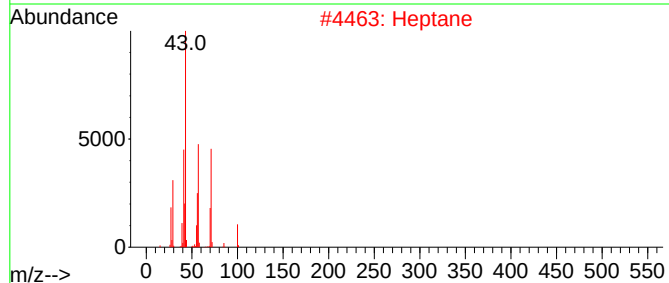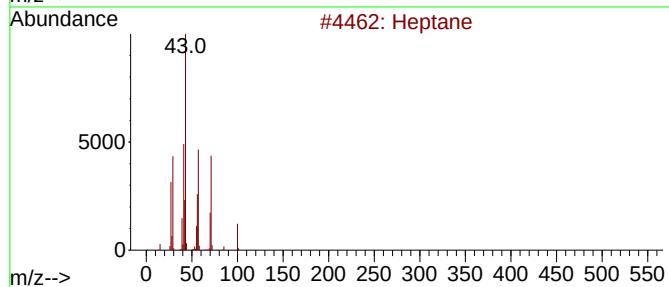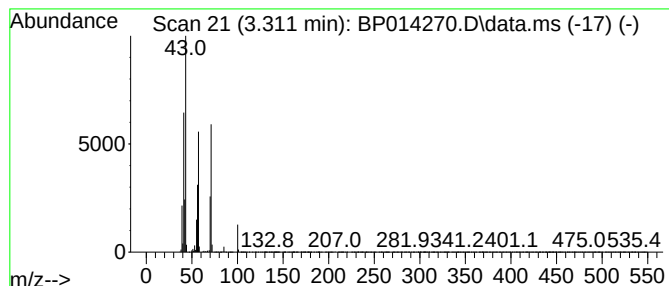

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032223\
Data File : BP014270.D
Acq On : 23 Mar 2023 22:42
Operator : CG/JU
Sample : PB151571BL
Misc :
ALS Vial : 50 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK571

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: S...	3.311	23.2	ng/u1	1174010	1	8.034	1013460	20.0