

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032223\
 Data File : BP014274.D
 Acq On : 24 Mar 2023 00:59
 Operator : CG/JU
 Sample : PB151570BL
 Misc :
 ALS Vial : 54 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK570

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
 Title : SVOA CALIBRATION

Signal : TIC: BP014274.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.217	3	5	7	rVB2	20650	17973	0.64%	0.170%
2	3.240	7	9	12	rVV3	9005	10214	0.37%	0.097%
3	3.270	12	14	16	rVV	16940	14844	0.53%	0.140%
4	3.305	16	20	36	rVB	517409	663139	23.71%	6.274%
5	3.664	77	81	89	rVB2	18636	25892	0.93%	0.245%
6	3.752	94	96	101	rVB6	3055	3346	0.12%	0.032%
7	4.158	161	165	168	rBV2	5563	8717	0.31%	0.082%
8	7.087	661	663	668	rBV6	1471	2815	0.10%	0.027%
9	8.034	815	824	836	rBV	295987	534013	19.10%	5.052%
10	9.081	998	1002	1007	rVB7	1862	3093	0.11%	0.029%
11	10.857	1297	1304	1320	rBV	376864	727418	26.01%	6.882%
12	11.281	1373	1376	1380	rBV6	2043	3185	0.11%	0.030%
13	14.681	1946	1954	1969	rBV	728861	1184424	42.35%	11.206%
14	15.981	2171	2175	2178	rBV6	1626	3122	0.11%	0.030%
15	17.439	2416	2423	2438	rBV	1113330	1844175	65.95%	17.448%
16	17.992	2513	2517	2518	rBV4	3020	4262	0.15%	0.040%
17	19.663	2798	2801	2805	rBV5	26558	37308	1.33%	0.353%
18	21.516	3111	3116	3127	rBV	1902818	2685015	96.01%	25.404%
19	24.033	3538	3544	3555	rVB2	1279247	2796463	100.00%	26.458%




Sum of corrected areas: 10569418

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032223\
Data File : BP014274.D
Acq On : 24 Mar 2023 00:59
Operator : CG/JU
Sample : PB151570BL
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK570

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

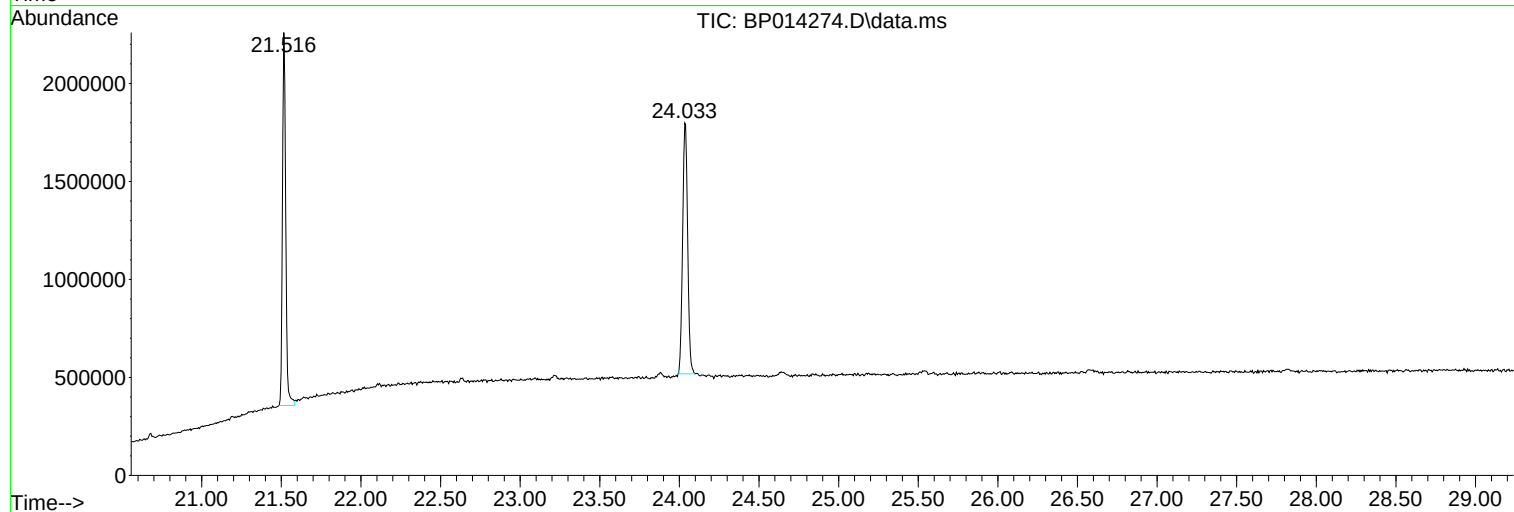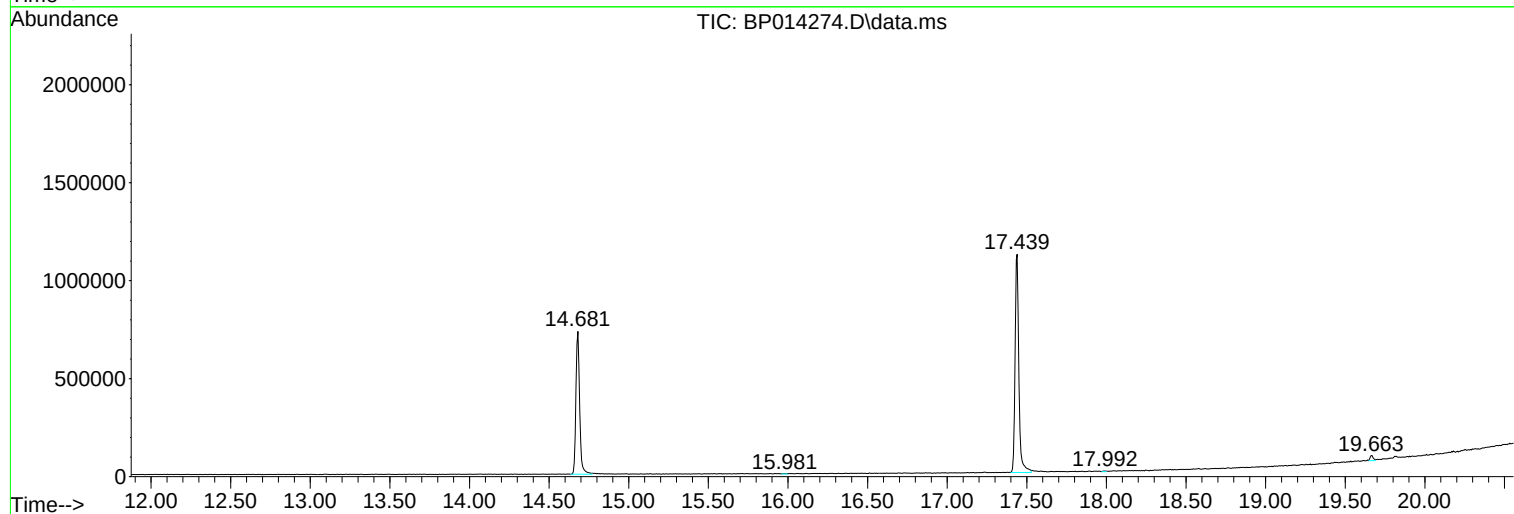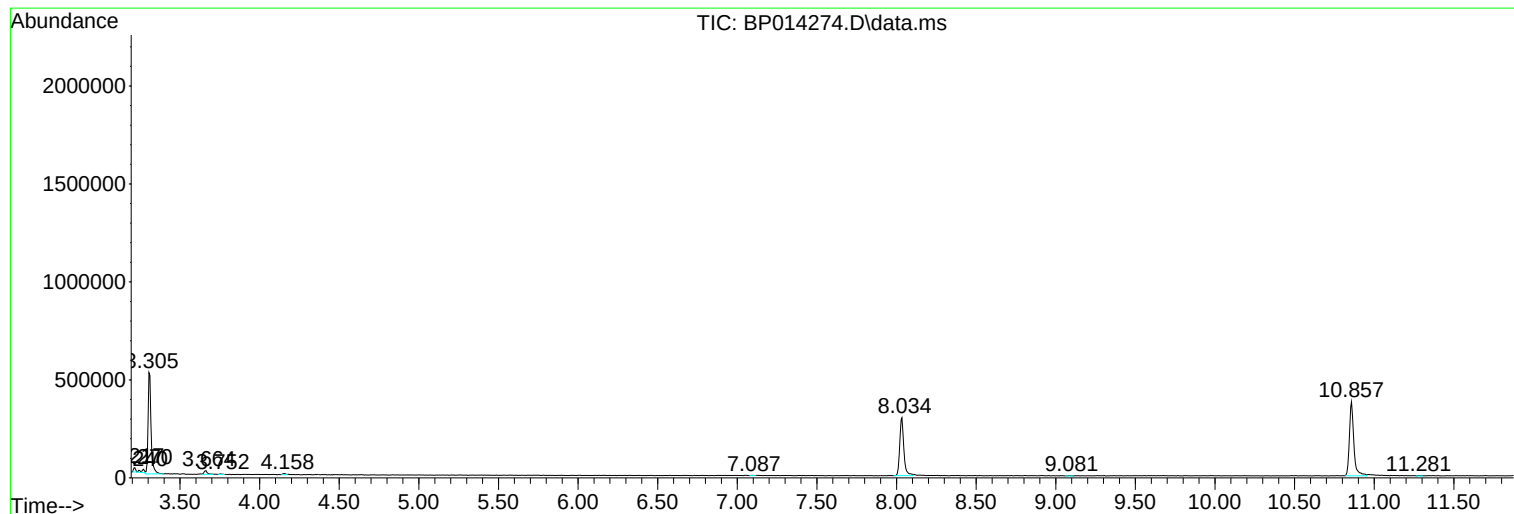

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032223\
Data File : BP014274.D
Acq On : 24 Mar 2023 00:59
Operator : CG/JU
Sample : PB151570BL
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK570










Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 (DEL) Alkane: Straight-Chai... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
3.305	24.84 ng/ul	663139	1,4-Dichlorobenzene-d4	8.034

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Heptane	100	C7H16	000142-82-5	94
2			Heptane	100	C7H16	000142-82-5	91
3			Heptane	100	C7H16	000142-82-5	90
4			Heptane	100	C7H16	000142-82-5	87
5			1-Hexene, 3,4,5-trimethyl-	126	C9H18	056728-10-0	52

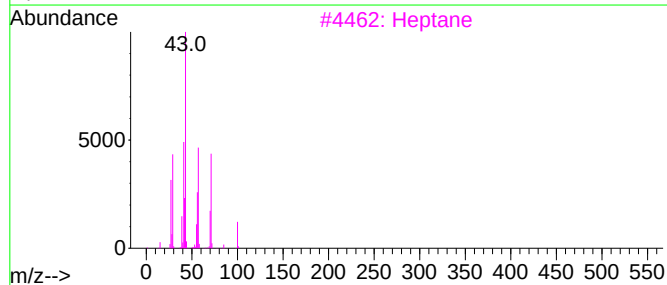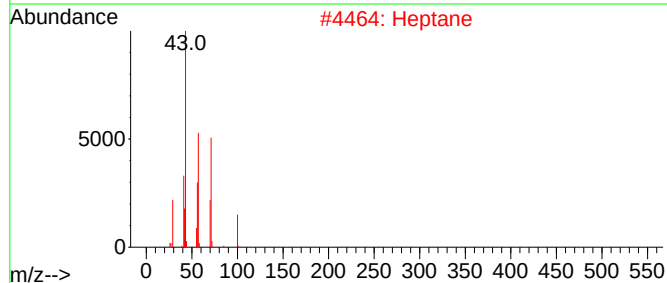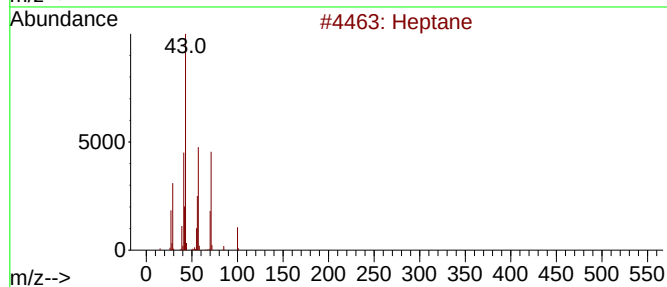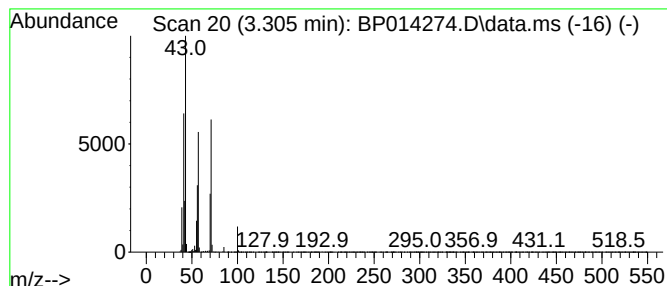

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032223\
Data File : BP014274.D
Acq On : 24 Mar 2023 00:59
Operator : CG/JU
Sample : PB151570BL
Misc :
ALS Vial : 54 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK570

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP030723.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST0.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
(DEL) Alkane: S...	3.305	24.8	ng/u1	663139	1	8.034	534013	20.0