




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032224\
Data File : BP019964.D
Acq On : 22 Mar 2024 20:41
Operator : MA/JU
Sample : P1813-11
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E0LX9

Manual IntegrationsAPPROVED

Quant Time: Mar 22 23:03:32 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032224.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 22 22:40:53 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 03/26/2024
Supervised By :mohammad ahmed 03/26/2024

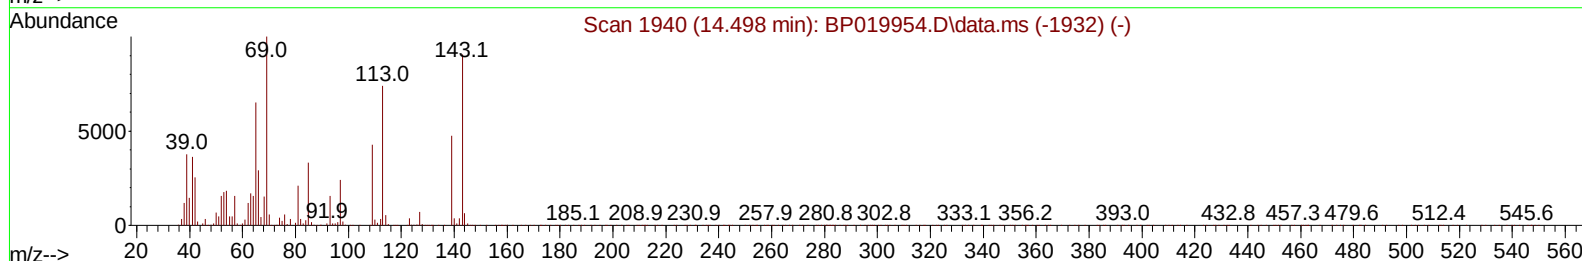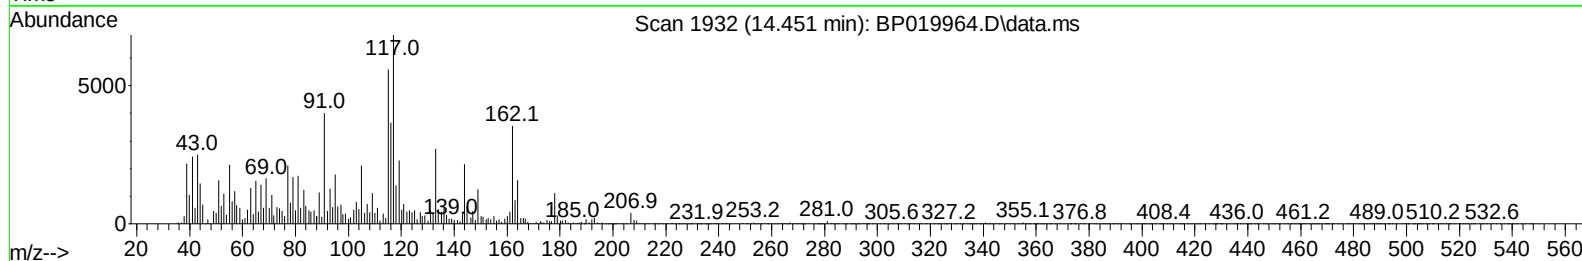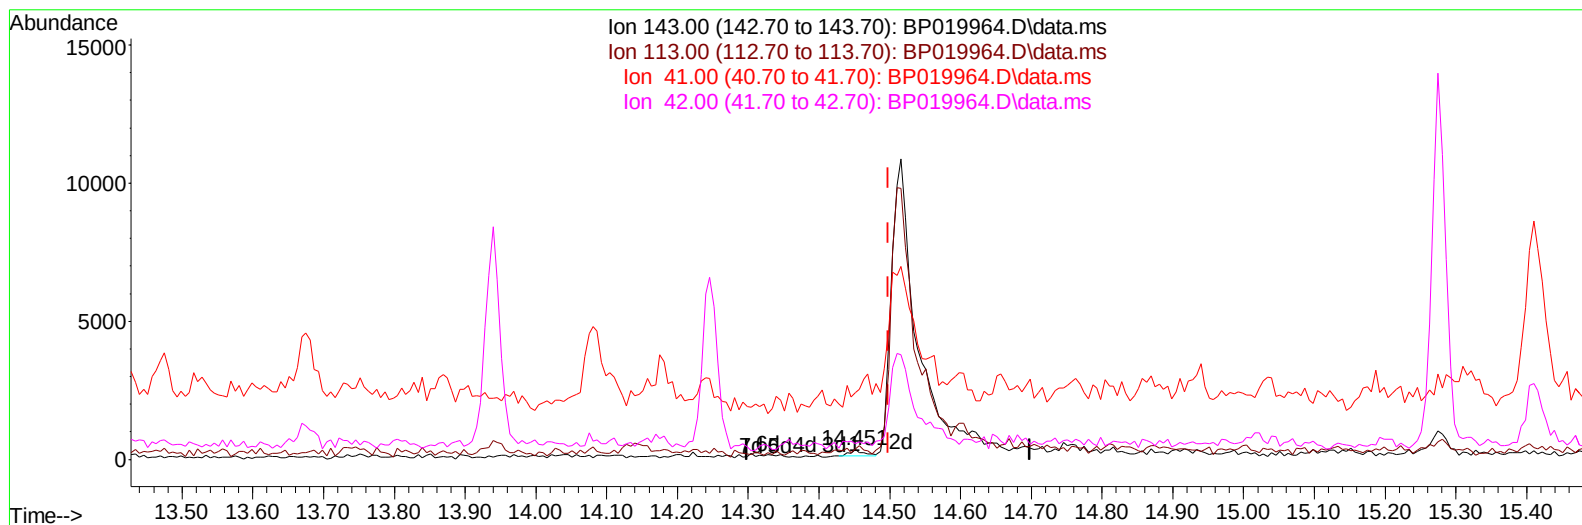

TIC: BP019964.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.451min (-0.047) 0.11 ng/u1

response 328

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	81.50	105.29#
41.00	40.90	678.27#
42.00	28.50	158.50#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032224\
Data File : BP019964.D
Acq On : 22 Mar 2024 20:41
Operator : MA/JU
Sample : P1813-11
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E0LX9

Manual IntegrationsAPPROVED

Quant Time: Mar 22 23:03:32 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032224.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 22 22:40:53 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 03/26/2024
Supervised By :mohammad ahmed 03/26/2024

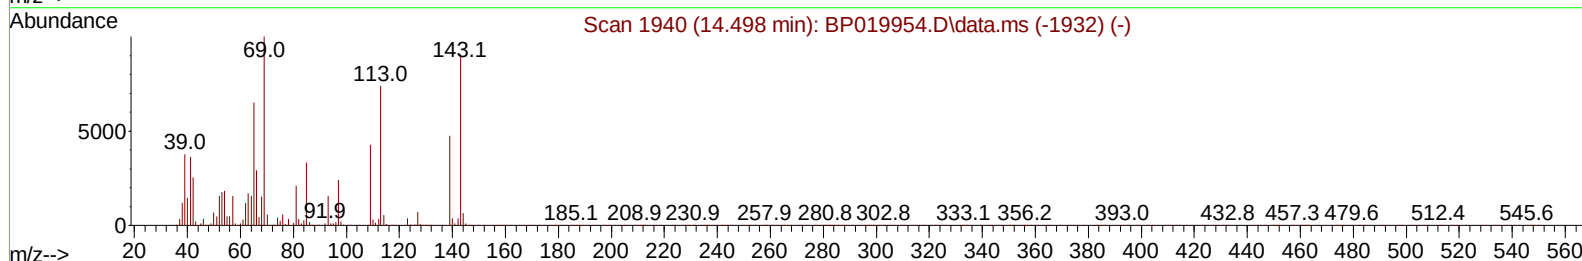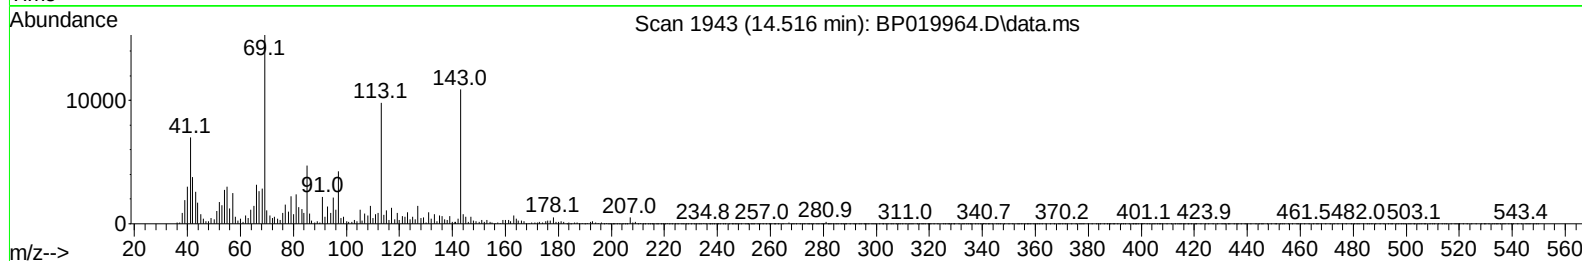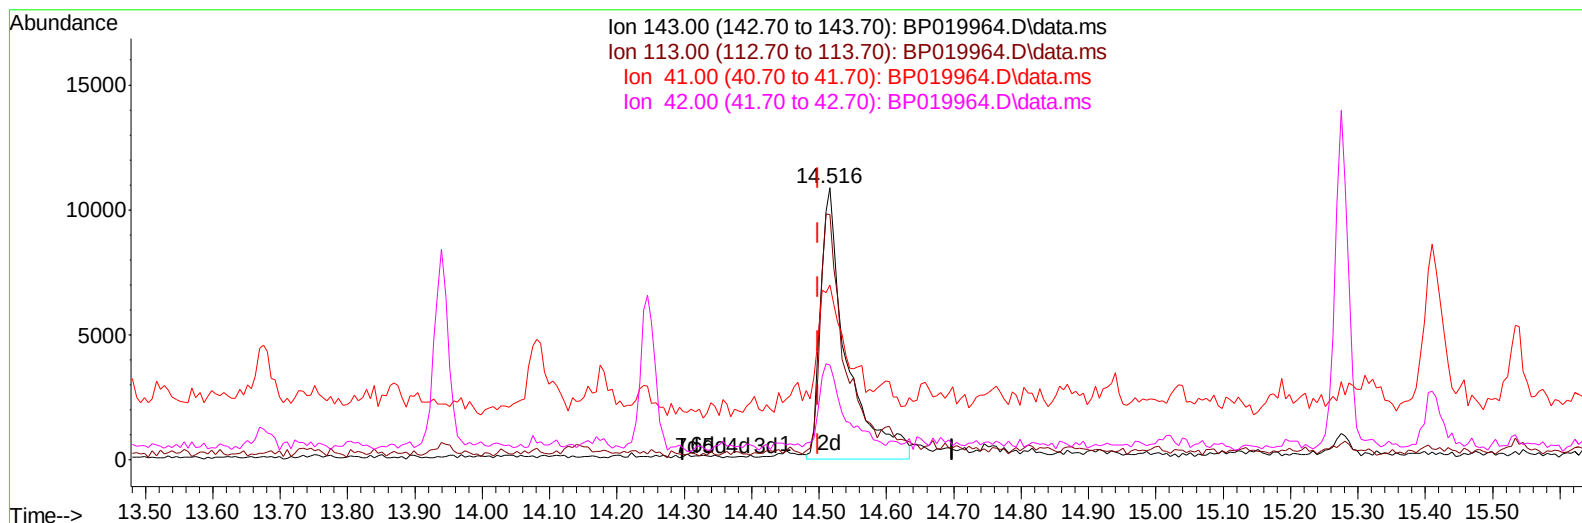

TIC: BP019964.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.516min (+ 0.018) 9.33 ng/ul m

response 28871

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	81.50	90.22
41.00	40.90	64.27#
42.00	28.50	34.90#

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032224\
 Data File : BP019964.D
 Acq On : 22 Mar 2024 20:41
 Operator : MA/JU
 Sample : P1813-11
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 E0LX9

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 03/26/2024
 Supervised By :mohammad ahmed 03/26/2024

Quant Time: Mar 22 23:23:54 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032224.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Mar 22 22:40:53 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.622	152	103848	20.000	ng/ul	0.00
20) Naphthalene-d8	10.369	136	430613	20.000	ng/ul	-0.01
38) Acenaphthene-d10	14.245	164	280661	20.000	ng/ul	-0.02
64) Phenanthrene-d10	17.081	188	606379	20.000	ng/ul	-0.01
79) Chrysene-d12	21.551	240	584138	20.000	ng/ul	0.00
88) Perylene-d12	24.839	264	695954	20.000	ng/ul	-0.02
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.246	96	14965	6.314	ng/uL	0.00
4) Pyridine-d5	3.646	84	93094	13.008	ng/ul	0.00
7) Phenol-d5	6.811	99	76003	8.678	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.969	67	230742	40.437	ng/ul	-0.01
11) 2-Chlorophenol-d4	7.163	132	195513	31.083	ng/ul	0.00
15) 4-Methylphenol-d8	8.322	113	137807	20.337	ng/ul	0.00
21) Nitrobenzene-d5	8.769	128	131587	39.868	ng/ul	0.00
24) 2-Nitrophenol-d4	9.475	143	138608	37.534	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.010	165	240932	35.724	ng/ul	0.00
31) 4-Chloroaniline-d4	10.528	131	194382	22.109	ng/ul	0.00
46) Dimethylphthalate-d6	13.675	166	828667	42.112	ng/ul	0.00
49) Acenaphthylene-d8	13.940	160	933483	40.610	ng/ul	-0.01
54) 4-Nitrophenol-d4	14.516	143	28871m	9.333	ng/ul	0.02
60) Fluorene-d10	15.275	176	705364	42.080	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.410	200	128598	35.429	ng/ul	-0.02
73) Anthracene-d10	17.192	188	1105532	41.187	ng/ul	0.00
81) Pyrene-d10	19.586	212	1369008	39.945	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.610	264	1417531	42.397	ng/ul	-0.02

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032224\
Data File : BP019964.D
Acq On : 22 Mar 2024 20:41
Operator : MA/JU
Sample : P1813-11
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E0LX9

Manual IntegrationsAPPROVED

Quant Time: Mar 22 23:23:54 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032224.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 22 22:40:53 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 03/26/2024
Supervised By :mohammad ahmed 03/26/2024

