




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032224\
Data File : BP019967.D
Acq On : 22 Mar 2024 22:49
Operator : MA/JU
Sample : P1813-14
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E0LY2

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 03/26/2024
Supervised By :mohammad ahmed 03/26/2024

Quant Time: Mar 22 23:30:17 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032224.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 22 22:40:53 2024
Response via : Initial Calibration

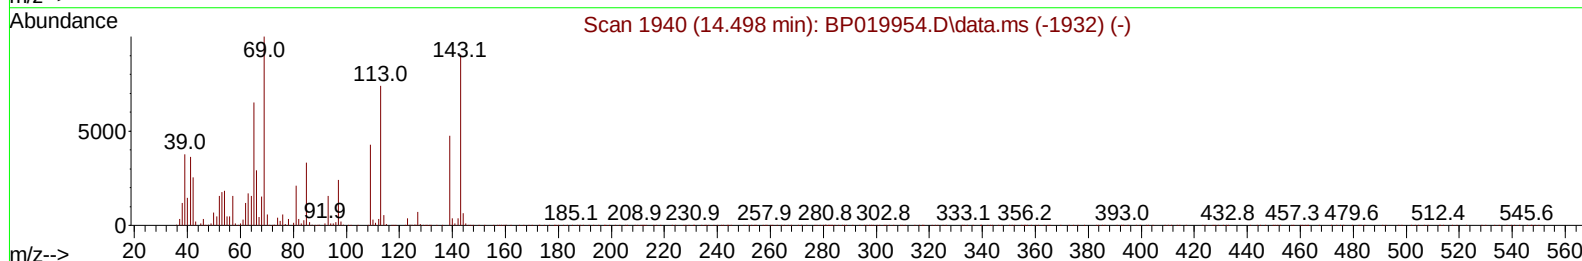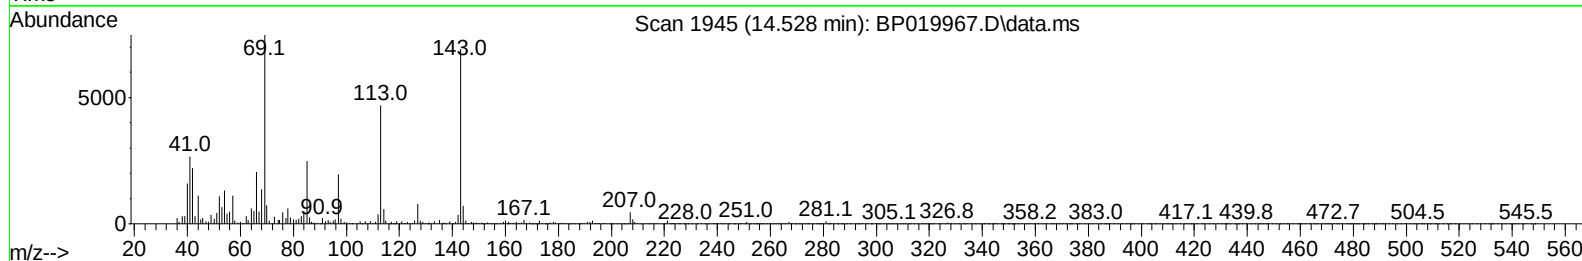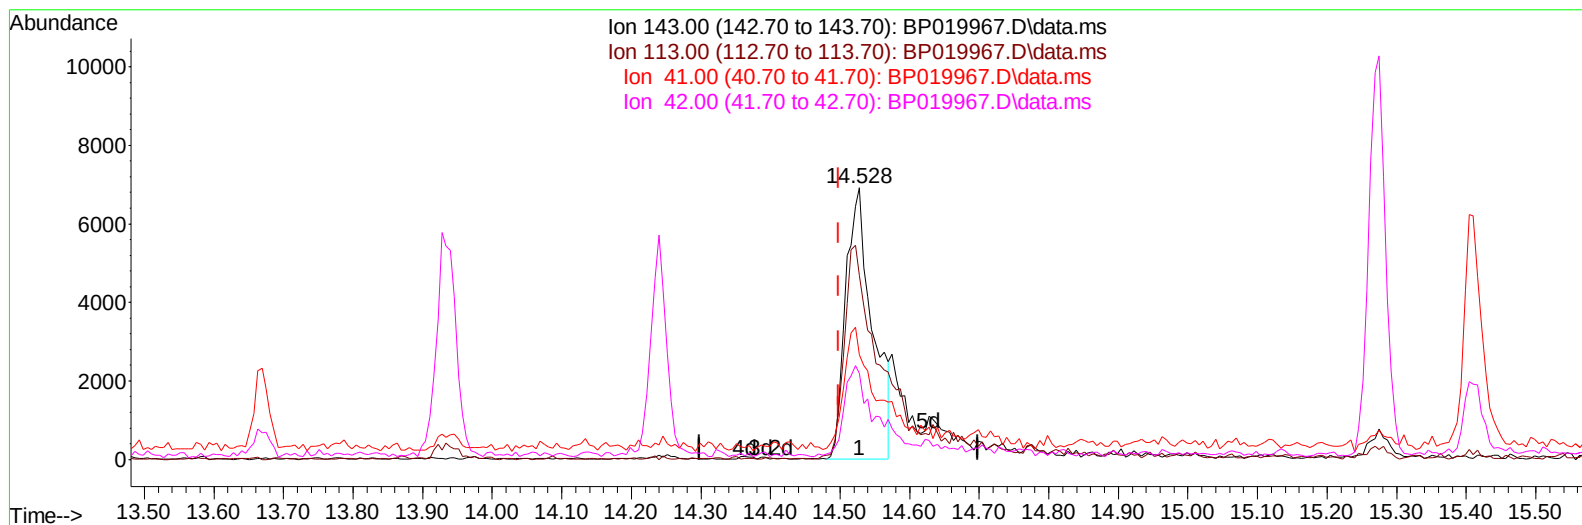

TIC: BP019967.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.528min (+ 0.030) 5.60 ng/ul

response 18470

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	81.50	67.73
41.00	40.90	38.45
42.00	28.50	31.74




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032224\
Data File : BP019967.D
Acq On : 22 Mar 2024 22:49
Operator : MA/JU
Sample : P1813-14
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E0LY2

Manual IntegrationsAPPROVED

Quant Time: Mar 22 23:30:17 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032224.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 22 22:40:53 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 03/26/2024
Supervised By :mohammad ahmed 03/26/2024

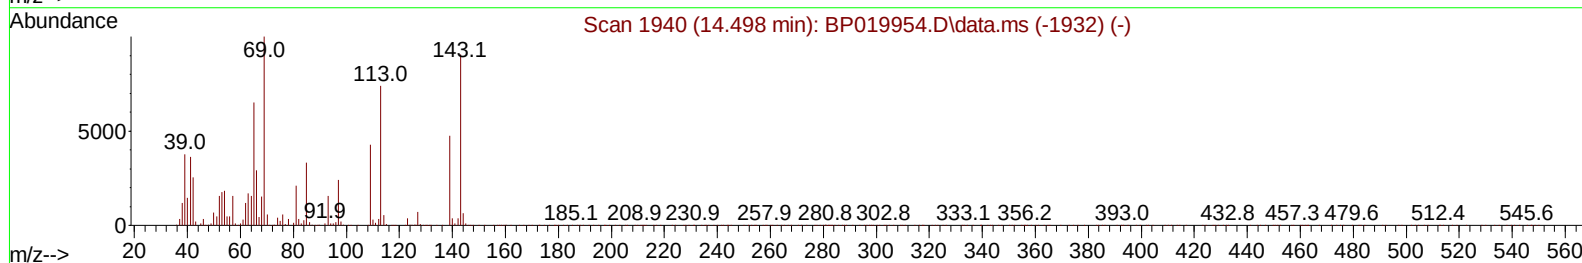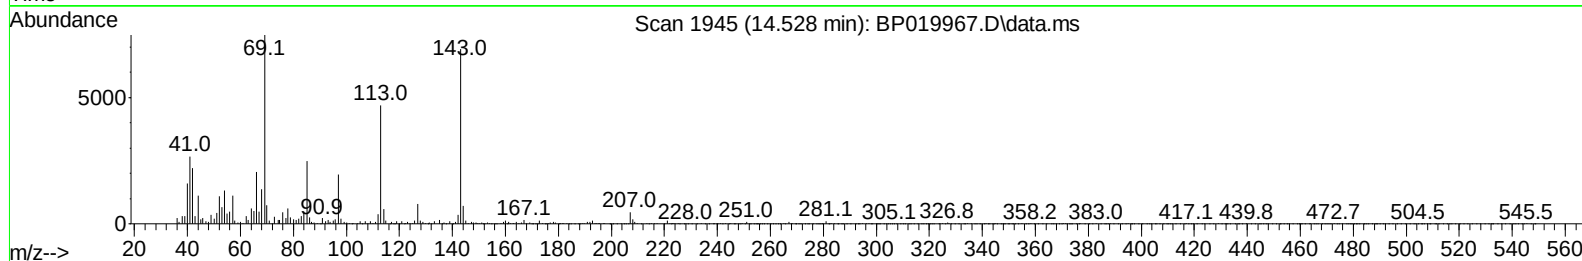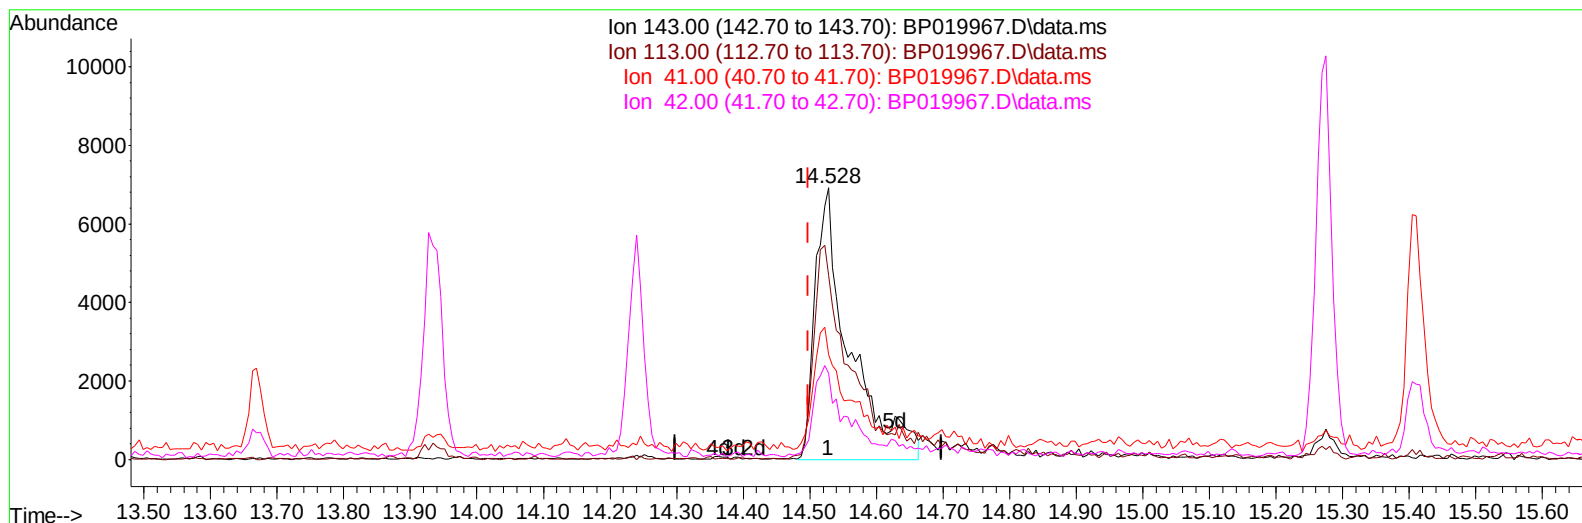

TIC: BP019967.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.528min (+ 0.030) 7.51 ng/ul m

response 24764

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	81.50	67.73
41.00	40.90	38.45
42.00	28.50	31.74

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032224\
 Data File : BP019967.D
 Acq On : 22 Mar 2024 22:49
 Operator : MA/JU
 Sample : P1813-14
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 E0LY2

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 03/26/2024
 Supervised By :mohammad ahmed 03/26/2024

Quant Time: Mar 22 23:31:02 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032224.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Mar 22 22:40:53 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.622	152	112777	20.000	ng/ul	0.00
20) Naphthalene-d8	10.375	136	460474	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.240	164	299328	20.000	ng/ul	-0.02
64) Phenanthrene-d10	17.069	188	614940	20.000	ng/ul	-0.02
79) Chrysene-d12	21.539	240	558361	20.000	ng/ul	-0.01
88) Perylene-d12	24.827	264	657622	20.000	ng/ul	-0.03
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.246	96	15325	5.954	ng/uL	0.00
4) Pyridine-d5	3.646	84	87950	11.316	ng/ul	0.00
7) Phenol-d5	6.811	99	67932	7.142	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.981	67	208670	33.674	ng/ul	0.00
11) 2-Chlorophenol-d4	7.164	132	175087	25.632	ng/ul	0.00
15) 4-Methylphenol-d8	8.316	113	129131	17.548	ng/ul	0.00
21) Nitrobenzene-d5	8.769	128	119734	33.924	ng/ul	0.00
24) 2-Nitrophenol-d4	9.481	143	128770	32.609	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.010	165	218039	30.233	ng/ul	0.00
31) 4-Chloroaniline-d4	10.522	131	275558	29.309	ng/ul	0.00
46) Dimethylphthalate-d6	13.669	166	835788	39.825	ng/ul	0.00
49) Acenaphthylene-d8	13.934	160	891398	36.360	ng/ul	-0.02
54) 4-Nitrophenol-d4	14.528	143	24764m	7.506	ng/ul	0.03
60) Fluorene-d10	15.275	176	691064	38.655	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.410	200	125886	34.199	ng/ul	-0.02
73) Anthracene-d10	17.175	188	1091941	40.114	ng/ul	-0.01
81) Pyrene-d10	19.563	212	1266109	38.648	ng/ul	-0.02
92) Benzo(a)pyrene-d12	24.604	264	1307313	41.379	ng/ul	-0.03

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032224\
Data File : BP019967.D
Acq On : 22 Mar 2024 22:49
Operator : MA/JU
Sample : P1813-14
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E0LY2

Manual IntegrationsAPPROVED

Quant Time: Mar 22 23:31:02 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032224.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 22 22:40:53 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 03/26/2024
Supervised By :mohammad ahmed 03/26/2024

