




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032224\
Data File : BP019968.D
Acq On : 22 Mar 2024 23:31
Operator : MA/JU
Sample : P1813-15
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E0LY3

Manual IntegrationsAPPROVED

Quant Time: Mar 23 00:19:08 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032224.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 22 22:40:53 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 03/26/2024
Supervised By :mohammad ahmed 03/26/2024

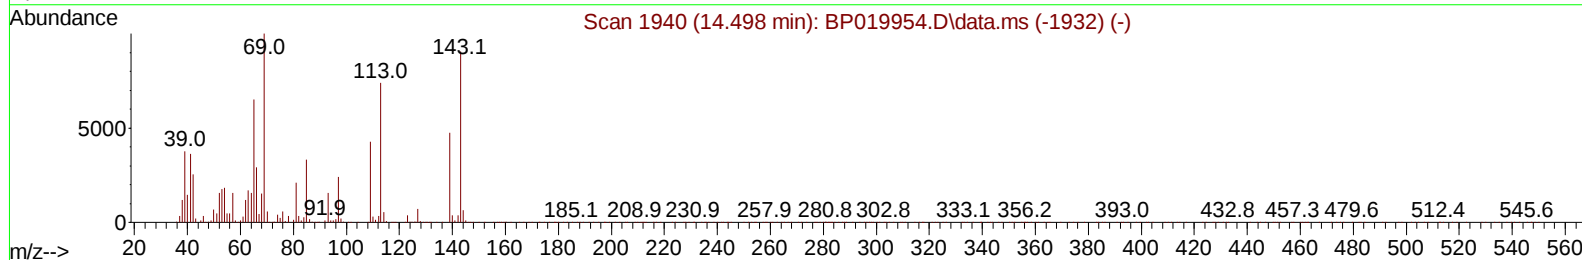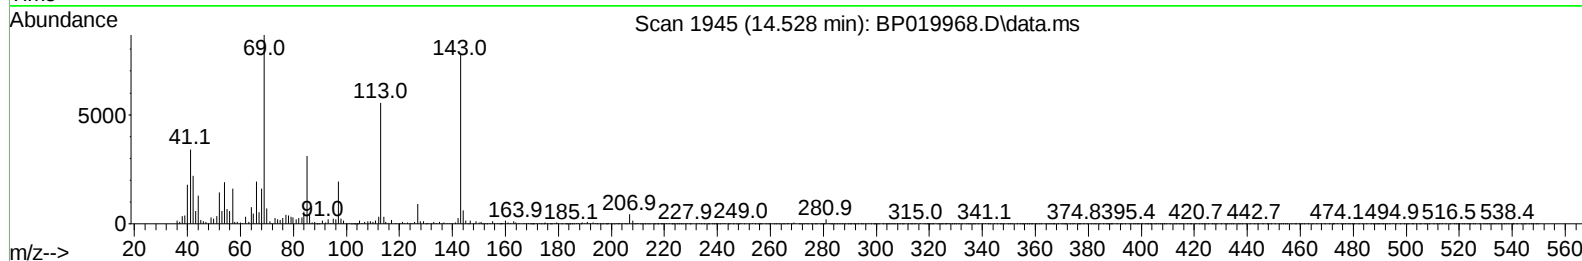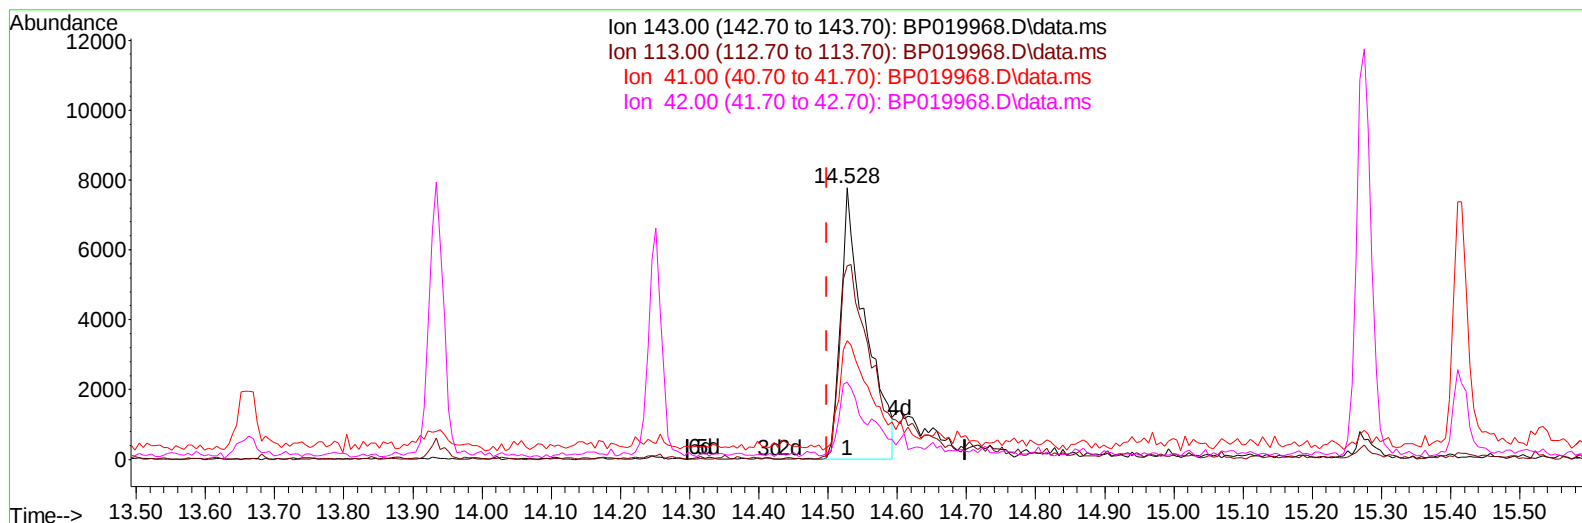

TIC: BP019968.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.528min (+ 0.030) 6.32 ng/u1

response 19239

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	81.50	71.27
41.00	40.90	43.84
42.00	28.50	28.33




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032224\
Data File : BP019968.D
Acq On : 22 Mar 2024 23:31
Operator : MA/JU
Sample : P1813-15
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E0LY3

Manual IntegrationsAPPROVED

Quant Time: Mar 23 00:19:08 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032224.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 22 22:40:53 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 03/26/2024
Supervised By :mohammad ahmed 03/26/2024

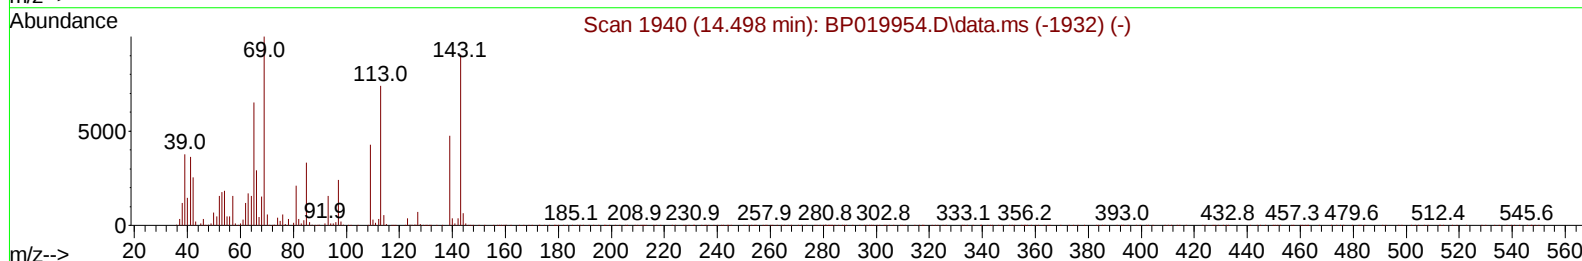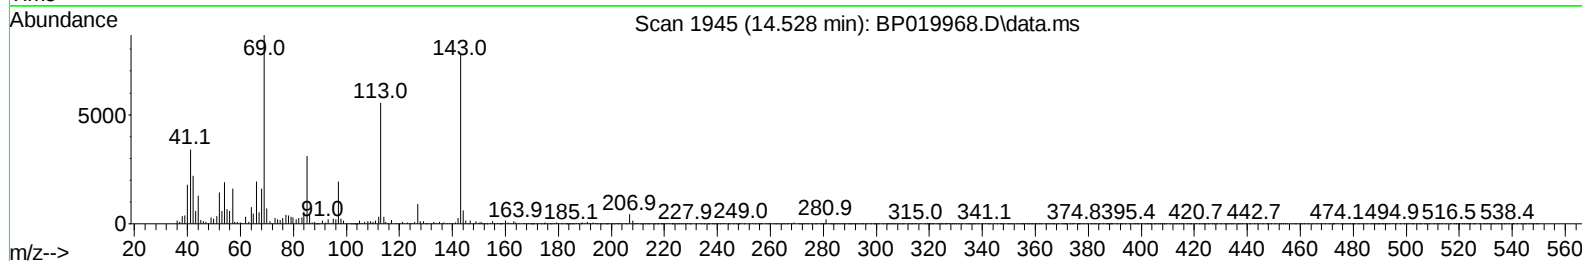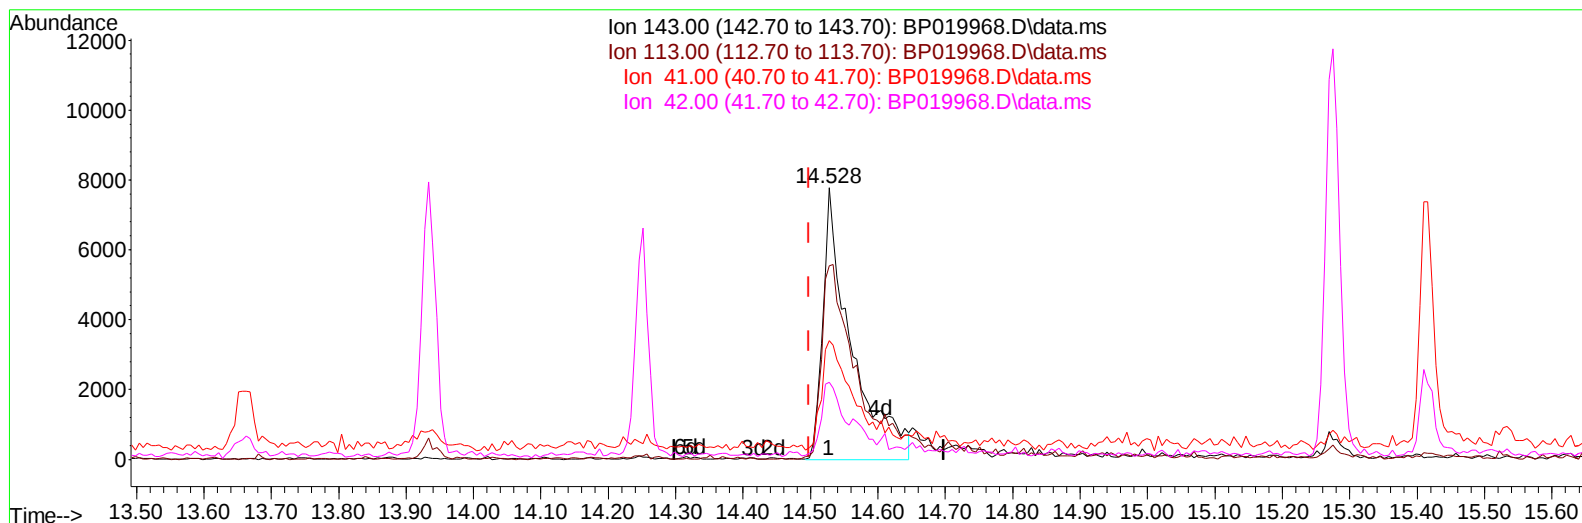

TIC: BP019968.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.528min (+ 0.030) 7.45 ng/ul m

response 22695

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	81.50	71.27
41.00	40.90	43.84
42.00	28.50	28.33

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032224\
 Data File : BP019968.D
 Acq On : 22 Mar 2024 23:31
 Operator : MA/JU
 Sample : P1813-15
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 E0LY3

Manual IntegrationsAPPROVED

Reviewed By :Yogesh Patel 03/26/2024
 Supervised By :mohammad ahmed 03/26/2024

Quant Time: Mar 23 00:20:24 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032224.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Mar 22 22:40:53 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.616	152	105164	20.000	ng/ul	0.00
20) Naphthalene-d8	10.363	136	435621	20.000	ng/ul	-0.02
38) Acenaphthene-d10	14.251	164	276312	20.000	ng/ul	-0.01
64) Phenanthrene-d10	17.069	188	549964	20.000	ng/ul	-0.02
79) Chrysene-d12	21.545	240	464701	20.000	ng/ul	0.00
88) Perylene-d12	24.833	264	544150	20.000	ng/ul	-0.03
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.246	96	14943	6.226	ng/uL	0.00
4) Pyridine-d5	3.646	84	91221	12.587	ng/ul	0.00
7) Phenol-d5	6.816	99	72702	8.197	ng/ul	0.00
9) Bis-(2-Chloroethyl)eth...	6.969	67	210942	36.504	ng/ul	-0.01
11) 2-Chlorophenol-d4	7.163	132	181434	28.484	ng/ul	0.00
15) 4-Methylphenol-d8	8.322	113	138167	20.135	ng/ul	0.00
21) Nitrobenzene-d5	8.769	128	121999	36.538	ng/ul	0.00
24) 2-Nitrophenol-d4	9.469	143	135340	36.228	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.004	165	236202	34.620	ng/ul	0.00
31) 4-Chloroaniline-d4	10.516	131	271336	30.507	ng/ul	0.00
46) Dimethylphthalate-d6	13.663	166	802863	41.443	ng/ul	0.00
49) Acenaphthylene-d8	13.934	160	926909	40.958	ng/ul	-0.02
54) 4-Nitrophenol-d4	14.528	143	22695m	7.452	ng/ul	0.03
60) Fluorene-d10	15.275	176	688484	41.719	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.416	200	118899	36.117	ng/ul	-0.02
73) Anthracene-d10	17.186	188	1043670	42.870	ng/ul	0.00
81) Pyrene-d10	19.575	212	1172223	42.994	ng/ul	-0.01
92) Benzo(a)pyrene-d12	24.610	264	1123703	42.985	ng/ul	-0.02

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032224\
Data File : BP019968.D
Acq On : 22 Mar 2024 23:31
Operator : MA/JU
Sample : P1813-15
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EOLY3

Manual IntegrationsAPPROVED

Quant Time: Mar 23 00:20:24 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032224.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 22 22:40:53 2024
Response via : Initial Calibration

Reviewed By :Yogesh Patel 03/26/2024
Supervised By :mohammad ahmed 03/26/2024

