

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032224\
 Data File : BP019961.D
 Acq On : 22 Mar 2024 18:32
 Operator : MA/JU
 Sample : PB159744BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK744

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032224.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP019961.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.240	23	26	32	rVB	27140	36276	1.50%	0.145%
2	3.646	91	95	111	rBV	320794	527563	21.74%	2.108%
3	3.934	142	144	150	rVB4	7062	8263	0.34%	0.033%
4	6.805	625	632	645	rBV	427913	716746	29.54%	2.864%
5	6.969	653	660	672	rBV	322064	553268	22.80%	2.211%
6	7.158	686	692	708	rBV	418041	704831	29.05%	2.817%
7	7.616	764	770	779	rBV	392252	618069	25.47%	2.470%
8	7.787	795	799	802	rBV5	1590	2506	0.10%	0.010%
9	8.322	882	890	902	rBV	509273	857095	35.32%	3.425%
10	8.587	933	935	941	rVB7	1910	2889	0.12%	0.012%
11	8.769	959	966	983	rBV	371842	703074	28.98%	2.810%
12	9.475	1077	1086	1099	rBV	332242	594257	24.49%	2.375%
13	9.563	1099	1101	1108	rVB7	2594	3229	0.13%	0.013%
14	10.016	1169	1178	1188	rBV	401409	789797	32.55%	3.156%
15	10.375	1231	1239	1252	rBV	451211	847703	34.94%	3.388%
16	10.528	1257	1265	1284	rBV	373405	809514	33.36%	3.235%
17	12.010	1512	1517	1525	rBV7	5312	11386	0.47%	0.046%
18	13.151	1703	1711	1715	rBV6	7359	16197	0.67%	0.065%
19	13.681	1792	1801	1813	rBV	817672	1214398	50.05%	4.853%
20	13.763	1813	1815	1822	rVB7	2475	4529	0.19%	0.018%
21	13.946	1837	1846	1860	rBV2	796657	1459883	60.16%	5.834%
22	14.251	1891	1898	1913	rBV	742767	1106837	45.61%	4.423%
23	14.504	1934	1941	1955	rBV2	187782	515131	21.23%	2.059%
24	15.281	2066	2073	2087	rVV	1153853	1741305	71.76%	6.959%
25	15.428	2090	2098	2112	rVV	240862	559486	23.06%	2.236%
26	15.534	2114	2116	2122	rVB7	6747	9091	0.37%	0.036%
27	16.081	2205	2209	2213	rVV7	5764	8603	0.35%	0.034%
28	16.757	2322	2324	2329	rBV6	1884	2813	0.12%	0.011%
29	16.863	2338	2342	2344	rBV5	2924	4643	0.19%	0.019%
30	17.087	2373	2380	2391	rBV	770309	1286989	53.04%	5.143%
31	17.192	2391	2398	2412	rVV	1315452	1929203	79.51%	7.709%
32	18.022	2537	2539	2541	rBV3	2688	2455	0.10%	0.010%
33	19.128	2724	2727	2732	rVB3	14514	19889	0.82%	0.079%
34	19.210	2737	2741	2743	rBV3	12116	16327	0.67%	0.065%
35	19.581	2798	2804	2817	rBV	1441137	2247371	92.62%	8.981%
36	21.545	3132	3138	3149	rBV	794732	1346077	55.47%	5.379%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032224\
Data File : BP019961.D
Acq On : 22 Mar 2024 18:32
Operator : MA/JU
Sample : PB159744BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK744

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032224.MA.M
Title : SVOA CALIBRATION

37	24.610	3651	3659	3674	rVB	844138	2426484	100.00%	9.697%
38	24.857	3694	3701	3712	rVB3	423677	1319937	54.40%	5.275%




Sum of corrected areas: 25024114

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032224\
Data File : BP019961.D
Acq On : 22 Mar 2024 18:32
Operator : MA/JU
Sample : PB159744BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK744

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

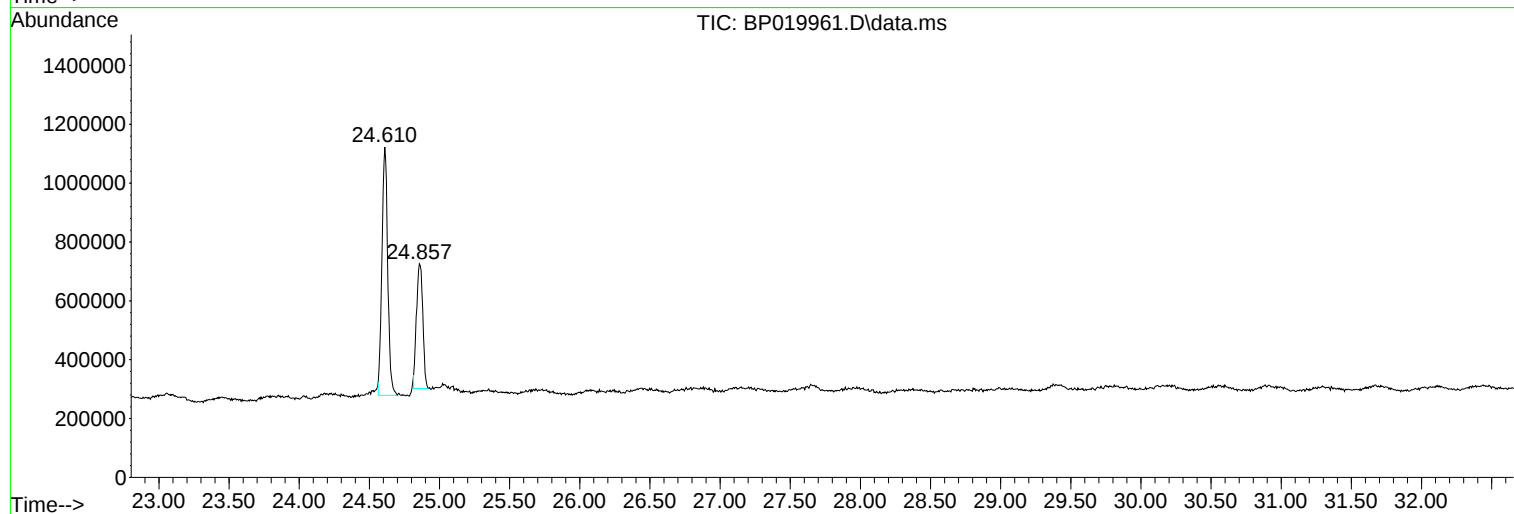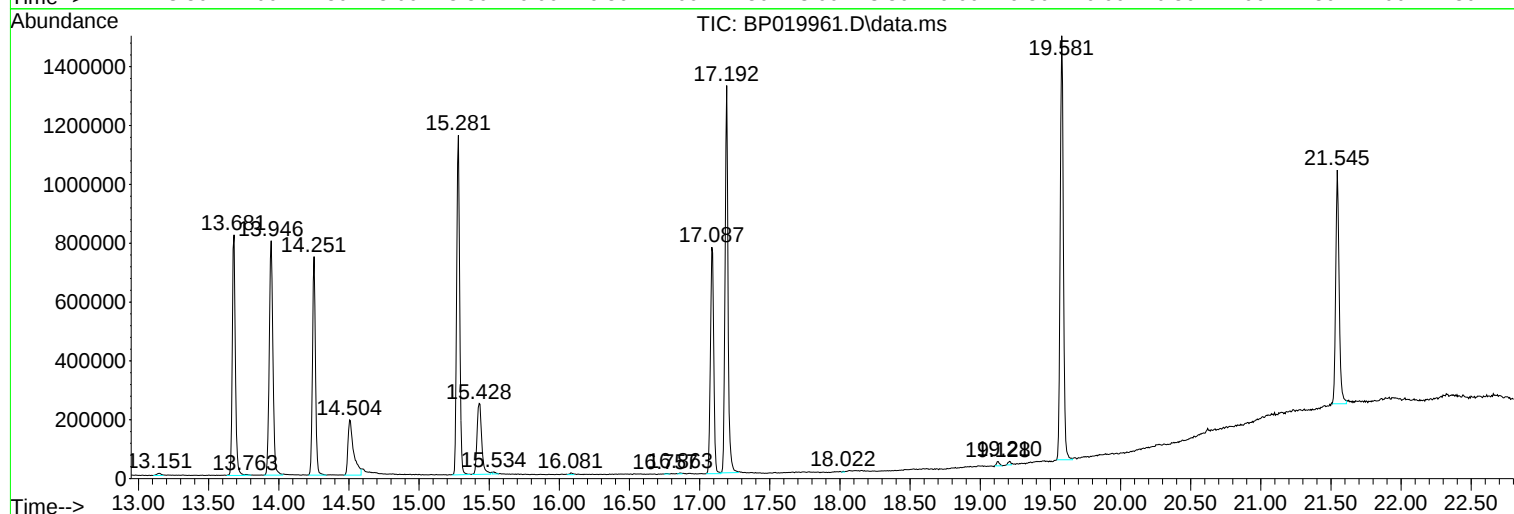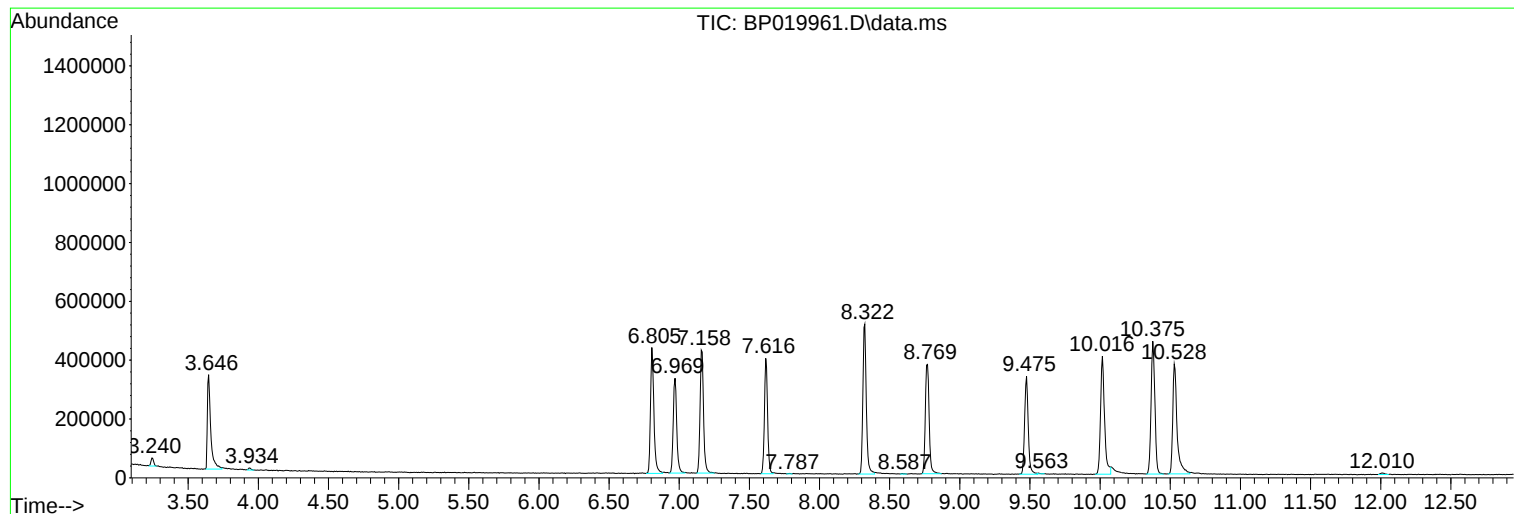

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032224\
Data File : BP019961.D
Acq On : 22 Mar 2024 18:32
Operator : MA/JU
Sample : PB159744BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK744

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032224\
Data File : BP019961.D
Acq On : 22 Mar 2024 18:32
Operator : MA/JU
Sample : PB159744BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK744

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------