

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032224\
 Data File : BP019962.D
 Acq On : 22 Mar 2024 19:15
 Operator : MA/JU
 Sample : PB159746BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK746

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032224.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP019962.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.246	23	27	36	rVB	35068	53530	1.86%	0.194%
2	3.640	90	94	113	rBV	372324	590085	20.45%	2.133%
3	3.940	143	145	150	rVB2	6392	6556	0.23%	0.024%
4	6.799	624	631	647	rBV	413075	793960	27.52%	2.870%
5	6.975	655	661	676	rVB	380752	608535	21.09%	2.200%
6	7.152	684	691	705	rBV	441731	772525	26.77%	2.793%
7	7.611	761	769	779	rBV	306326	575056	19.93%	2.079%
8	8.305	880	887	905	rBV	510620	946802	32.81%	3.423%
9	8.763	957	965	980	rBV	405756	773472	26.81%	2.796%
10	9.469	1076	1085	1095	rBV	370518	651882	22.59%	2.357%
11	10.005	1168	1176	1196	rBV	461927	943900	32.71%	3.412%
12	10.375	1231	1239	1249	rVB	440308	766772	26.57%	2.772%
13	10.522	1255	1264	1278	rBV	388532	873241	30.26%	3.157%
14	12.004	1507	1516	1524	rBV5	5920	15173	0.53%	0.055%
15	13.146	1702	1710	1718	rBV7	9909	24526	0.85%	0.089%
16	13.675	1791	1800	1809	rBV	1028441	1419993	49.21%	5.133%
17	13.946	1838	1846	1860	rBV2	925045	1623277	56.26%	5.868%
18	14.257	1891	1899	1908	rBV	578324	1019327	35.33%	3.685%
19	14.498	1932	1940	1953	rBV	250786	582904	20.20%	2.107%
20	15.275	2065	2072	2083	rBV2	1155759	1981063	68.66%	7.161%
21	15.440	2091	2100	2113	rBV	360193	696442	24.14%	2.518%
22	16.069	2201	2207	2212	rVB10	5543	10330	0.36%	0.037%
23	16.757	2318	2324	2329	rVV9	3255	6684	0.23%	0.024%
24	17.092	2375	2381	2390	rBV	803067	1236783	42.86%	4.471%
25	17.187	2390	2397	2414	rVV	1446945	2261082	78.36%	8.174%
26	18.063	2543	2546	2551	rBV6	4258	6708	0.23%	0.024%
27	19.128	2723	2727	2731	rVB5	15794	22382	0.78%	0.081%
28	19.204	2736	2740	2744	rBV3	19183	30437	1.05%	0.110%
29	19.581	2798	2804	2815	rBV	1947351	2724622	94.43%	9.849%
30	21.551	3133	3139	3149	rBV2	769900	1380633	47.85%	4.991%
31	24.616	3652	3660	3673	rVB2	1069013	2885336	100.00%	10.430%
32	24.863	3694	3702	3714	rVB	453446	1378857	47.79%	4.985%




Sum of corrected areas: 27662875

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032224\
Data File : BP019962.D
Acq On : 22 Mar 2024 19:15
Operator : MA/JU
Sample : PB159746BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK746

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

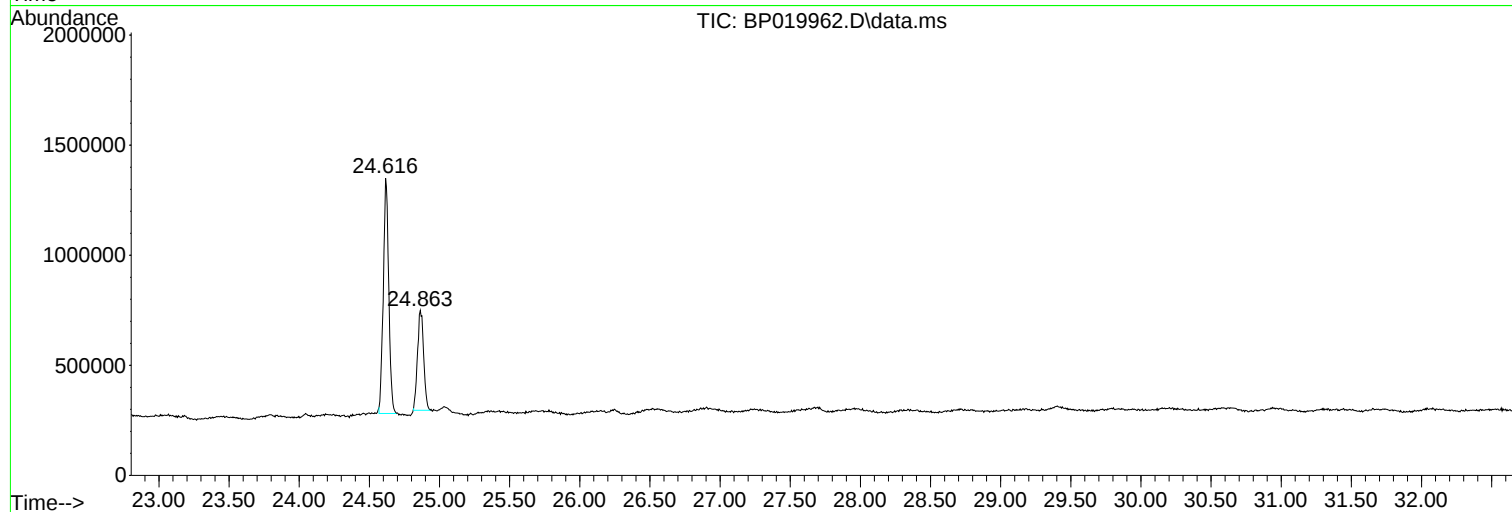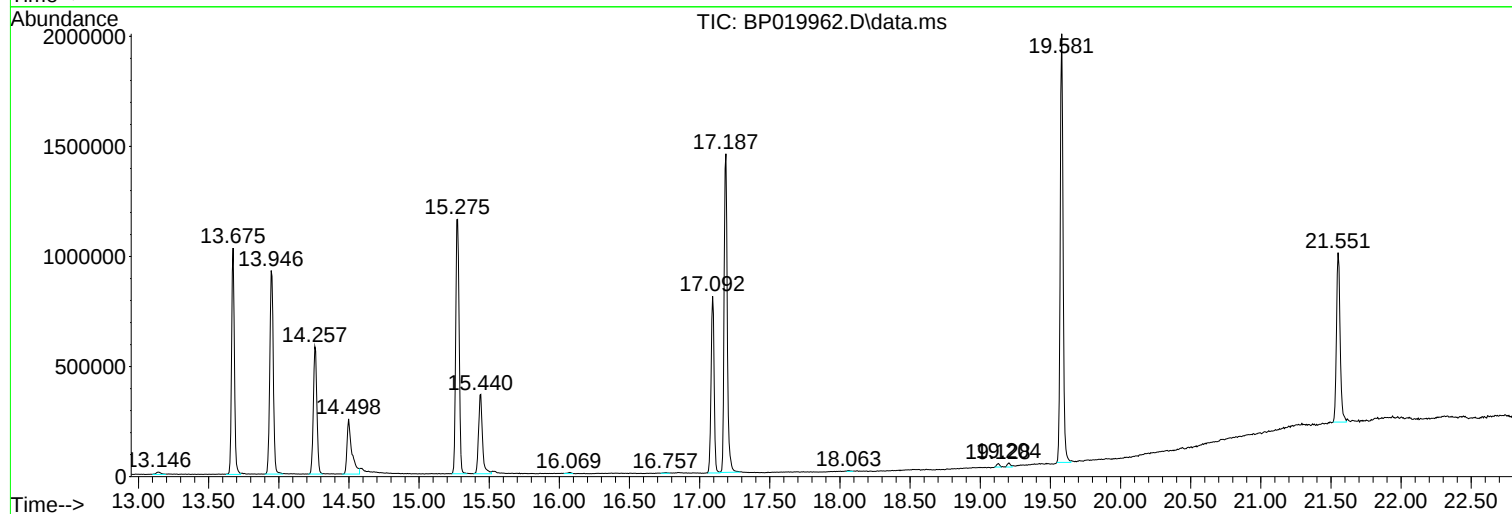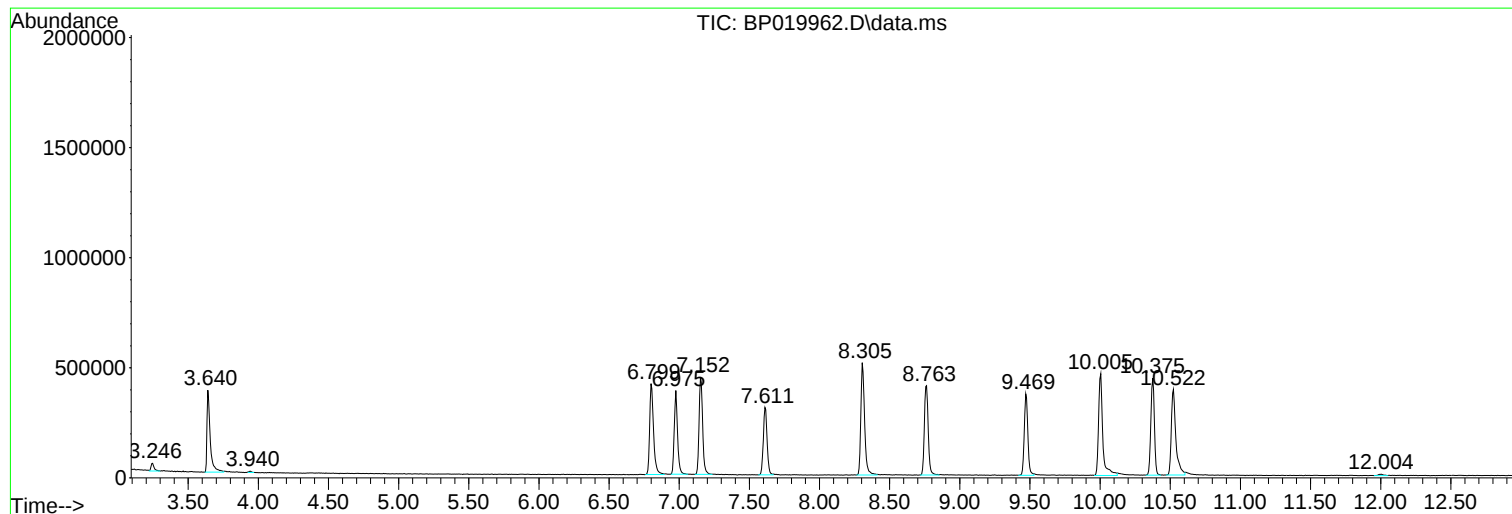

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032224\
Data File : BP019962.D
Acq On : 22 Mar 2024 19:15
Operator : MA/JU
Sample : PB159746BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK746

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032224\
Data File : BP019962.D
Acq On : 22 Mar 2024 19:15
Operator : MA/JU
Sample : PB159746BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK746

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------