

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032224\
 Data File : BP019968.D
 Acq On : 22 Mar 2024 23:31
 Operator : MA/JU
 Sample : P1813-15
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 E0LY3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032224.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP019968.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.240	23	26	34	rVB	31670	43648	1.48%	0.146%
2	3.646	92	95	109	rBV	150583	255062	8.63%	0.852%
3	3.934	141	144	149	rVB2	9450	12181	0.41%	0.041%
4	3.975	149	151	155	rBV4	2444	3261	0.11%	0.011%
5	5.111	342	344	351	rVB8	2522	4261	0.14%	0.014%
6	5.981	488	492	497	rBV7	1546	3211	0.11%	0.011%
7	6.675	606	610	613	rBV6	2661	5121	0.17%	0.017%
8	6.816	626	634	646	rBV	103374	209986	7.11%	0.701%
9	6.969	652	660	674	rVV	443822	719532	24.36%	2.403%
10	7.163	686	693	706	rBV	418778	715682	24.23%	2.390%
11	7.616	763	770	785	rBV	406855	660238	22.35%	2.205%
12	8.322	882	890	905	rVV	342970	630381	21.34%	2.105%
13	8.763	957	965	980	rBV	538666	953477	32.28%	3.184%
14	8.922	990	992	996	rVB4	2398	3269	0.11%	0.011%
15	8.969	996	1000	1008	rVB10	3033	6289	0.21%	0.021%
16	9.116	1019	1025	1034	rBV8	6486	15038	0.51%	0.050%
17	9.469	1077	1085	1099	rBV	410607	789526	26.73%	2.637%
18	10.004	1169	1176	1201	rBV	561096	1149507	38.91%	3.839%
19	10.363	1227	1237	1251	rVB	500682	943962	31.95%	3.152%
20	10.516	1255	1263	1280	rBV	461582	962269	32.57%	3.214%
21	10.775	1299	1307	1313	rBV	9117	17051	0.58%	0.057%
22	10.869	1316	1323	1325	rBV8	2679	5782	0.20%	0.019%
23	10.904	1325	1329	1341	rVB8	6529	21469	0.73%	0.072%
24	11.057	1350	1355	1361	rBV9	1433	2994	0.10%	0.010%
25	11.193	1368	1378	1386	rBV3	29765	66657	2.26%	0.223%
26	11.257	1386	1389	1393	rVV4	9530	15931	0.54%	0.053%
27	11.298	1393	1396	1404	rVB3	10241	18669	0.63%	0.062%
28	11.587	1440	1445	1448	rBV6	3950	7479	0.25%	0.025%
29	11.640	1451	1454	1459	rVV7	3683	5736	0.19%	0.019%
30	11.734	1465	1470	1471	rVB3	2807	4024	0.14%	0.013%
31	11.863	1488	1492	1497	rBV4	3363	6339	0.21%	0.021%
32	11.916	1497	1501	1502	rVV4	4182	5058	0.17%	0.017%
33	11.969	1506	1510	1516	rVB5	5826	12700	0.43%	0.042%
34	13.128	1702	1707	1715	rVB3	14161	25137	0.85%	0.084%
35	13.204	1715	1720	1726	rBV10	2882	7139	0.24%	0.024%
36	13.657	1789	1797	1814	rBV	1031273	1800220	60.94%	6.012%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032224\
 Data File : BP019968.D
 Acq On : 22 Mar 2024 23:31
 Operator : MA/JU
 Sample : P1813-15
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 E0LY3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032224.MA.M
 Title : SVOA CALIBRATION

37	13.934	1836	1844	1861	rBV	1458884	2181653	73.85%	7.286%
38	14.181	1884	1886	1891	rVV6	3429	4802	0.16%	0.016%
39	14.251	1891	1898	1907	rVV	877684	1217559	41.22%	4.066%
40	14.334	1910	1912	1918	rVB7	5268	8528	0.29%	0.028%
41	14.528	1939	1945	1955	rBV2	51354	143989	4.87%	0.481%
42	14.698	1972	1974	1989	rVB2	5946	16646	0.56%	0.056%
43	15.110	2041	2044	2049	rVB4	5363	8589	0.29%	0.029%
44	15.275	2065	2072	2089	rBV	1769734	2612271	88.43%	8.724%
45	15.416	2090	2096	2108	rVV	582230	835592	28.29%	2.791%
46	15.522	2111	2114	2119	rVB5	12537	19587	0.66%	0.065%
47	15.628	2129	2132	2136	rBV6	2570	3320	0.11%	0.011%
48	16.092	2207	2211	2216	rVB8	6988	12376	0.42%	0.041%
49	16.492	2275	2279	2283	rBV7	3931	6931	0.23%	0.023%
50	17.069	2370	2377	2386	rBV	913029	1346042	45.57%	4.495%
51	17.186	2389	2397	2411	rBV	1607043	2710973	91.77%	9.054%
52	18.028	2536	2540	2545	rBV2	46089	73367	2.48%	0.245%
53	19.116	2722	2725	2733	rVB3	27046	39155	1.33%	0.131%
54	19.375	2766	2769	2775	rBV7	21122	32035	1.08%	0.107%
55	19.575	2797	2803	2810	rVB	2078314	2954046	100.00%	9.865%
56	21.545	3132	3138	3148	rBV	837124	1334034	45.16%	4.455%
57	24.610	3650	3659	3670	rBV	1239841	2921964	98.91%	9.758%
58	24.833	3689	3697	3709	rVB	436781	1352135	45.77%	4.516%


Sum of corrected areas: 29943880

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032224\
Data File : BP019968.D
Acq On : 22 Mar 2024 23:31
Operator : MA/JU
Sample : P1813-15
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EOLY3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

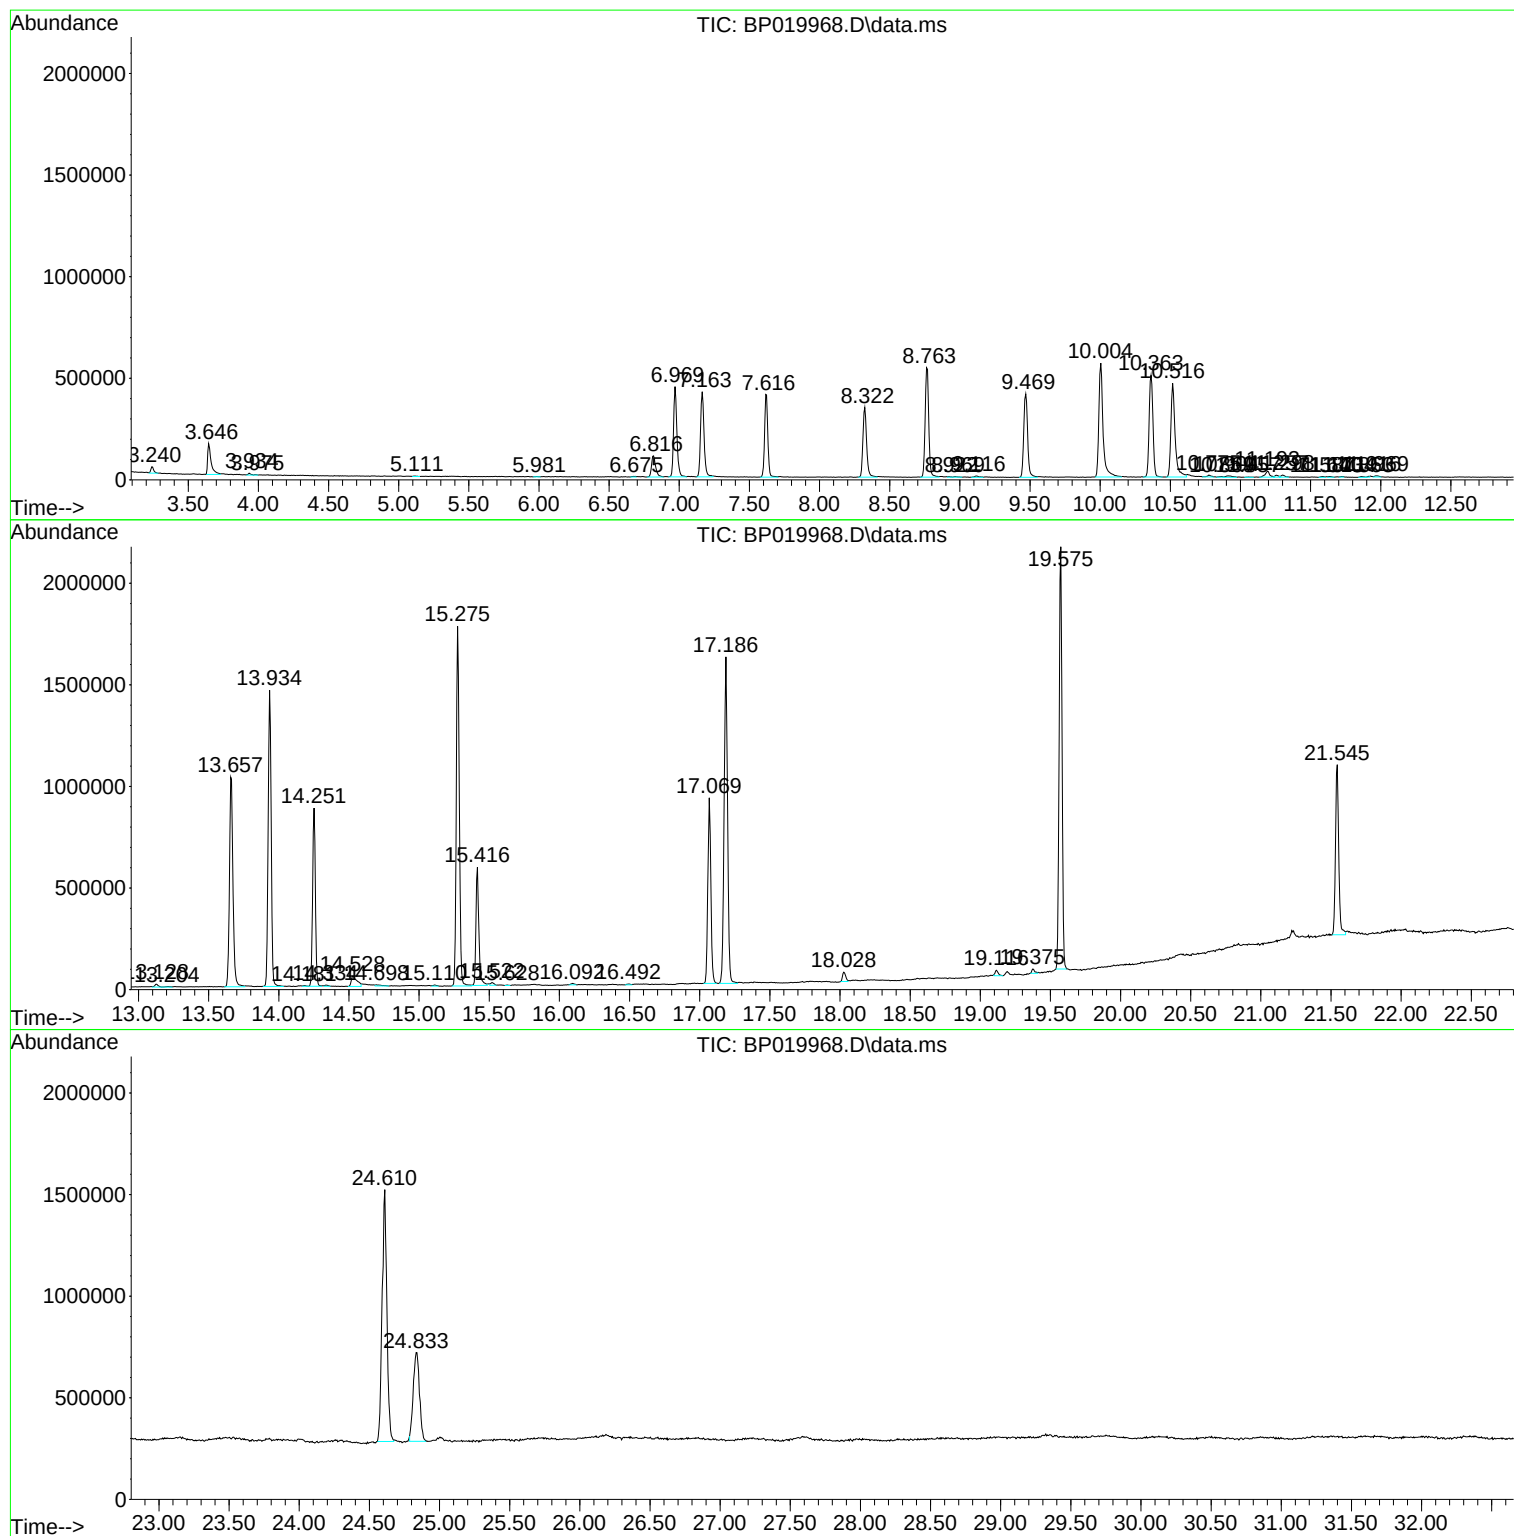

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032224\
Data File : BP019968.D
Acq On : 22 Mar 2024 23:31
Operator : MA/JU
Sample : P1813-15
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E0LY3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032224\
Data File : BP019968.D
Acq On : 22 Mar 2024 23:31
Operator : MA/JU
Sample : P1813-15
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E0LY3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------