

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032224\
 Data File : BP019969.D
 Acq On : 23 Mar 2024 00:14
 Operator : MA/JU
 Sample : P1841-01
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AK3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032224.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP019969.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.211	16	21	40	rVB	1623306	2318824	65.94%	7.246%
2	3.652	92	96	113	rBV	112740	193894	5.51%	0.606%
3	3.940	142	145	150	rVB2	8398	10995	0.31%	0.034%
4	4.440	224	230	241	rVB	309475	481406	13.69%	1.504%
5	5.064	333	336	341	rBV7	3134	4503	0.13%	0.014%
6	5.387	387	391	393	rBV4	3102	5005	0.14%	0.016%
7	6.616	599	600	604	rVB4	3773	3971	0.11%	0.012%
8	6.816	627	634	650	rBV	63661	156051	4.44%	0.488%
9	6.975	655	661	674	rBV	388027	653023	18.57%	2.041%
10	7.163	686	693	703	rBV	318070	598202	17.01%	1.869%
11	7.622	762	771	780	rBV	331117	604484	17.19%	1.889%
12	7.728	784	789	794	rVB2	16724	28375	0.81%	0.089%
13	7.969	826	830	831	rBV4	3830	4140	0.12%	0.013%
14	8.322	883	890	901	rBV	216874	446931	12.71%	1.397%
15	8.399	901	903	910	rVB7	5290	9418	0.27%	0.029%
16	8.769	959	966	978	rBV	464089	834185	23.72%	2.607%
17	9.475	1078	1086	1100	rBV	391033	686739	19.53%	2.146%
18	10.004	1166	1176	1197	rBV	419305	918194	26.11%	2.869%
19	10.369	1229	1238	1250	rBV	489436	816018	23.21%	2.550%
20	10.528	1256	1265	1286	rBV	365357	881918	25.08%	2.756%
21	11.204	1374	1380	1387	rBV10	6232	14542	0.41%	0.045%
22	11.981	1507	1512	1519	rBV4	5645	11898	0.34%	0.037%
23	13.128	1702	1707	1714	rBV3	11919	20160	0.57%	0.063%
24	13.663	1788	1798	1816	rBV	903684	1657139	47.12%	5.178%
25	13.940	1838	1845	1854	rBV	1224216	1821150	51.79%	5.691%
26	14.257	1893	1899	1918	rBV	820487	1104380	31.41%	3.451%
27	14.539	1939	1947	1958	rBV4	32704	113323	3.22%	0.354%
28	14.616	1958	1960	1970	rVB10	7699	20716	0.59%	0.065%
29	15.069	2034	2037	2042	rVB	12181	15866	0.45%	0.050%
30	15.275	2064	2072	2084	rBV	1479613	2396032	68.14%	7.487%
31	15.416	2090	2096	2107	rBV	533603	829188	23.58%	2.591%
32	15.516	2110	2113	2120	rVB8	8988	17870	0.51%	0.056%
33	15.863	2169	2172	2176	rVB6	2708	3883	0.11%	0.012%
34	16.092	2206	2211	2215	rBV9	5816	10022	0.28%	0.031%
35	16.739	2316	2321	2327	rVB10	4016	7135	0.20%	0.022%
36	16.851	2332	2340	2345	rBV10	5126	13162	0.37%	0.041%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032224\
 Data File : BP019969.D
 Acq On : 23 Mar 2024 00:14
 Operator : MA/JU
 Sample : P1841-01
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AK3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032224.MA.M
 Title : SVOA CALIBRATION

37	16.933	2351	2354	2357	rBV5	2962	3982	0.11%	0.012%
38	17.063	2370	2376	2387	rBV	908792	1349334	38.37%	4.216%
39	17.181	2387	2396	2413	rVV	1476355	2745909	78.09%	8.580%
40	17.504	2449	2451	2455	rVB5	3250	3539	0.10%	0.011%
41	18.033	2537	2541	2549	rVB8	15148	25244	0.72%	0.079%
42	18.927	2689	2693	2698	rBV2	24553	36401	1.04%	0.114%
43	19.110	2720	2724	2730	rBV4	26116	42148	1.20%	0.132%
44	19.192	2734	2738	2743	rVV	17717	27848	0.79%	0.087%
45	19.375	2767	2769	2776	rBV7	9321	14184	0.40%	0.044%
46	19.569	2796	2802	2812	rVB2	2180542	3307792	94.06%	10.336%
47	21.551	3133	3139	3147	rBV	1032252	1548860	44.04%	4.840%
48	24.610	3650	3659	3672	rVB2	1297367	3516543	100.00%	10.989%
49	24.821	3688	3695	3711	rVB	596304	1667266	47.41%	5.210%




Sum of corrected areas: 32001792

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032224\
Data File : BP019969.D
Acq On : 23 Mar 2024 00:14
Operator : MA/JU
Sample : P1841-01
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AK3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

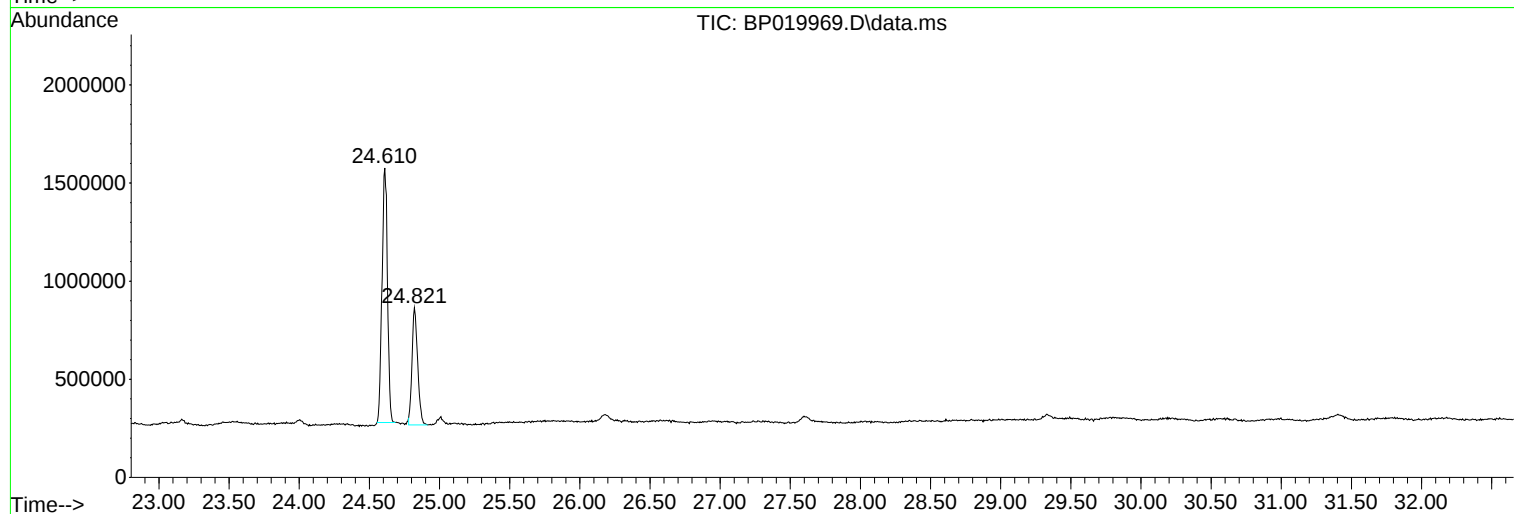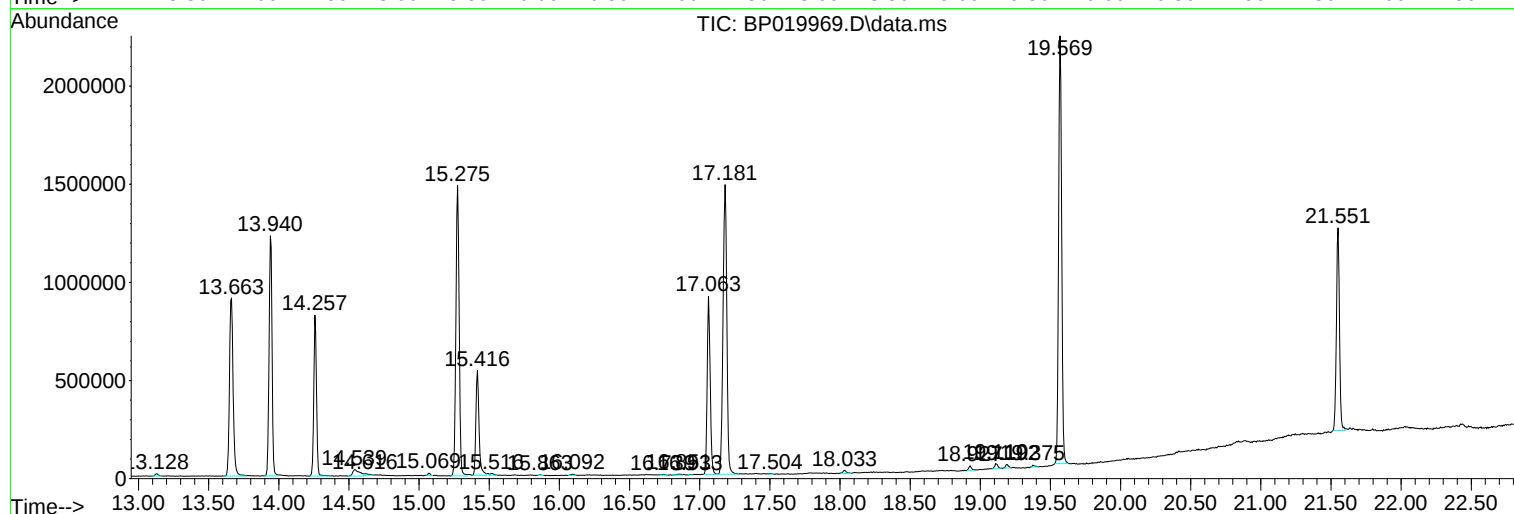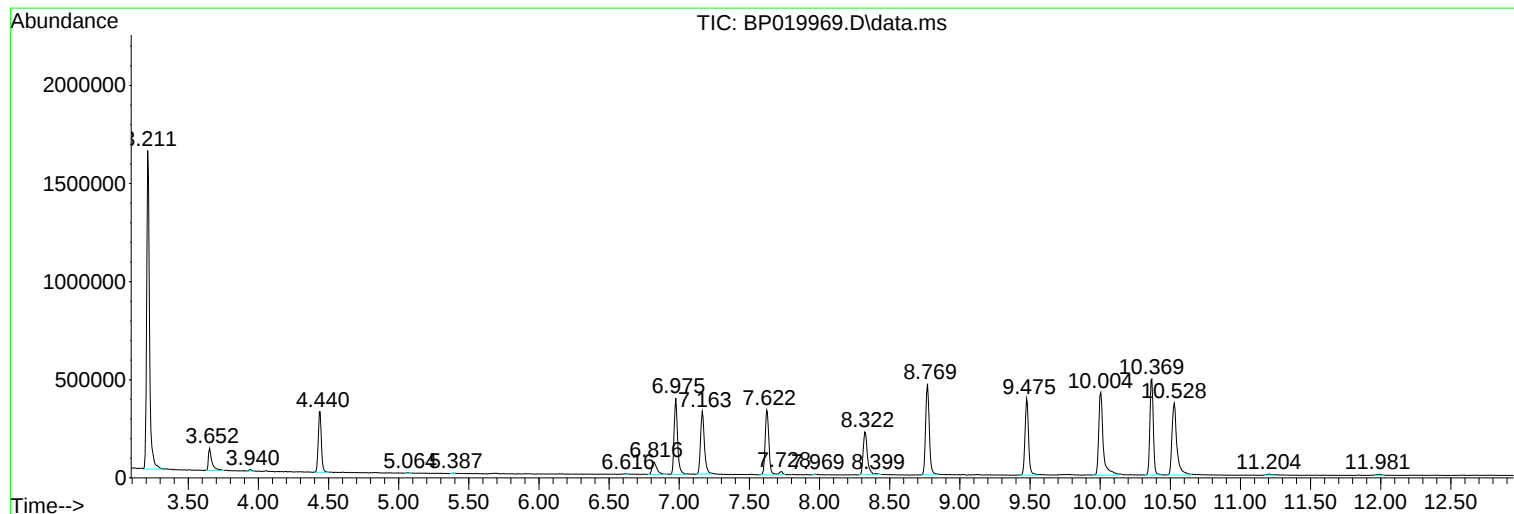

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032224\
Data File : BP019969.D
Acq On : 23 Mar 2024 00:14
Operator : MA/JU
Sample : P1841-01
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AK3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032224\
Data File : BP019969.D
Acq On : 23 Mar 2024 00:14
Operator : MA/JU
Sample : P1841-01
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AK3

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc