

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032224\
 Data File : BP019972.D
 Acq On : 23 Mar 2024 02:22
 Operator : MA/JU
 Sample : P1841-04
 Misc :
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 C0AK9

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032224.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP019972.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.240	23	26	31	rVB	23455	29438	0.81%	0.098%
2	3.652	93	96	107	rBV	44150	76455	2.09%	0.255%
3	3.934	142	144	149	rVB5	7250	8144	0.22%	0.027%
4	6.816	627	634	649	rBV	68963	157834	4.32%	0.526%
5	6.969	654	660	672	rBV	373482	623182	17.07%	2.076%
6	7.163	685	693	707	rBV	318481	597555	16.37%	1.991%
7	7.622	763	771	783	rBV	338198	608510	16.67%	2.027%
8	8.328	881	891	908	rBV	220250	460686	12.62%	1.535%
9	8.769	958	966	979	rBV	431378	812727	22.26%	2.708%
10	9.122	1022	1026	1030	rVB3	6004	8646	0.24%	0.029%
11	9.475	1078	1086	1100	rBV	366801	670873	18.38%	2.235%
12	10.004	1169	1176	1203	rBV	391808	902534	24.72%	3.007%
13	10.363	1230	1237	1248	rBV	520516	846909	23.20%	2.822%
14	10.522	1256	1264	1285	rBV	269299	667031	18.27%	2.222%
15	11.987	1506	1513	1518	rBV7	6025	14896	0.41%	0.050%
16	13.134	1702	1708	1713	rBV2	11080	17050	0.47%	0.057%
17	13.198	1716	1719	1729	rVB2	2689	6135	0.17%	0.020%
18	13.645	1788	1795	1814	rBV	1019487	1690524	46.30%	5.632%
19	13.934	1838	1844	1862	rBV	1368670	1871972	51.27%	6.237%
20	14.257	1891	1899	1910	rBV	760795	1195398	32.74%	3.983%
21	14.522	1938	1944	1948	rBV3	28947	61324	1.68%	0.204%
22	15.069	2034	2037	2043	rBV	6501	8963	0.25%	0.030%
23	15.263	2061	2070	2083	rBV	1442752	2421246	66.32%	8.067%
24	15.416	2090	2096	2110	rBV	603160	926956	25.39%	3.088%
25	15.516	2111	2113	2120	rVB3	11669	16680	0.46%	0.056%
26	16.086	2203	2210	2215	rBV9	5795	12740	0.35%	0.042%
27	16.745	2315	2322	2330	rBV9	3120	8294	0.23%	0.028%
28	16.851	2337	2340	2345	rBV7	3095	5938	0.16%	0.020%
29	17.069	2371	2377	2387	rBV	1075838	1510816	41.38%	5.033%
30	17.175	2387	2395	2417	rVB2	1670128	2982015	81.68%	9.935%
31	17.404	2429	2434	2438	rVB8	2388	3940	0.11%	0.013%
32	17.780	2493	2498	2500	rBV6	2963	5036	0.14%	0.017%
33	18.033	2536	2541	2548	rBV6	18958	34618	0.95%	0.115%
34	19.122	2722	2726	2732	rBV3	25067	33275	0.91%	0.111%
35	19.192	2734	2738	2745	rBV2	19771	34050	0.93%	0.113%
36	19.569	2796	2802	2815	rBV2	2292684	3609122	98.86%	12.024%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032224\
Data File : BP019972.D
Acq On : 23 Mar 2024 02:22
Operator : MA/JU
Sample : P1841-04
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AK9

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032224.MA.M
Title : SVOA CALIBRATION

37	21.551	3133	3139	3149	rVB	968249	1688658	46.25%	5.626%
38	24.609	3650	3659	3672	rVB	1445811	3650851	100.00%	12.163%
39	24.845	3691	3699	3711	rVB	622324	1734412	47.51%	5.778%




Sum of corrected areas: 30015433

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032224\
Data File : BP019972.D
Acq On : 23 Mar 2024 02:22
Operator : MA/JU
Sample : P1841-04
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AK9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

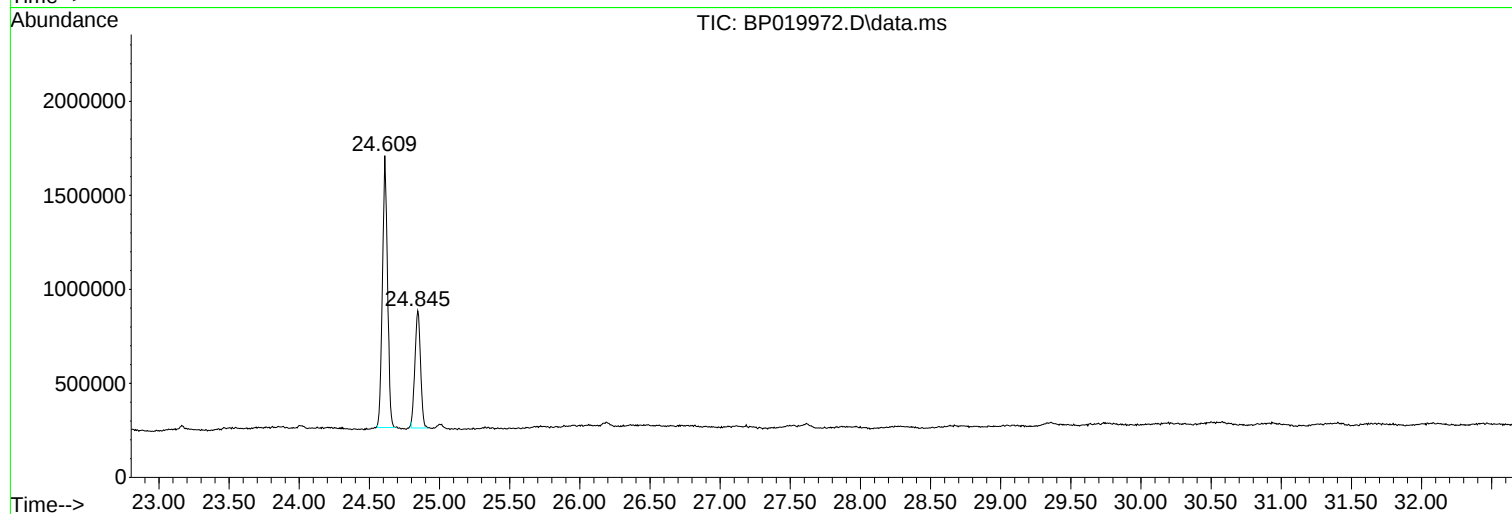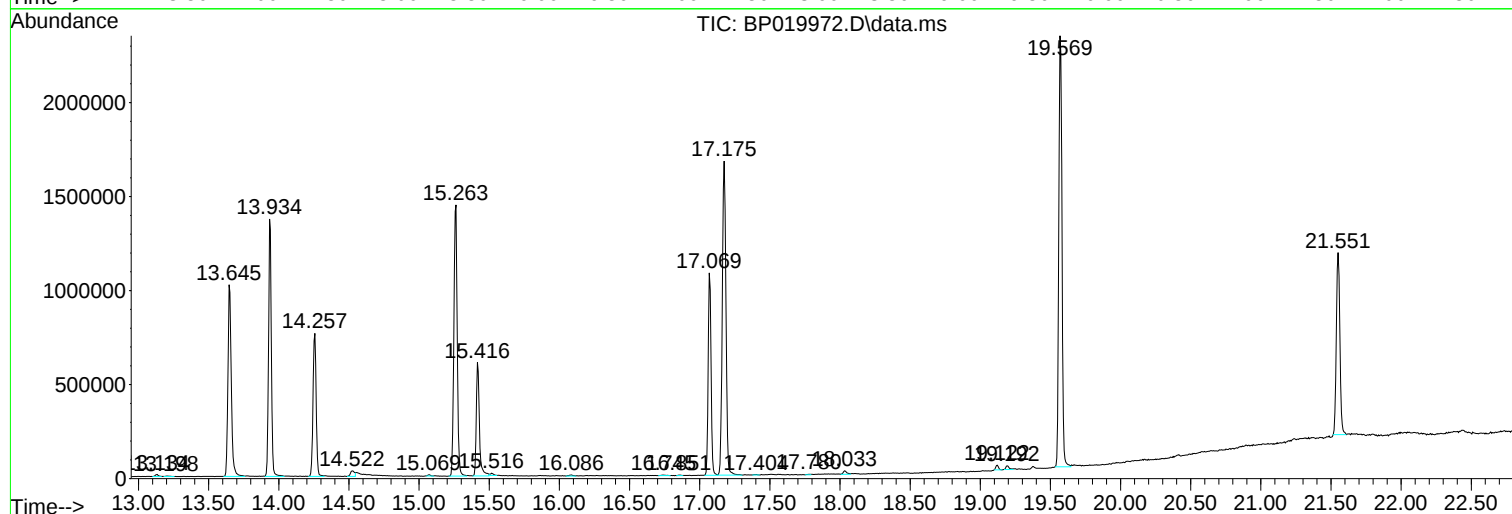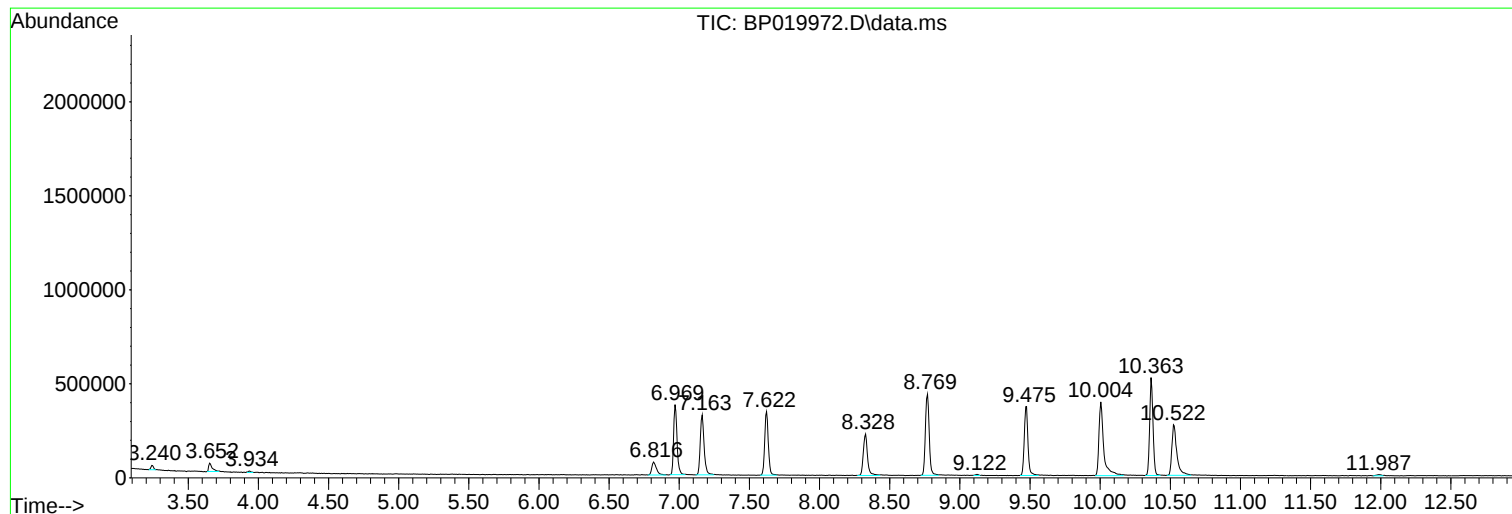

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032224\
Data File : BP019972.D
Acq On : 23 Mar 2024 02:22
Operator : MA/JU
Sample : P1841-04
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AK9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032224\
Data File : BP019972.D
Acq On : 23 Mar 2024 02:22
Operator : MA/JU
Sample : P1841-04
Misc :
ALS Vial : 14 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
C0AK9

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc