
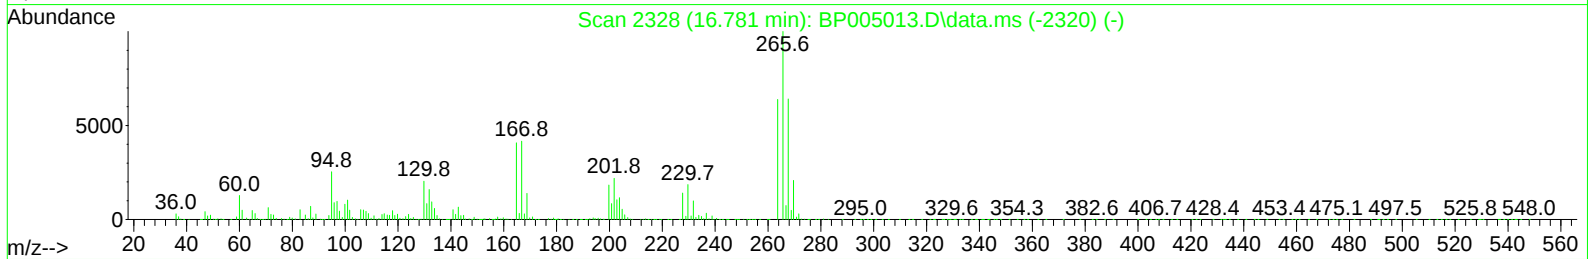
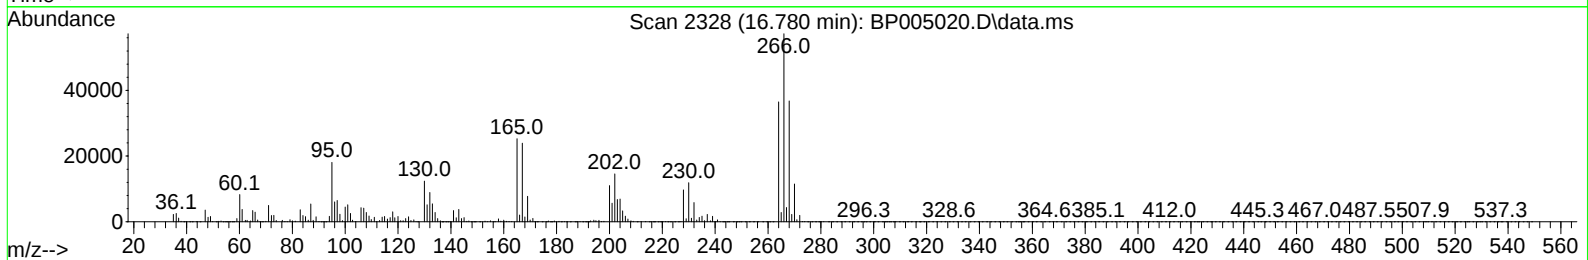


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032321\
 Data File : BP005020.D
 Acq On : 23 Mar 2021 12:25
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 23 12:58:55 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP032321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Mar 23 12:07:46 2021
 Response via : Initial Calibration

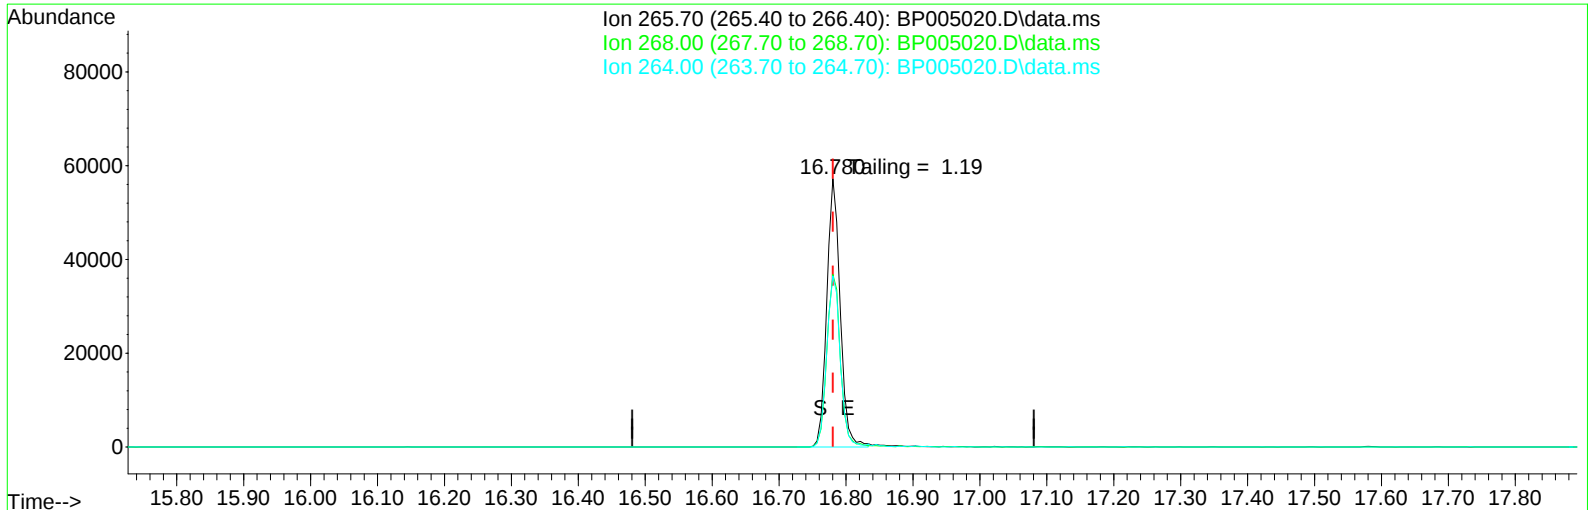




TIC: BP005020.D\data.ms

(70) Pentachlorophenol (C)**16.780min (-0.000) 1562123.11 ng****response 80570**

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.90	64.28
264.00	63.30	63.76
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032321\
 Data File : BP005020.D
 Acq On : 23 Mar 2021 12:25
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 23 12:58:55 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP032321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Mar 23 12:07:46 2021
 Response via : Initial Calibration

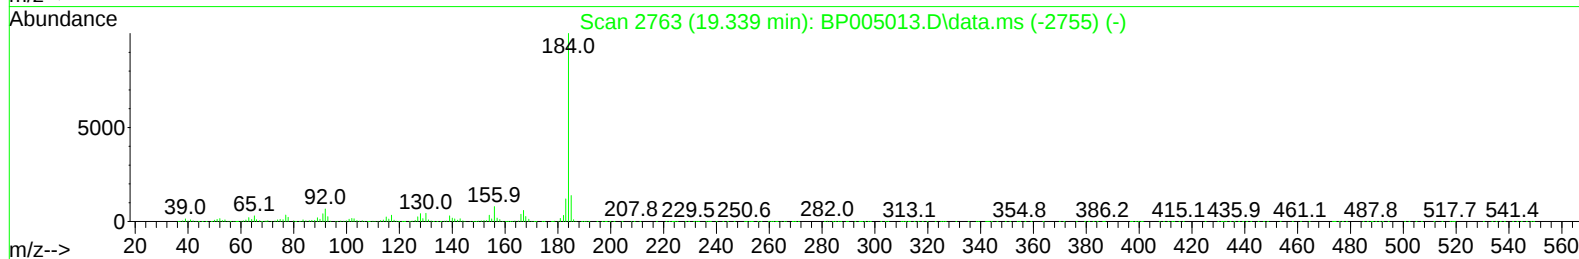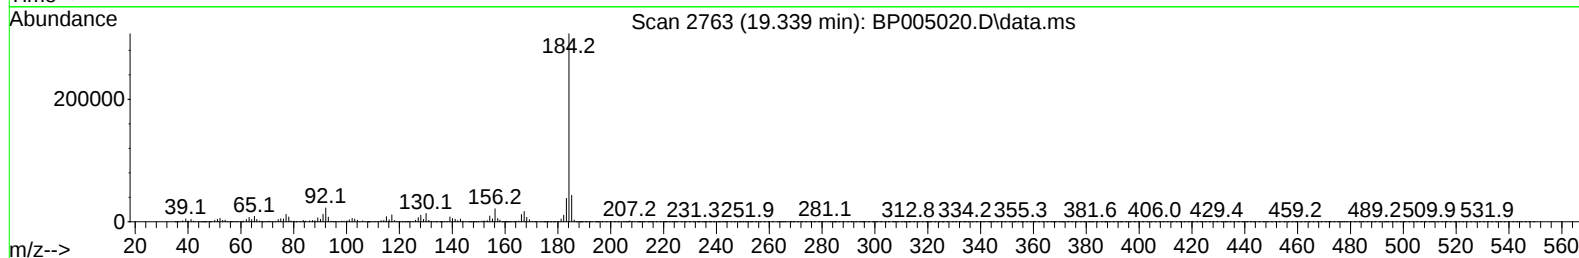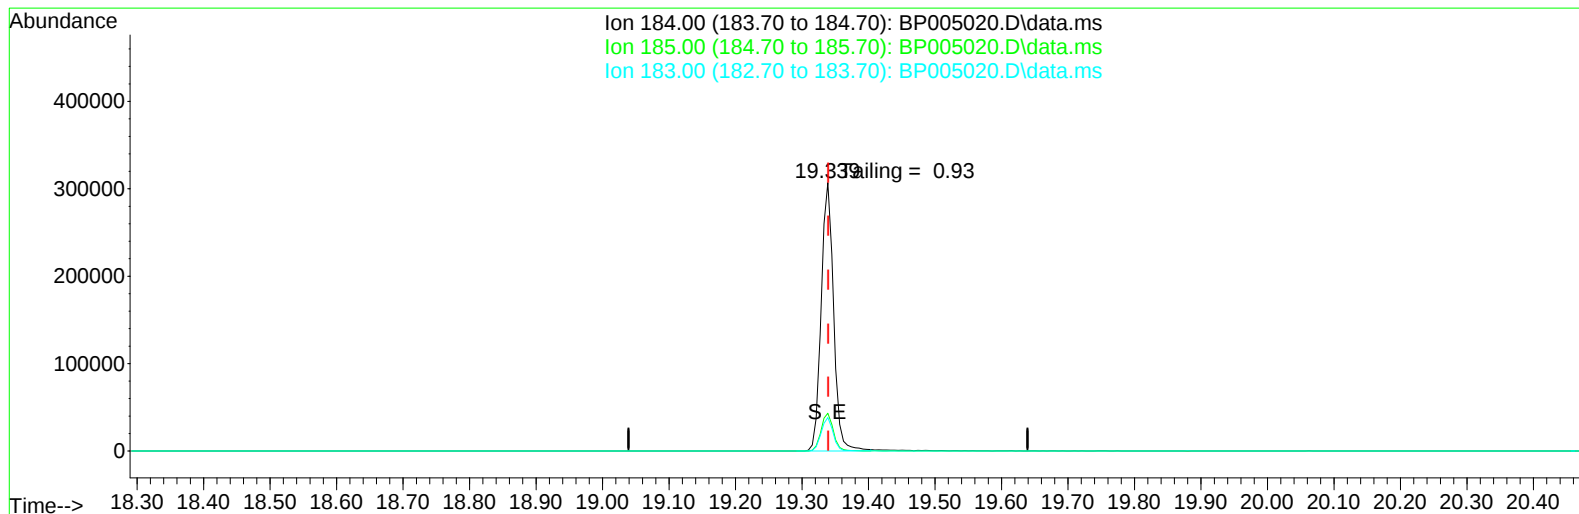

TIC: BP005020.D\data.ms

(77) Benzidine**19.339min (-0.001) 2425852.84 ng****response 402669**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.08
183.00	12.00	12.47
0.00	0.00	0.00