
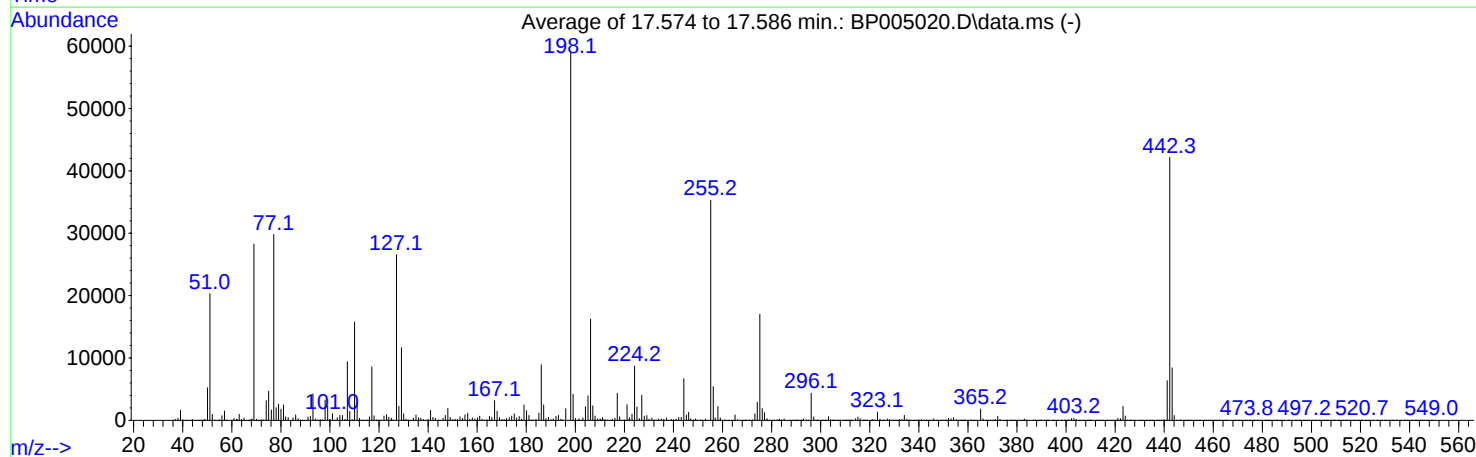


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032321\
 Data File : BP005020.D
 Acq On : 23 Mar 2021 12:25
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP032321.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Mar 24 10:16:52 2021

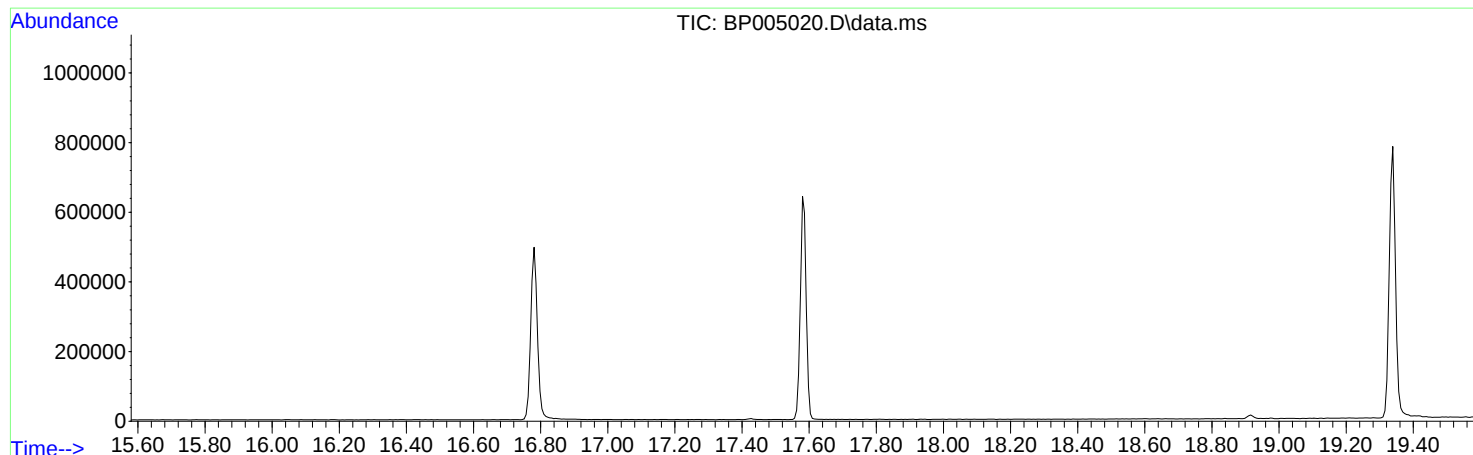




AutoFind: Scans 2463, 2464, 2465; Background Corrected with Scan 2455

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	34.5	20321	PASS
68	69	0.00	2	0.9	242	PASS
69	198	0.00	100	47.9	28271	PASS
70	69	0.00	2	0.7	188	PASS
127	198	10	80	45.0	26539	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	58973	PASS
199	198	5	9	7.1	4188	PASS
275	198	10	60	28.9	17022	PASS
365	198	1	100	3.1	1834	PASS
441	198	0.01	100	10.8	6365	PASS
442	442	100	100	100.0	42160	PASS
443	442	15	24	19.9	8406	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032321\
Data File : BP005020.D
Acq On : 23 Mar 2021 12:25
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Mar 23 12:58:55 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP032321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 23 12:07:46 2021
Response via : Initial Calibration

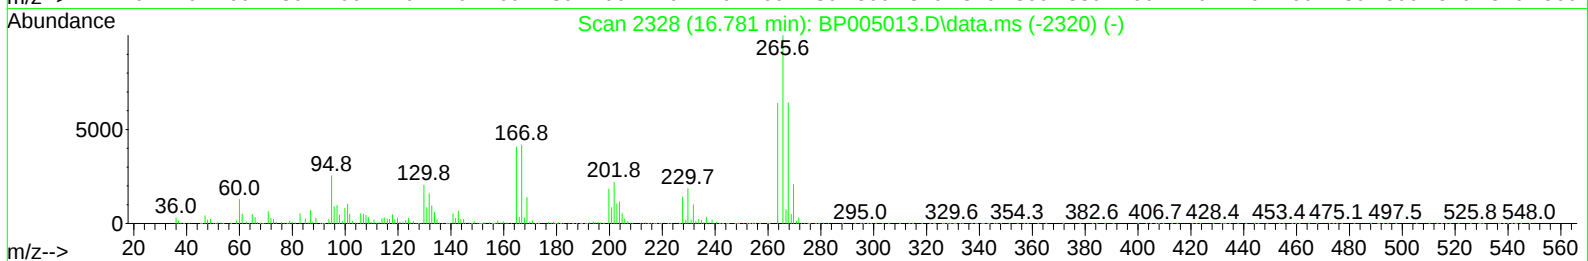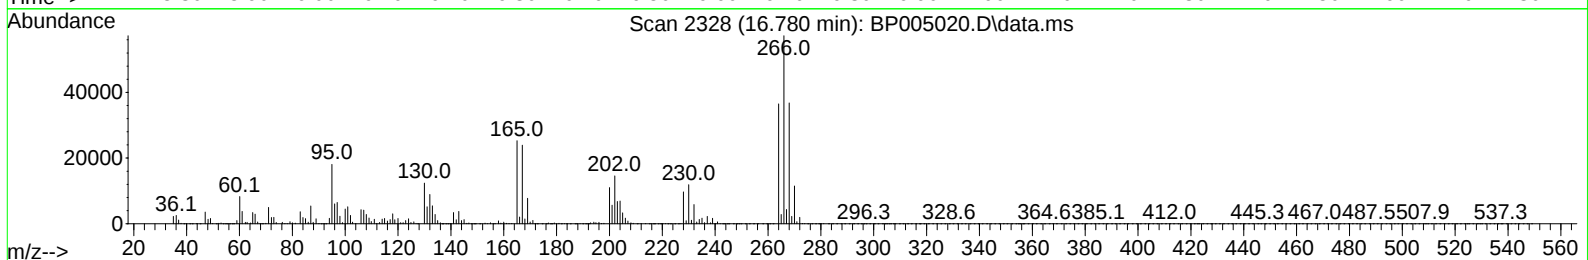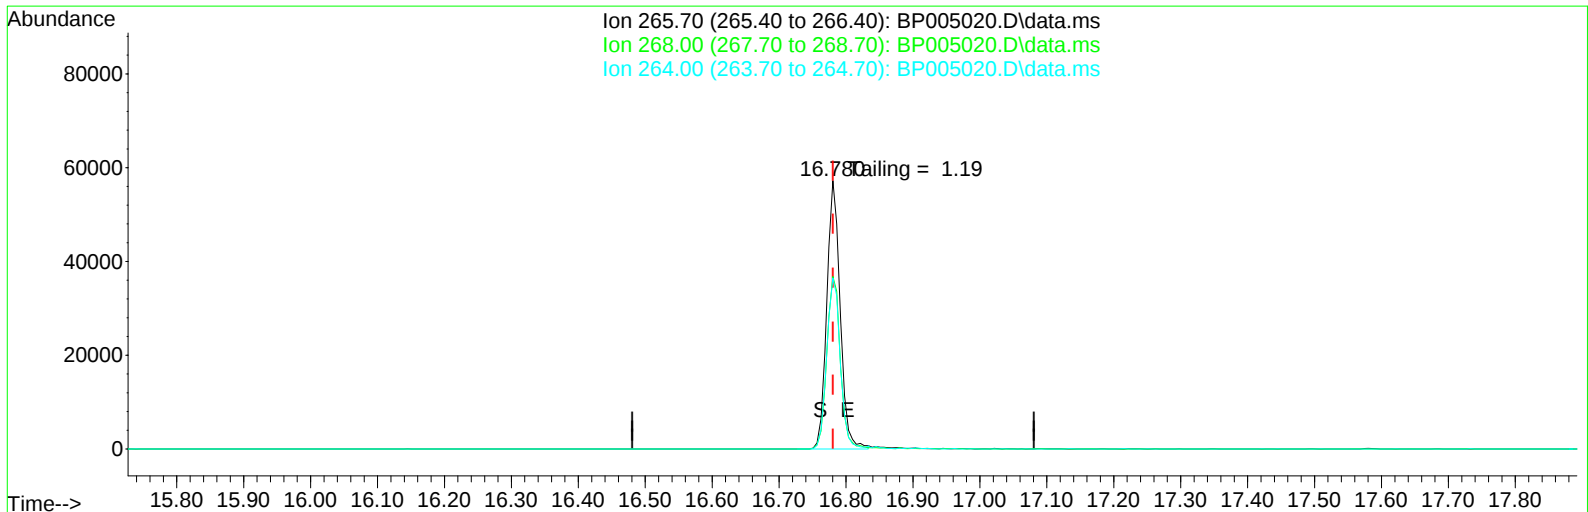

TIC: BP005020.D\data.ms

(70) Pentachlorophenol (C)

16.780min (-0.000) 1562123.11 ng




response 80570

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.90	64.28
264.00	63.30	63.76
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032321\
 Data File : BP005020.D
 Acq On : 23 Mar 2021 12:25
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Mar 23 12:58:55 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP032321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Mar 23 12:07:46 2021
 Response via : Initial Calibration

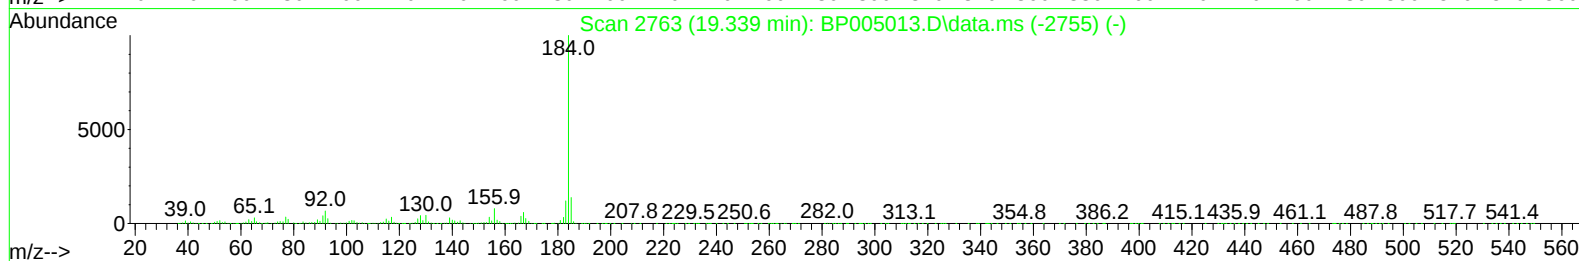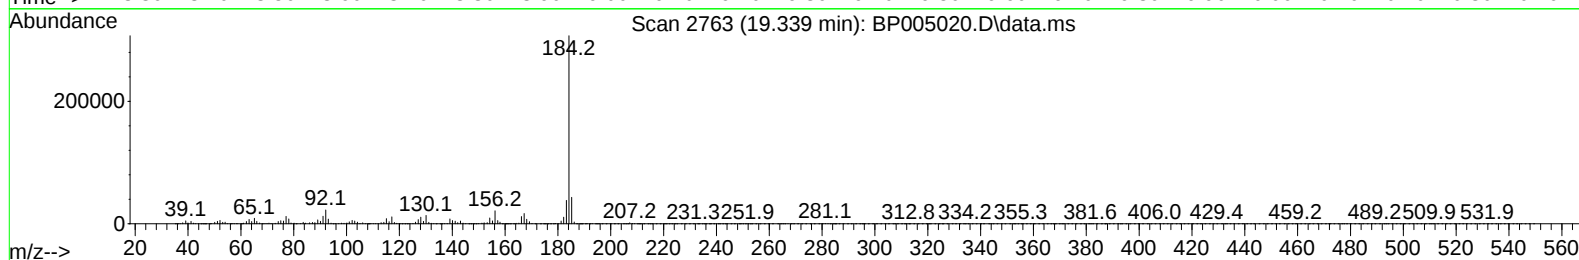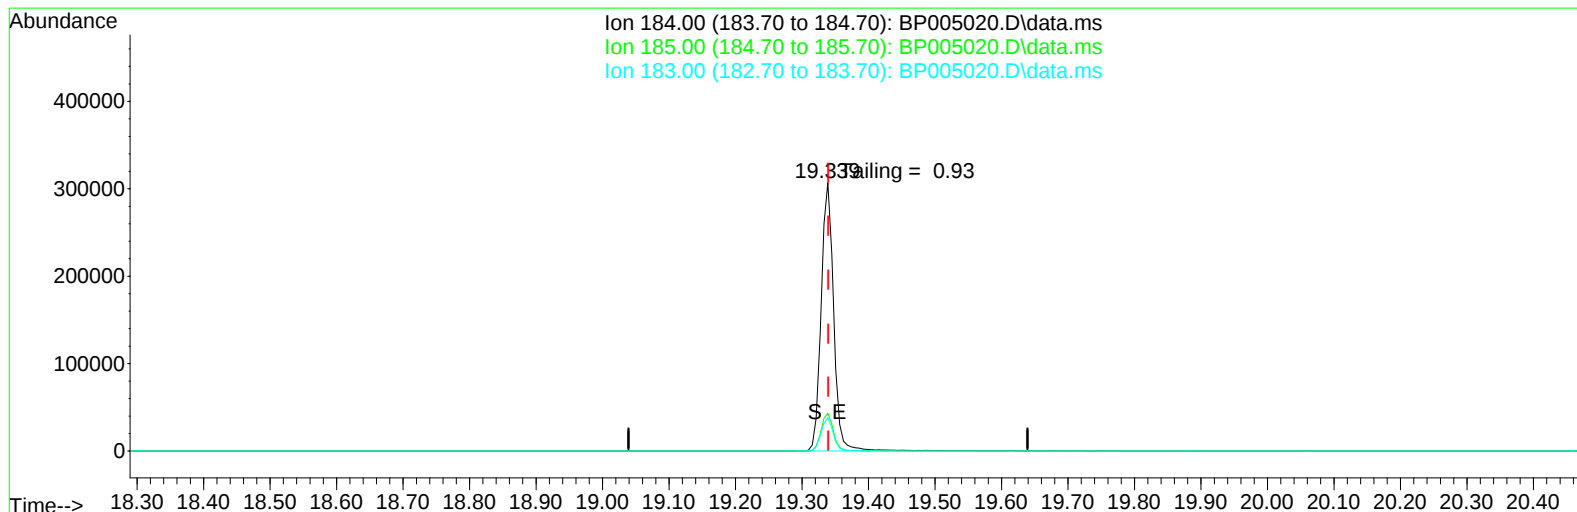

TIC: BP005020.D\data.ms

(77) Benzidine

19.339min (-0.001) 2425852.84 ng

response 402669

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.08
183.00	12.00	12.47
0.00	0.00	0.00

DDT Breakdown

Instrument :
BNA_P
ClientSampleId :
DFTPP

Date	Instrument Name	DFTPP Data File
03/23/2021	BNA_P	BP005020.D
Compound Name	Response	Retention Time
DDT	232814	20.53
DDD	2151	20.1
DDE	659	19.61
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
2810	235624	1.19