
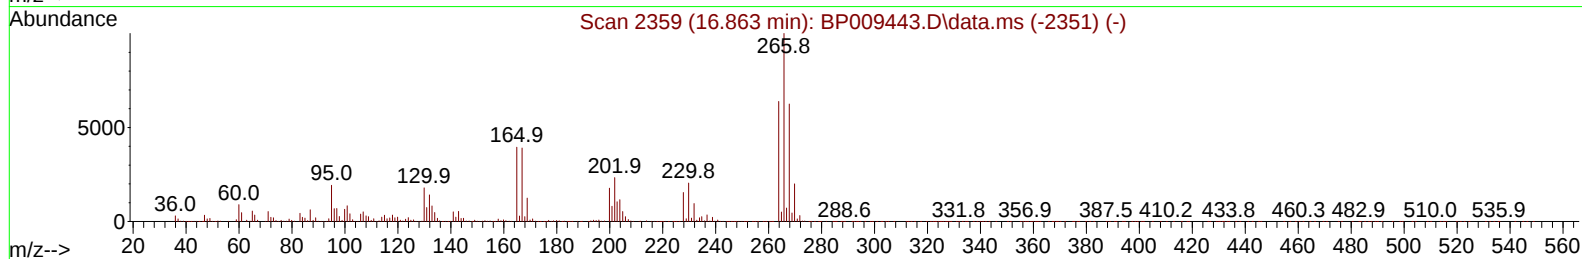
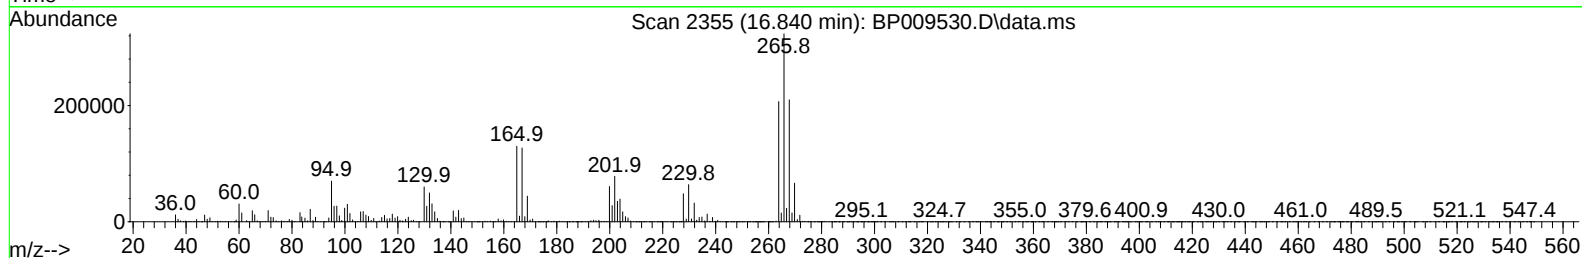


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032422\
Data File : BP009530.D
Acq On : 24 Mar 2022 15:34
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 25 07:45:37 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 25 06:34:38 2022
Response via : Initial Calibration

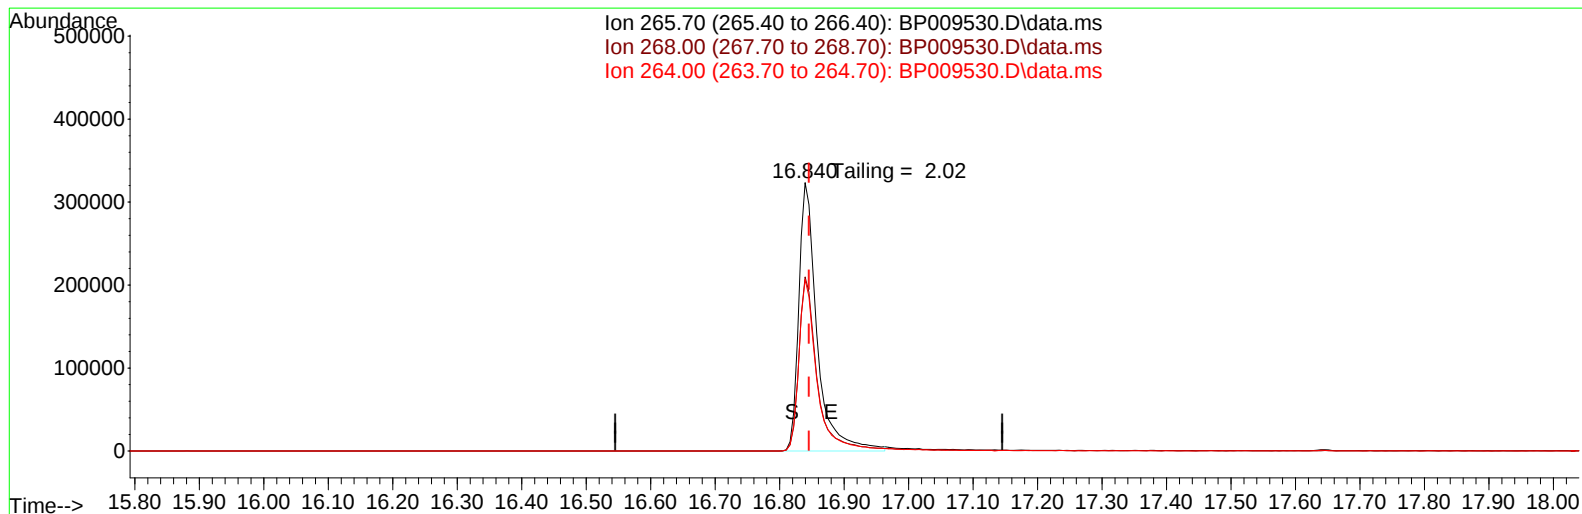

TIC: BP009530.D\data.ms

(70) Pentachlorophenol (C)




16.840min (-0.006) 108376.42 ng

response 650258

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.30	64.86
264.00	63.60	63.93
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032422\
 Data File : BP009530.D
 Acq On : 24 Mar 2022 15:34
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 25 07:45:37 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031722.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Mar 25 06:34:38 2022
 Response via : Initial Calibration

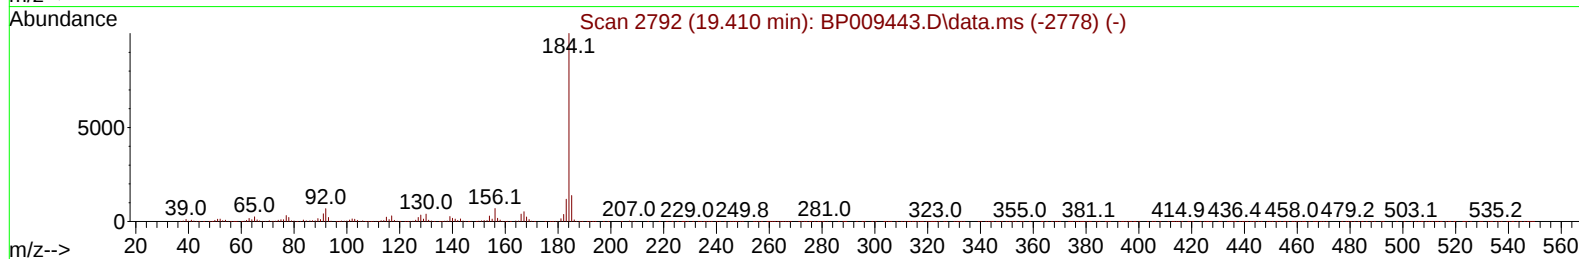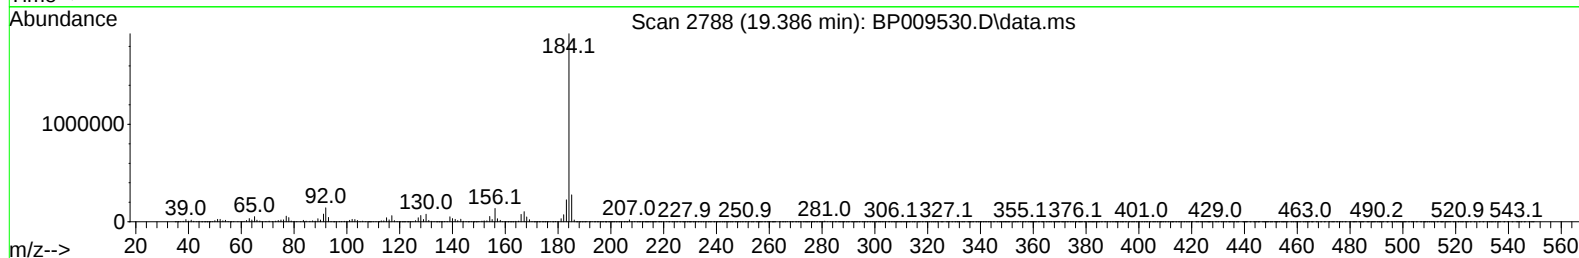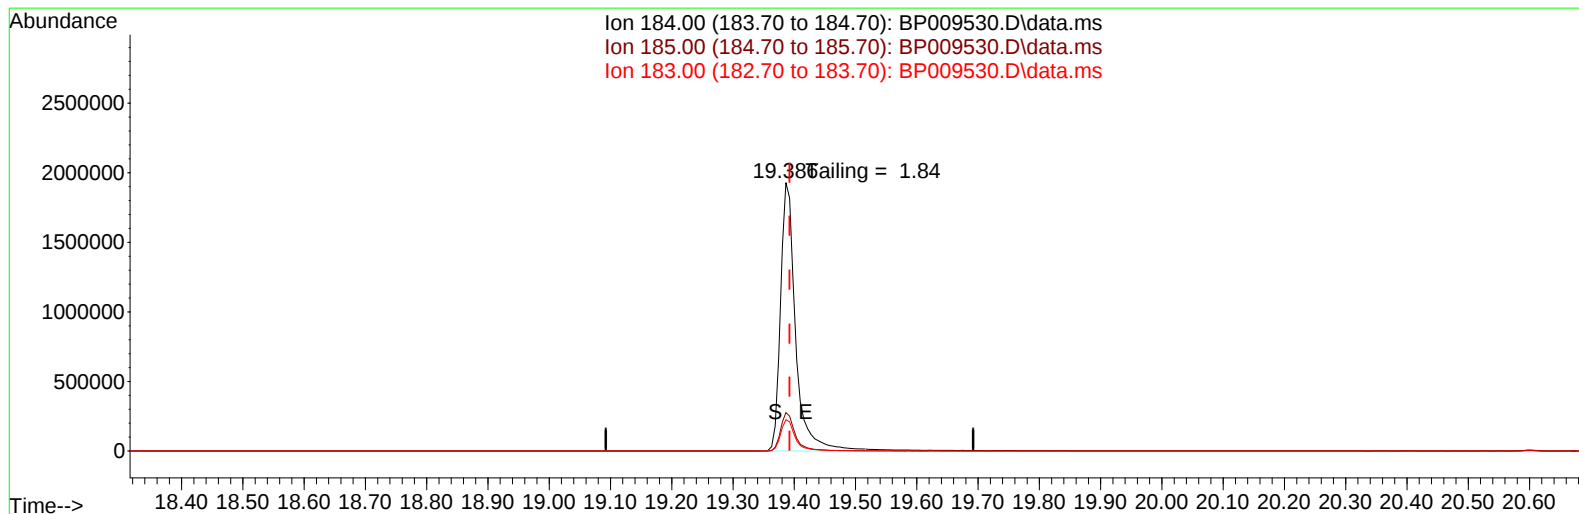

TIC: BP009530.D\data.ms

(77) Benzidine**19.386min (-0.006) 32241.54 ng****response 3364234**

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.32
183.00	11.70	11.68
0.00	0.00	0.00