

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032422\
 Data File : BP009538.D
 Acq On : 24 Mar 2022 20:07
 Operator : CG/JU
 Sample : N2090-22
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 FB032122

Quant Time: Mar 25 06:55:10 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031722.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Mar 25 06:34:38 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.769	152	253229	20.000	ng	0.00
21) Naphthalene-d8	10.563	136	977622	20.000	ng	0.00
39) Acenaphthene-d10	14.416	164	601906	20.000	ng	0.00
64) Phenanthrene-d10	17.181	188	1272704	20.000	ng	0.00
76) Chrysene-d12	21.292	240	1401685	20.000	ng	0.00
86) Perylene-d12	23.686	264	1565201	20.000	ng	0.00
System Monitoring Compounds						
5) 2-Fluorophenol	5.375	112	1018483	70.221	ng	0.00
7) Phenol-d6	6.964	99	724712	36.948	ng	0.00
23) Nitrobenzene-d5	8.928	82	1865240	101.389	ng	0.00
42) 2,4,6-Tribromophenol	15.916	330	1295780	130.459	ng	0.00
45) 2-Fluorobiphenyl	13.040	172	4376371	100.795	ng	0.00
79) Terphenyl-d14	19.763	244	7335795	93.937	ng	0.00


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032422\
Data File : BP009538.D
Acq On : 24 Mar 2022 20:07
Operator : CG/JU
Sample : N2090-22
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
FB032122

Quant Time: Mar 25 06:55:10 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 25 06:34:38 2022
Response via : Initial Calibration




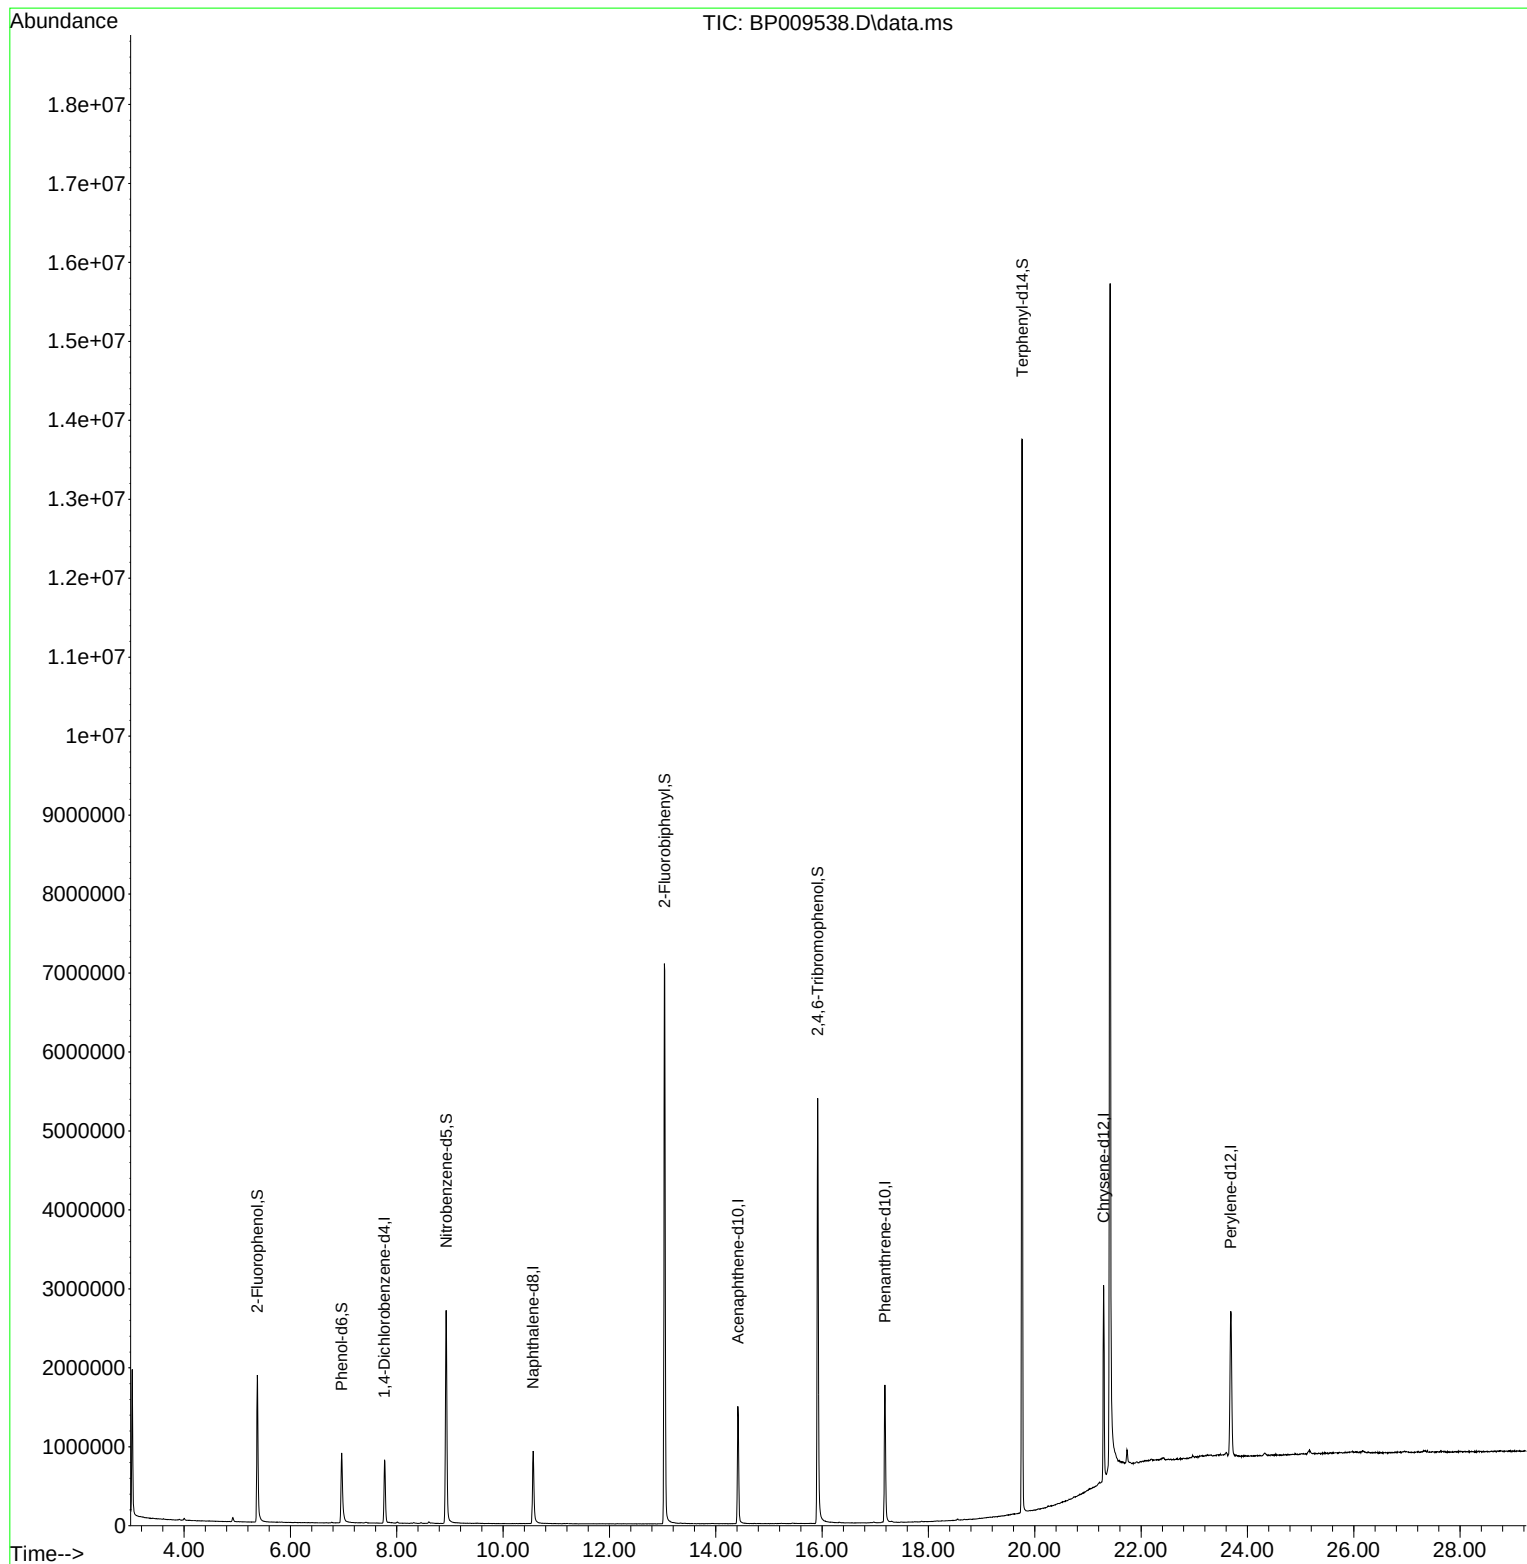


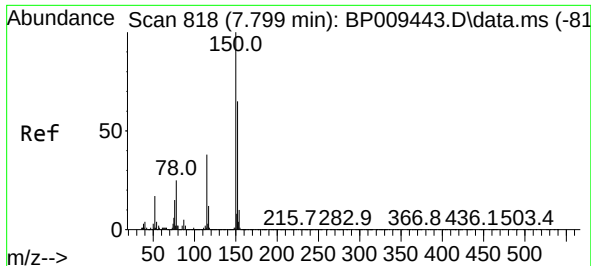

#1
 1,4-Dichlorobenzene-d4
 Concen: 20.000 ng
 RT: 7.769 min Scan# 81
 Delta R.T. -0.006 min
 Lab File: BP009538.D
 Acq: 24 Mar 2022 20:07




Instrument :
 BNA_P
 ClientSampleId :
 FB032122


Tgt Ion:152 Resp: 253229
 Ion Ratio Lower Upper
 152 100
 150 155.4 124.5 186.7
 115 58.1 48.2 72.4

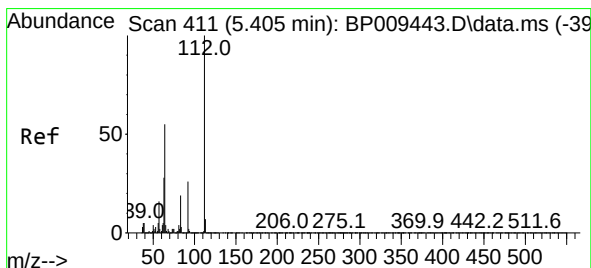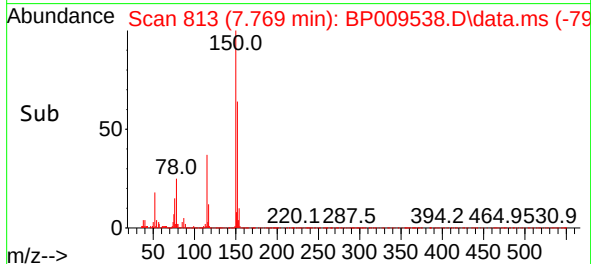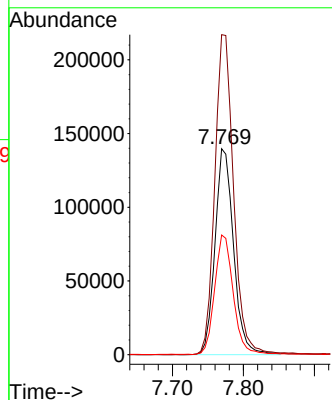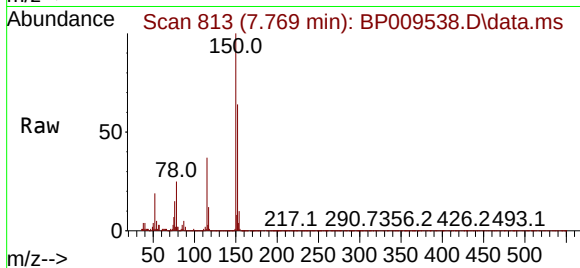

#5
 2-Fluorophenol
 Concen: 70.221 ng
 RT: 5.375 min Scan# 406
 Delta R.T. -0.000 min
 Lab File: BP009538.D
 Acq: 24 Mar 2022 20:07

Tgt Ion:112 Resp: 1018483
 Ion Ratio Lower Upper
 112 100
 64 54.2 45.0 67.4
 63 28.3 23.0 34.6


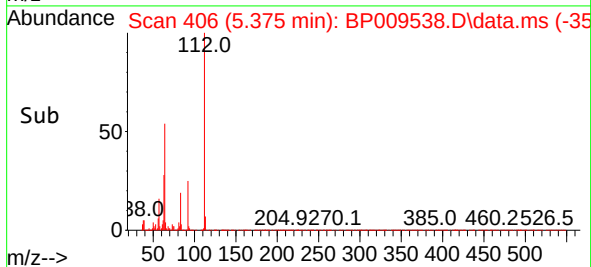
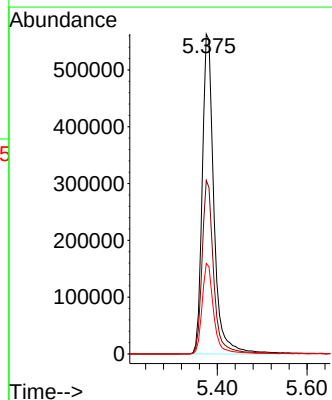
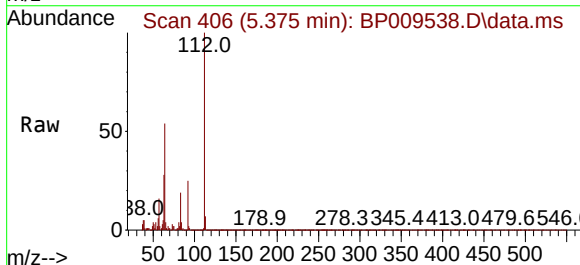


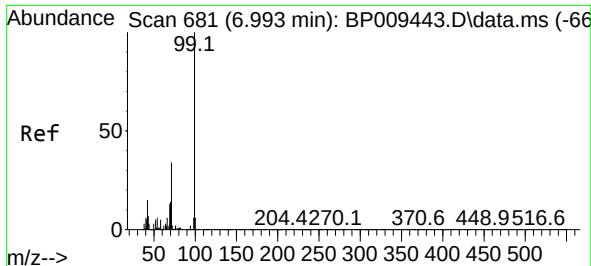

#7
Phenol-d6
Concen: 36.948 ng
RT: 6.964 min Scan# 61
Delta R.T. -0.000 min
Lab File: BP009538.D
Acq: 24 Mar 2022 20:07




Instrument :
BNA_P
ClientSampleId :
FB032122


Tgt Ion: 99 Resp: 724712
Ion Ratio Lower Upper
99 100
42 15.8 12.8 19.2
71 32.2 26.3 39.5

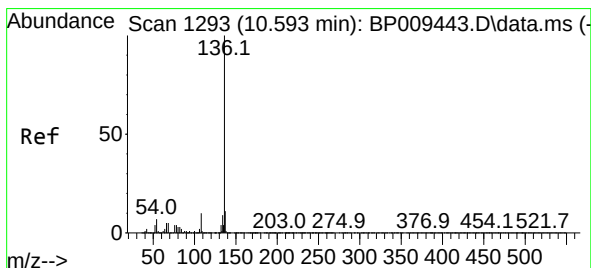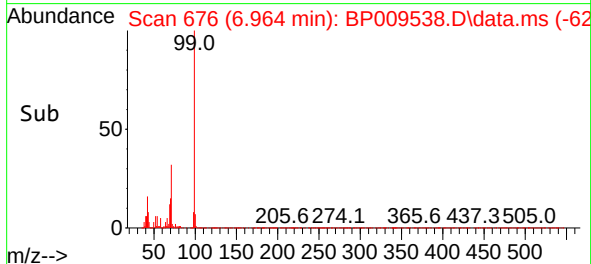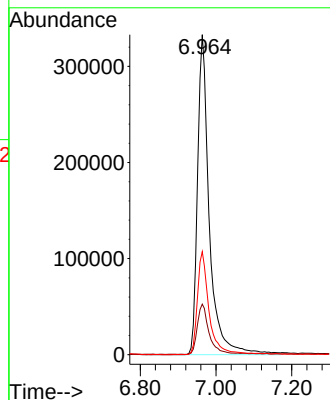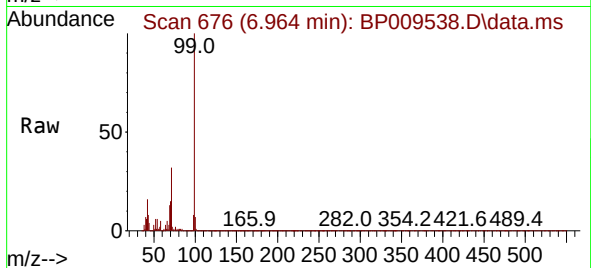

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.563 min Scan# 1288
Delta R.T. -0.000 min
Lab File: BP009538.D
Acq: 24 Mar 2022 20:07

Tgt Ion: 136 Resp: 977622
Ion Ratio Lower Upper
136 100
137 11.3 8.6 12.8
54 7.0 5.8 8.8
68 6.2 5.2 7.8


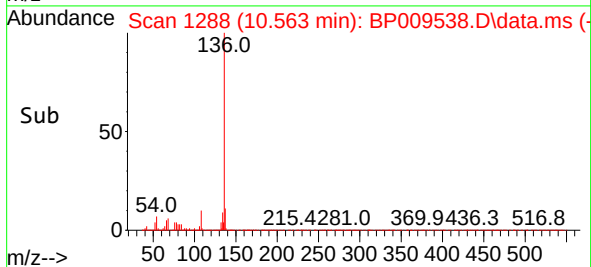
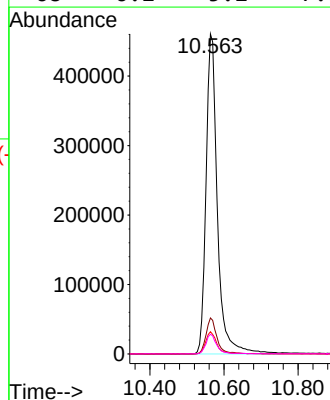
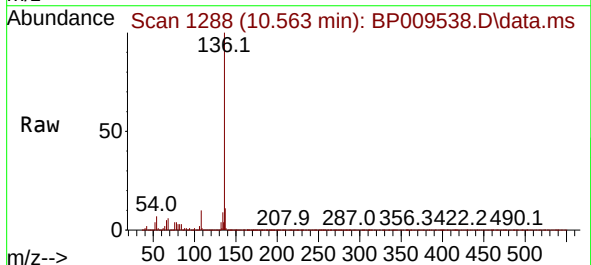


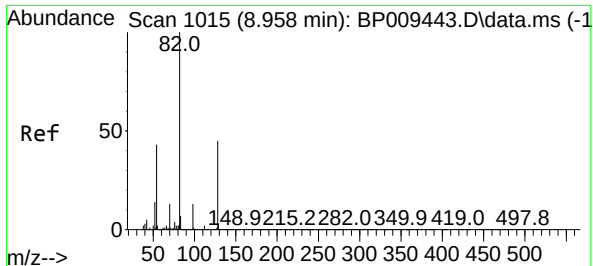

#23
Nitrobenzene-d5
Concen: 101.389 ng
RT: 8.928 min Scan# 1010
Delta R.T. -0.006 min
Lab File: BP009538.D
Acq: 24 Mar 2022 20:07




Instrument :
BNA_P
ClientSampleId :
FB032122


Tgt Ion: 82 Resp: 1865240
Ion Ratio Lower Upper
82 100
128 44.4 34.2 51.4
54 43.2 34.7 52.1

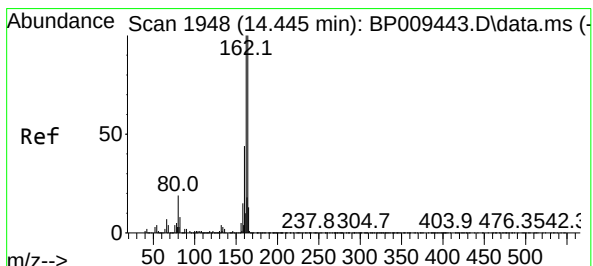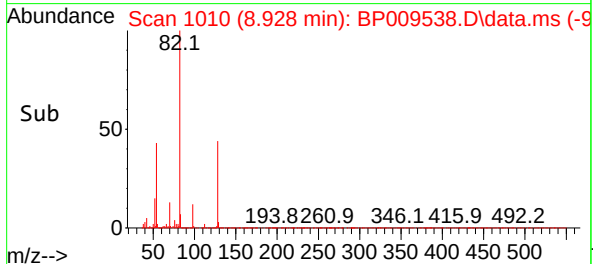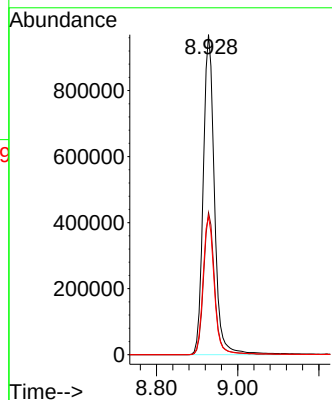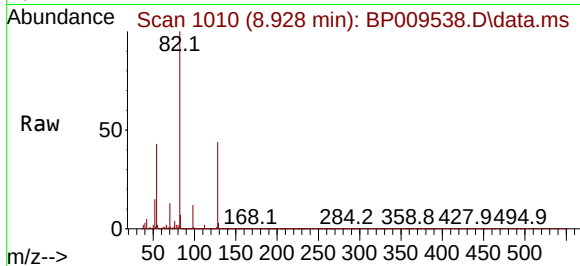

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.416 min Scan# 1943
Delta R.T. -0.006 min
Lab File: BP009538.D
Acq: 24 Mar 2022 20:07

Tgt Ion:164 Resp: 601906
Ion Ratio Lower Upper
164 100
162 101.3 79.1 118.7
160 44.7 34.9 52.3


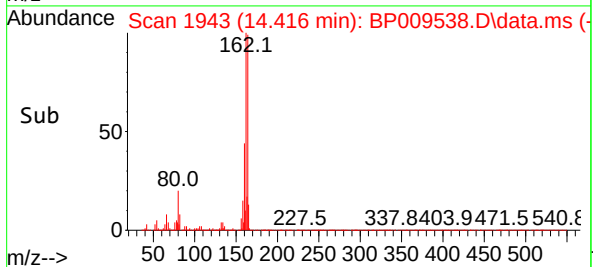
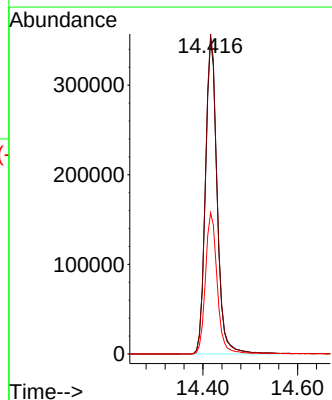
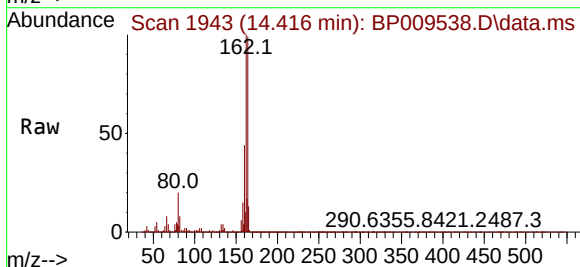


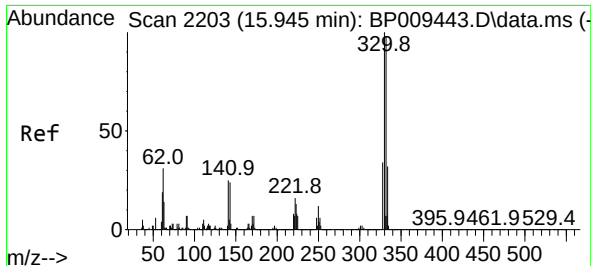

#42
2,4,6-Tribromophenol
Concen: 130.459 ng
RT: 15.916 min Scan# 21
Delta R.T. -0.006 min
Lab File: BP009538.D
Acq: 24 Mar 2022 20:07




Instrument :
BNA_P
ClientSampleId :
FB032122


Tgt Ion:330 Resp: 1295780
Ion Ratio Lower Upper
330 100
332 96.6 77.0 115.6
141 29.2 27.6 41.4

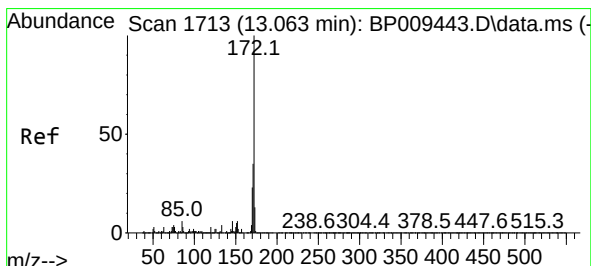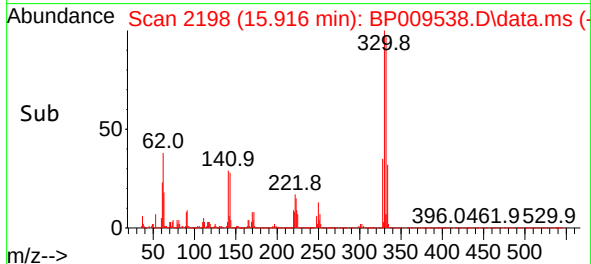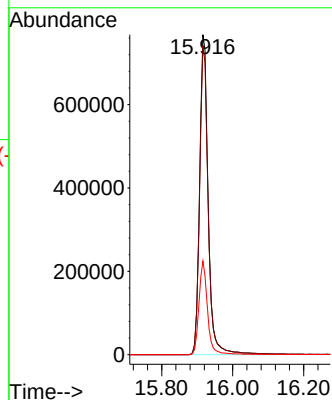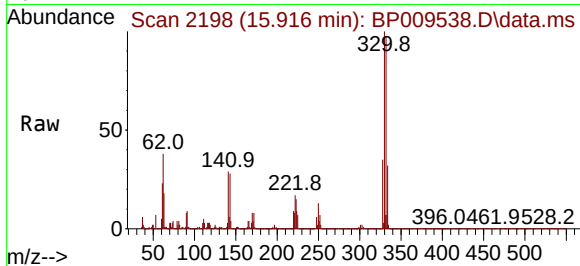

#45
2-Fluorobiphenyl
Concen: 100.795 ng
RT: 13.040 min Scan# 1709
Delta R.T. -0.000 min
Lab File: BP009538.D
Acq: 24 Mar 2022 20:07

Tgt Ion:172 Resp: 4376371
Ion Ratio Lower Upper
172 100
171 35.0 28.0 42.0
170 23.5 18.6 27.8


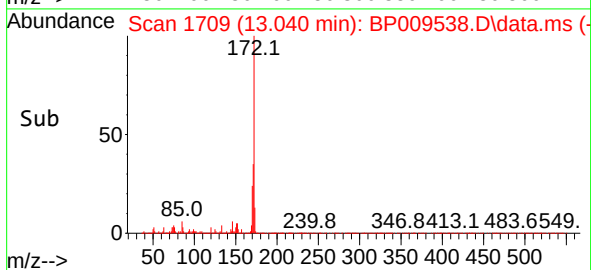
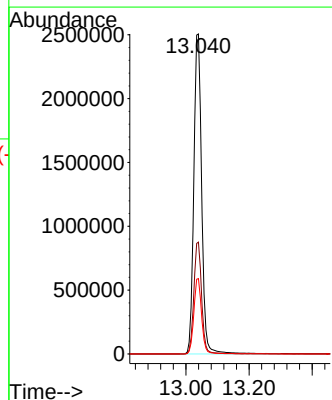
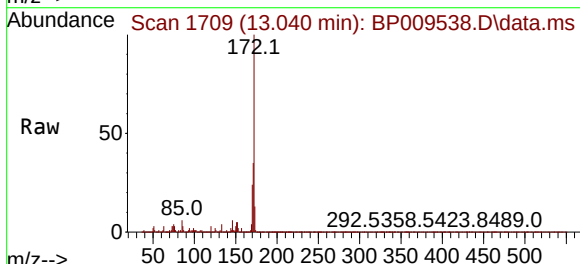


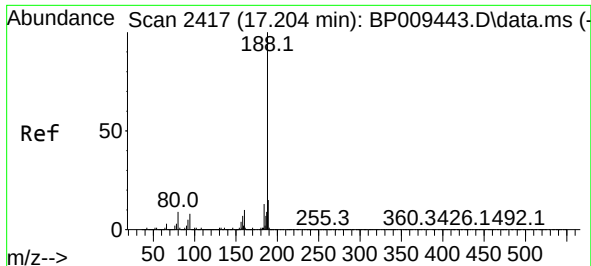

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.181 min Scan# 2417
Delta R.T. -0.006 min
Lab File: BP009538.D
Acq: 24 Mar 2022 20:07




Instrument :
BNA_P
ClientSampleId :
FB032122


Tgt Ion:188 Resp: 1272704
Ion Ratio Lower Upper
188 100
94 8.6 7.9 11.9
80 9.7 8.8 13.2

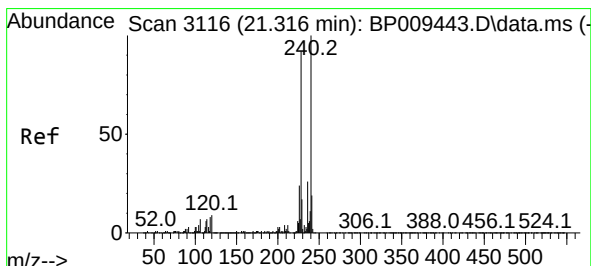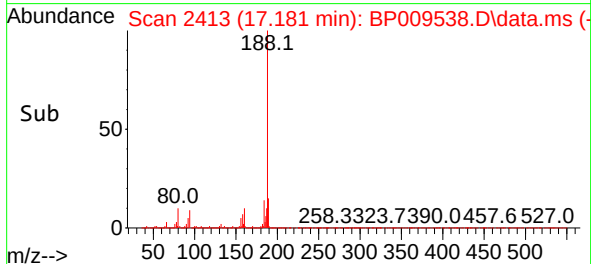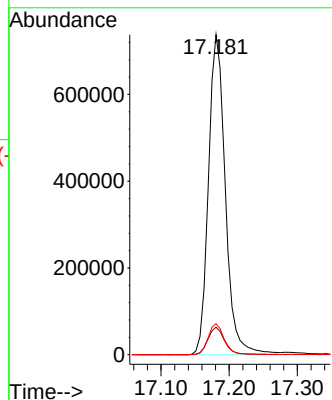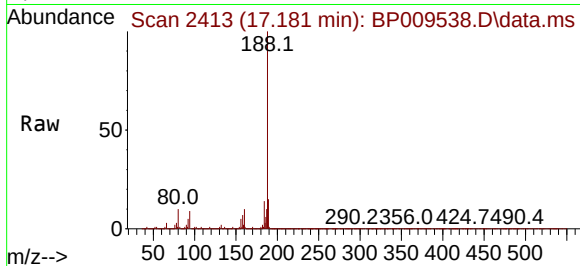

#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.292 min Scan# 3112
Delta R.T. -0.006 min
Lab File: BP009538.D
Acq: 24 Mar 2022 20:07

Tgt Ion:240 Resp: 1401685
Ion Ratio Lower Upper
240 100
120 9.8 9.0 13.4
236 25.5 20.6 30.8


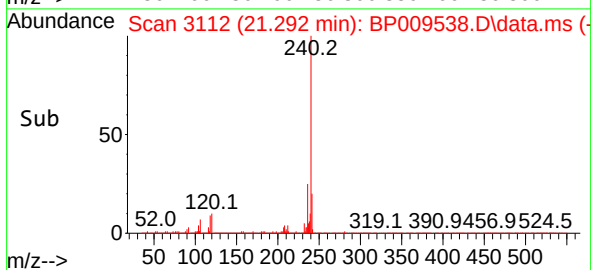
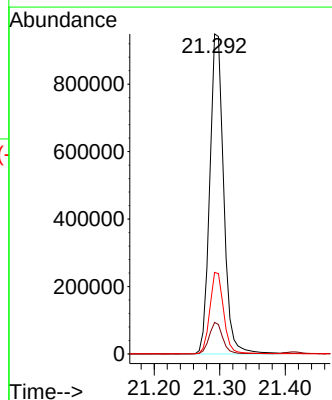
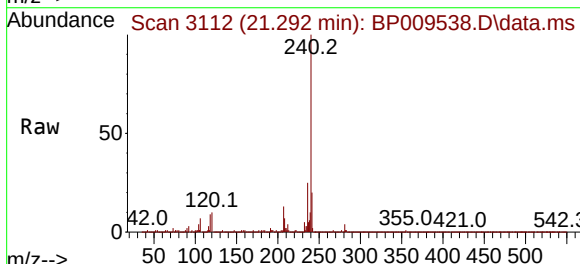


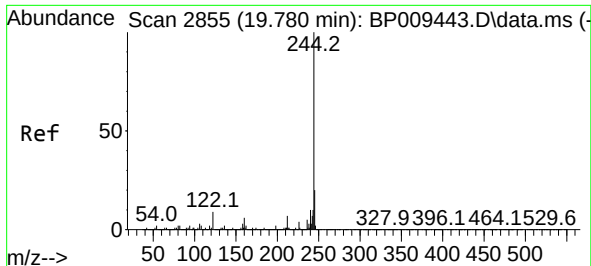

#79
 Terphenyl-d14
 Concen: 93.937 ng
 RT: 19.763 min Scan# 21
 Delta R.T. -0.000 min
 Lab File: BP009538.D
 Acq: 24 Mar 2022 20:07

Instrument :
 BNA_P
 ClientSampleId :
 FB032122

Tgt Ion:244 Resp: 7335795
 Ion Ratio Lower Upper
 244 100
 212 7.1 5.8 8.6
 122 9.1 8.3 12.5

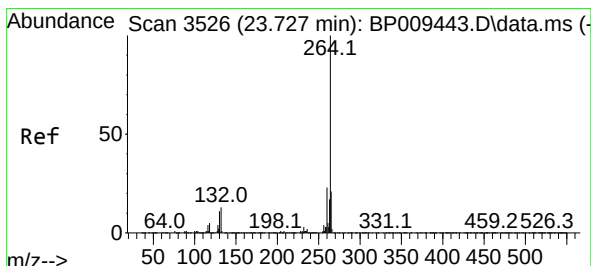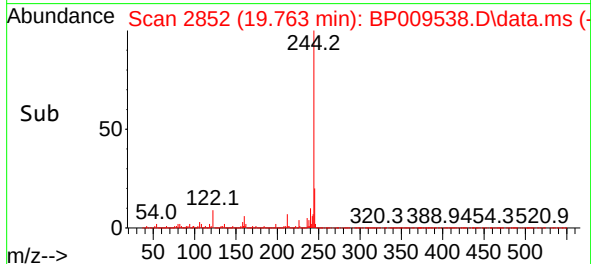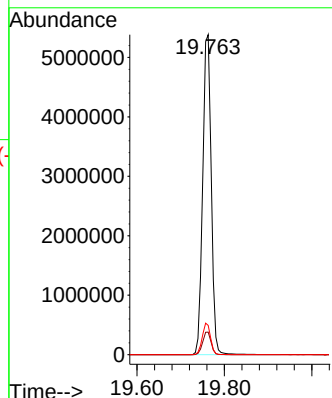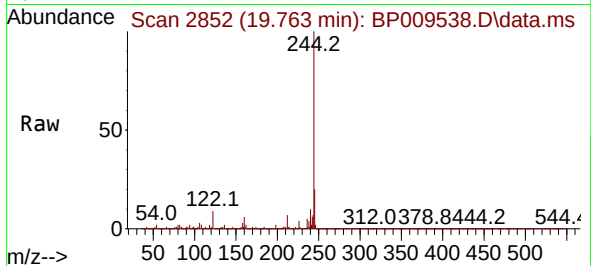

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 23.686 min Scan# 3519
 Delta R.T. -0.006 min
 Lab File: BP009538.D
 Acq: 24 Mar 2022 20:07

Tgt Ion:264 Resp: 1565201
 Ion Ratio Lower Upper
 264 100
 260 24.2 19.4 29.0
 265 21.6 17.2 25.8

