

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032422\
 Data File : BP009532.D
 Acq On : 24 Mar 2022 16:42
 Operator : CG/JU
 Sample : PB143484BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 PB143484BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031722.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BP009532.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.381	400	407	432	rBV	6293906	10839492	50.19%	10.448%
2	6.963	668	676	704	rBV	5985351	10912509	50.53%	10.519%
3	7.775	806	814	826	rBV	1256070	2237350	10.36%	2.157%
4	8.928	1002	1010	1032	rBV	3812941	7317419	33.88%	7.053%
5	10.569	1278	1289	1312	rBV	1441518	3077526	14.25%	2.967%
6	13.040	1701	1709	1736	rBV	10829094	17933263	83.03%	17.286%
7	14.416	1935	1943	1959	rBV	2431733	4115307	19.05%	3.967%
8	15.916	2190	2198	2227	rBV	7762845	13248657	61.34%	12.771%
9	17.181	2406	2413	2428	rBV	2745816	4598195	21.29%	4.432%
10	19.763	2846	2852	2869	rBV	16194135	21597774	100.00%	20.819%
11	21.298	3108	3113	3126	rBV	2720332	4097993	18.97%	3.950%
12	23.692	3513	3520	3534	rVB2	1597029	3766779	17.44%	3.631%




Sum of corrected areas: 103742264

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032422\
Data File : BP009532.D
Acq On : 24 Mar 2022 16:42
Operator : CG/JU
Sample : PB143484BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB143484BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

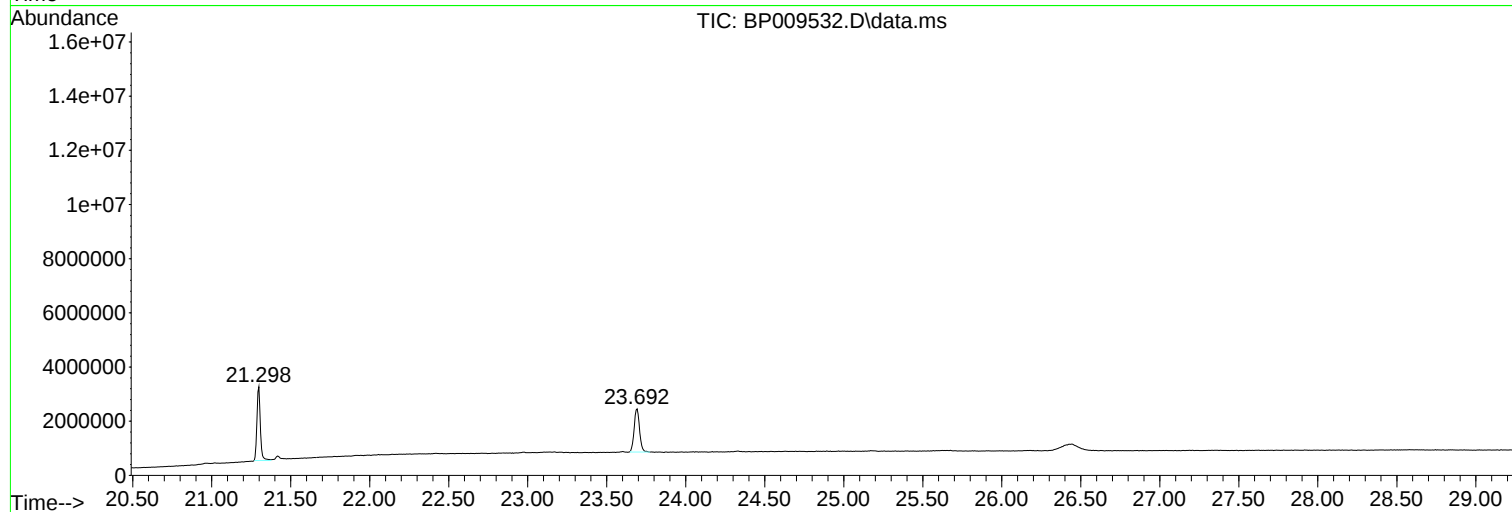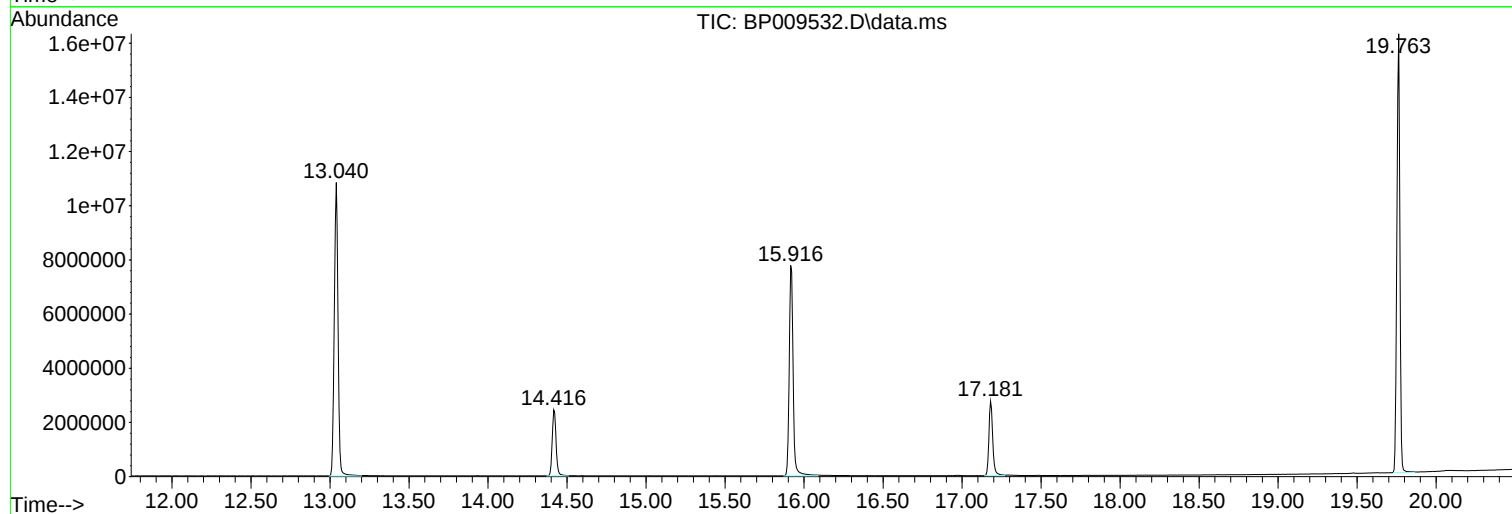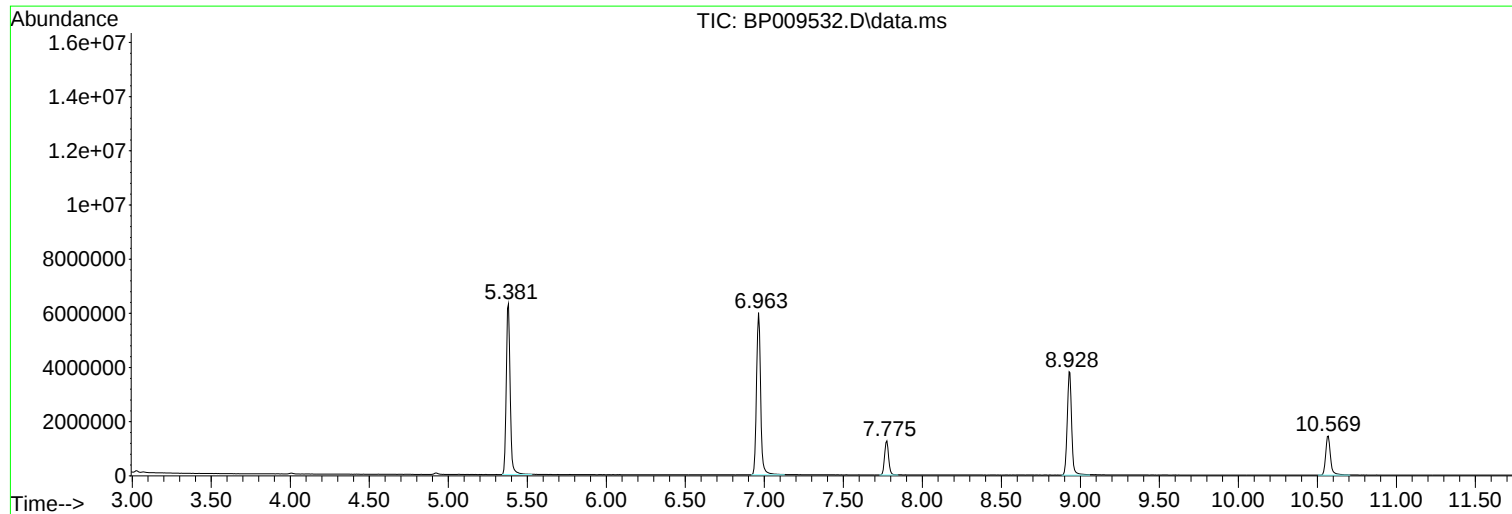

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032422\
Data File : BP009532.D
Acq On : 24 Mar 2022 16:42
Operator : CG/JU
Sample : PB143484BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB143484BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032422\
Data File : BP009532.D
Acq On : 24 Mar 2022 16:42
Operator : CG/JU
Sample : PB143484BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
PB143484BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------