
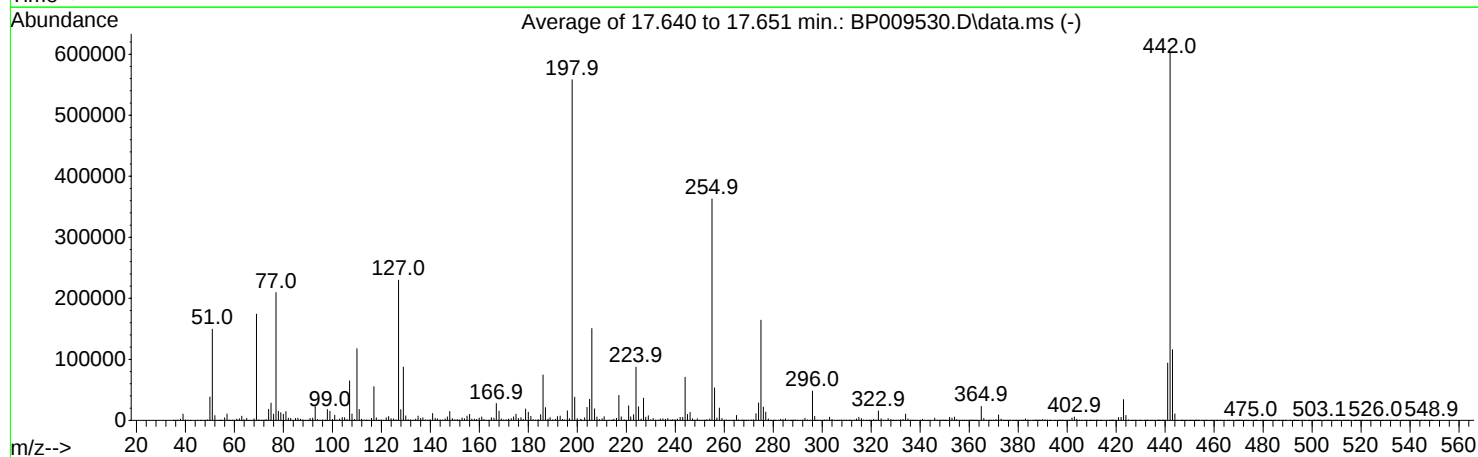


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032422\
 Data File : BP009530.D
 Acq On : 24 Mar 2022 15:34
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031722.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Fri Mar 25 06:34:38 2022

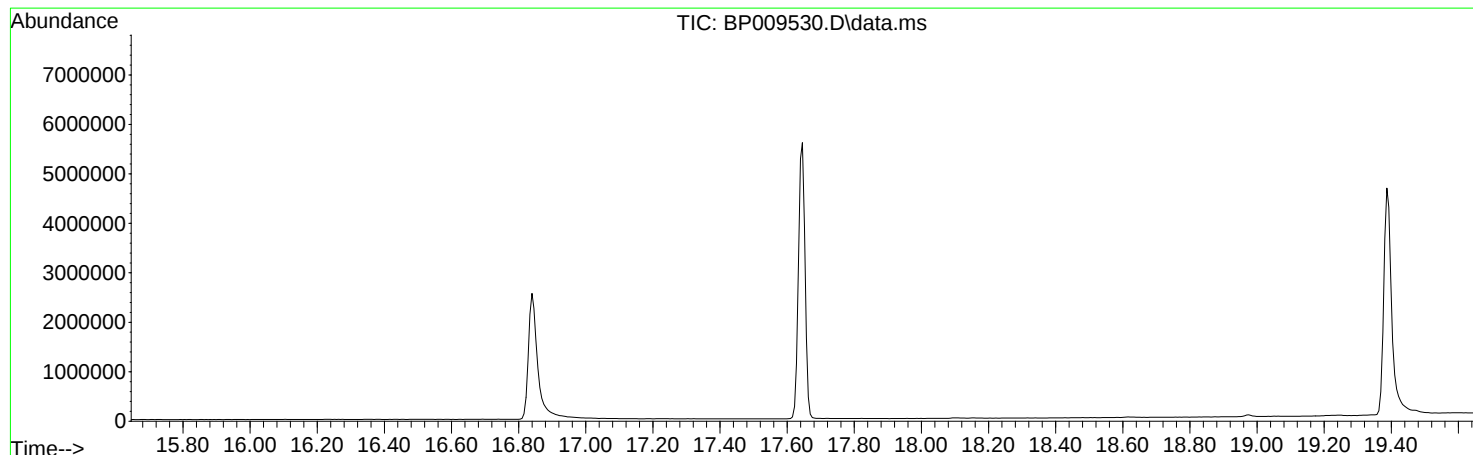




AutoFind: Scans 2491, 2492, 2493; Background Corrected with Scan 2483

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	26.8	149491	PASS
68	69	0.00	2	1.6	2778	PASS
69	198	0.00	100	31.2	173984	PASS
70	69	0.00	2	0.6	1013	PASS
127	198	10	80	41.2	229736	PASS
197	198	0.00	2	0.5	2853	PASS
198	198	100	100	100.0	558234	PASS
199	198	5	9	6.8	38063	PASS
275	198	10	60	29.4	164053	PASS
365	198	1	100	4.1	22873	PASS
441	198	0.01	100	16.8	93955	PASS
442	442	100	100	100.0	602795	PASS
443	442	15	24	19.2	115883	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032422\
Data File : BP009530.D
Acq On : 24 Mar 2022 15:34
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
DFTPP

Quant Time: Mar 25 07:45:37 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031722.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Fri Mar 25 06:34:38 2022
Response via : Initial Calibration

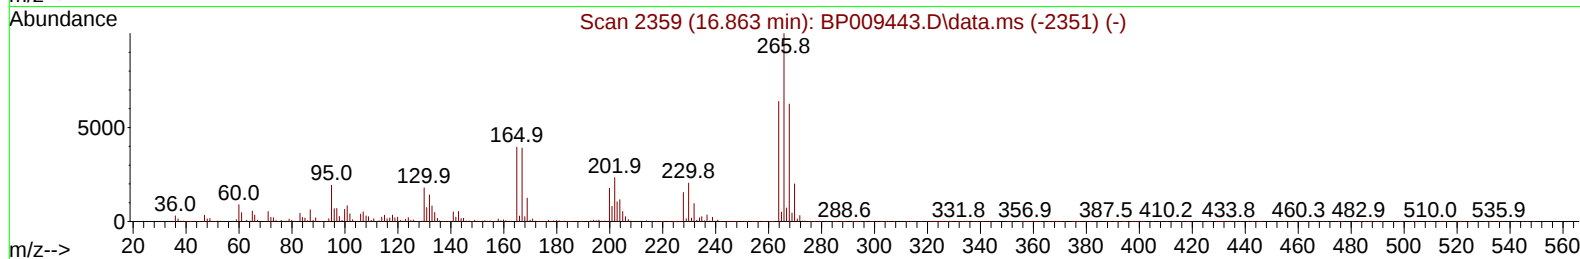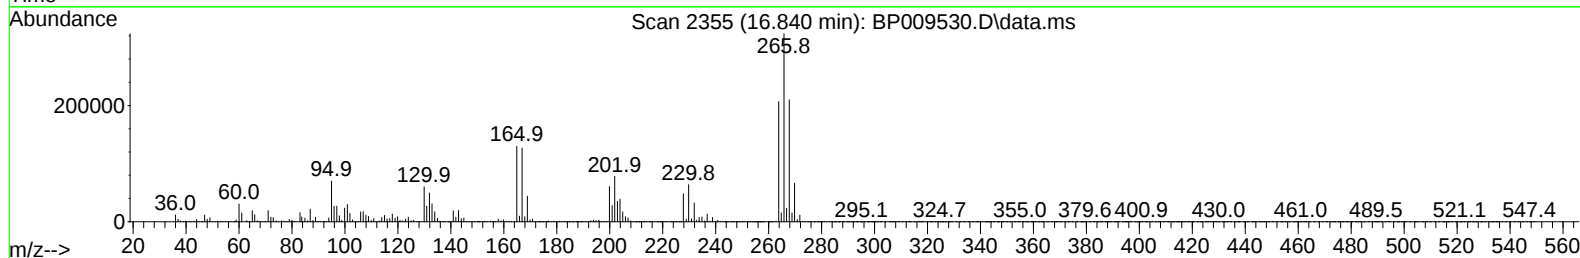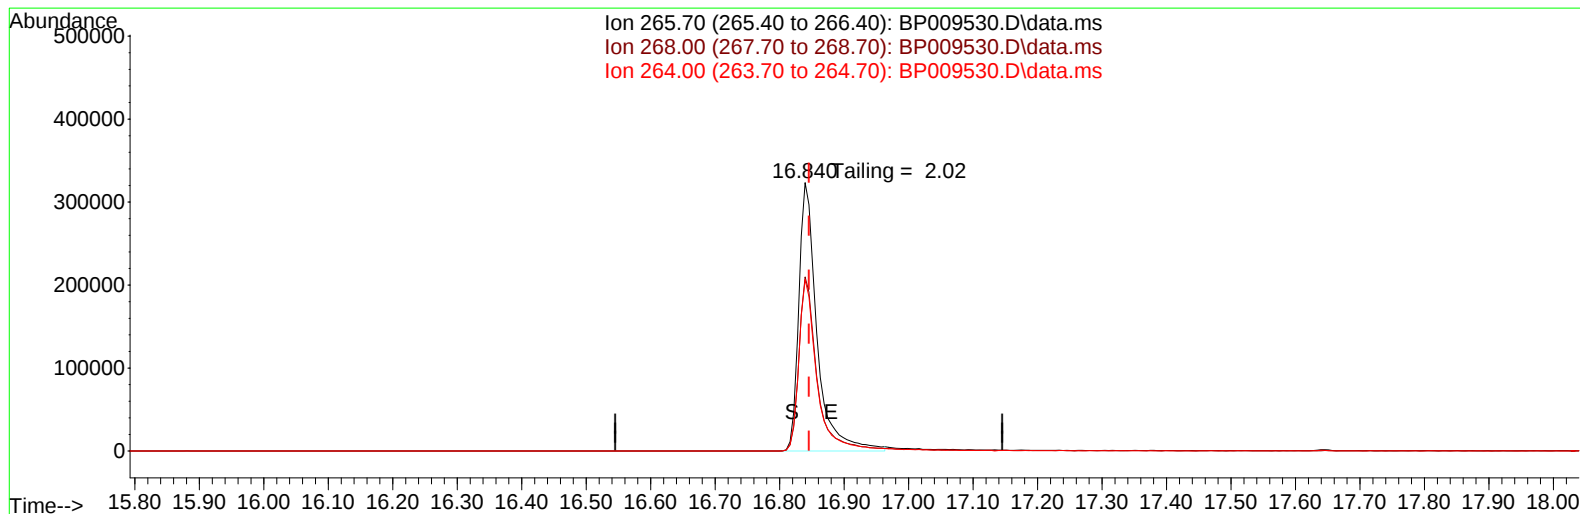

TIC: BP009530.D\data.ms

(70) Pentachlorophenol (C)

16.840min (-0.006) 108376.42 ng




response 650258

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.30	64.86
264.00	63.60	63.93
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032422\
 Data File : BP009530.D
 Acq On : 24 Mar 2022 15:34
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Mar 25 07:45:37 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP031722.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Fri Mar 25 06:34:38 2022
 Response via : Initial Calibration

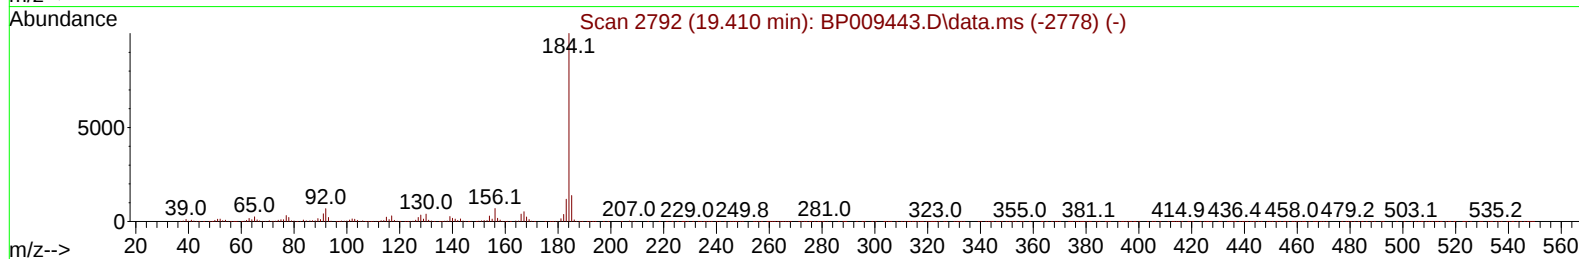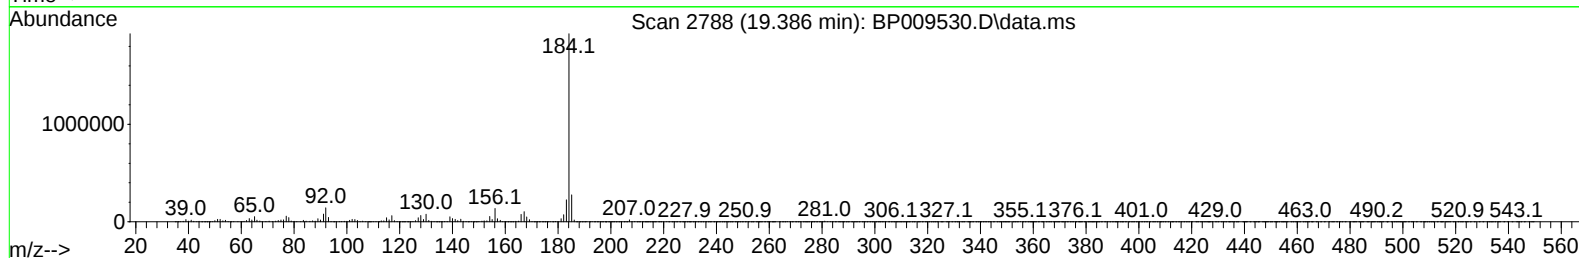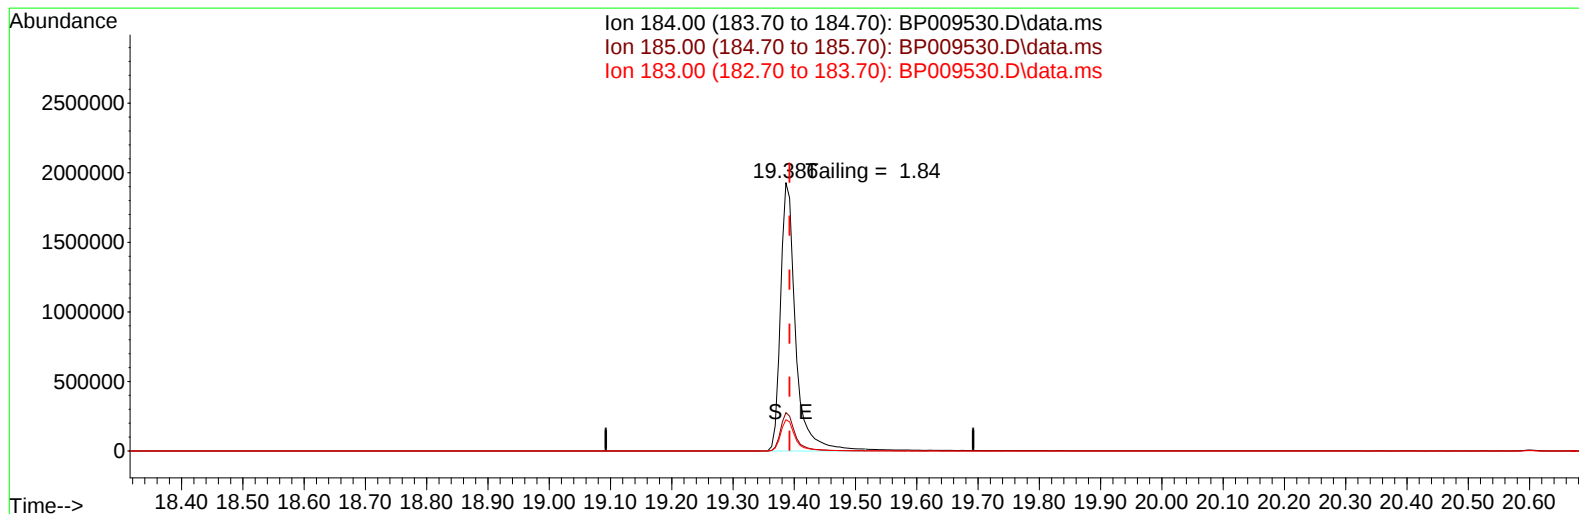

TIC: BP009530.D\data.ms

(77) Benzidine

19.386min (-0.006) 32241.54 ng

response 3364234

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	14.32
183.00	11.70	11.68
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/24/2022	BNA_P	BP009530.D
Compound Name	Response	Retention Time
DDT	1974829	20.604
DDD	28986	20.169
DDE	2658	19.675
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
31644	2006473	1.58

Instrument :
BNA_P
ClientSampleId :
DFTPP