
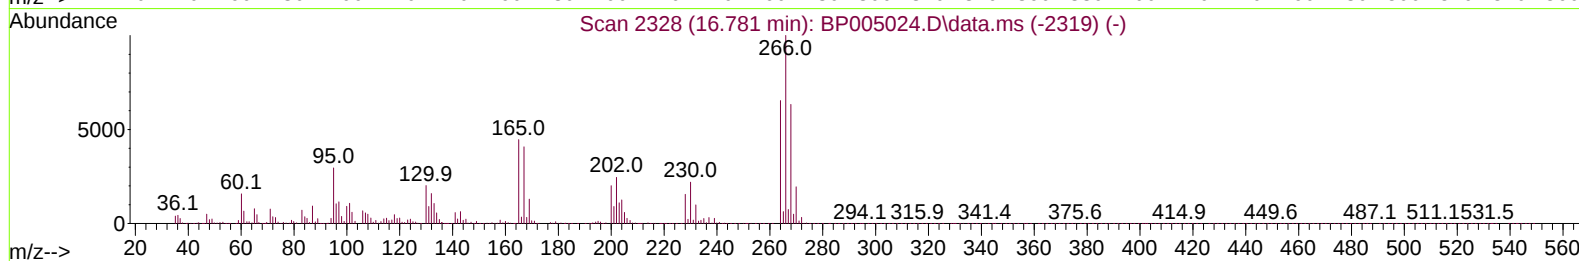
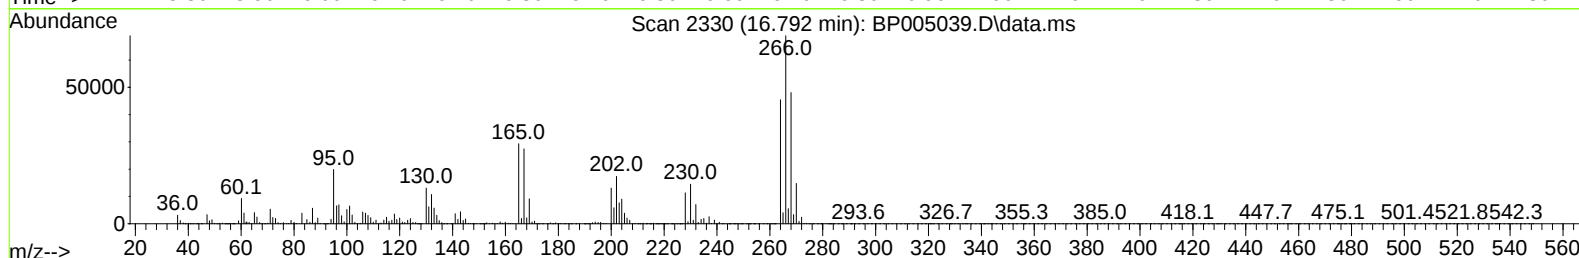


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032521\
 Data File : BP005039.D
 Acq On : 25 Mar 2021 08:54
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 26 03:03:34 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP032321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 25 10:21:09 2021
 Response via : Initial Calibration

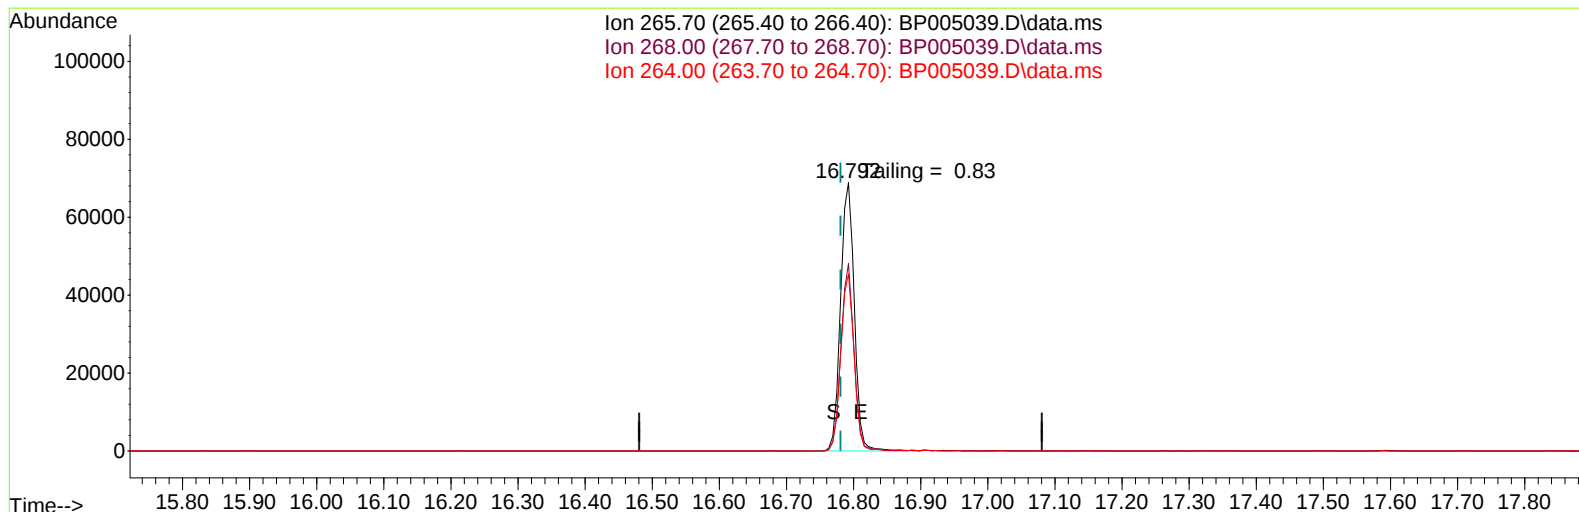

TIC: BP005039.D\data.ms

(70) Pentachlorophenol (C)




16.792min (+ 0.012) 98380.23 ng

response 98177

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.90	69.79
264.00	63.30	65.98
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032521\
Data File : BP005039.D
Acq On : 25 Mar 2021 08:54
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 26 03:03:34 2021
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP032321.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Thu Mar 25 10:21:09 2021
Response via : Initial Calibration

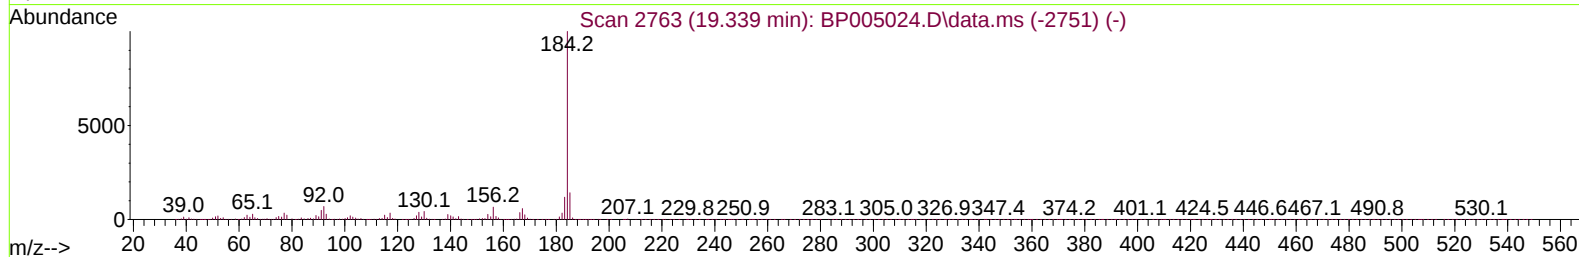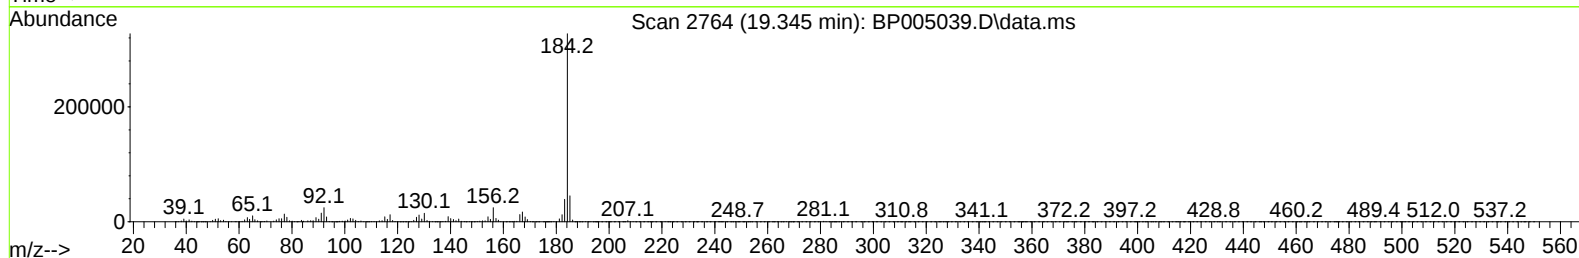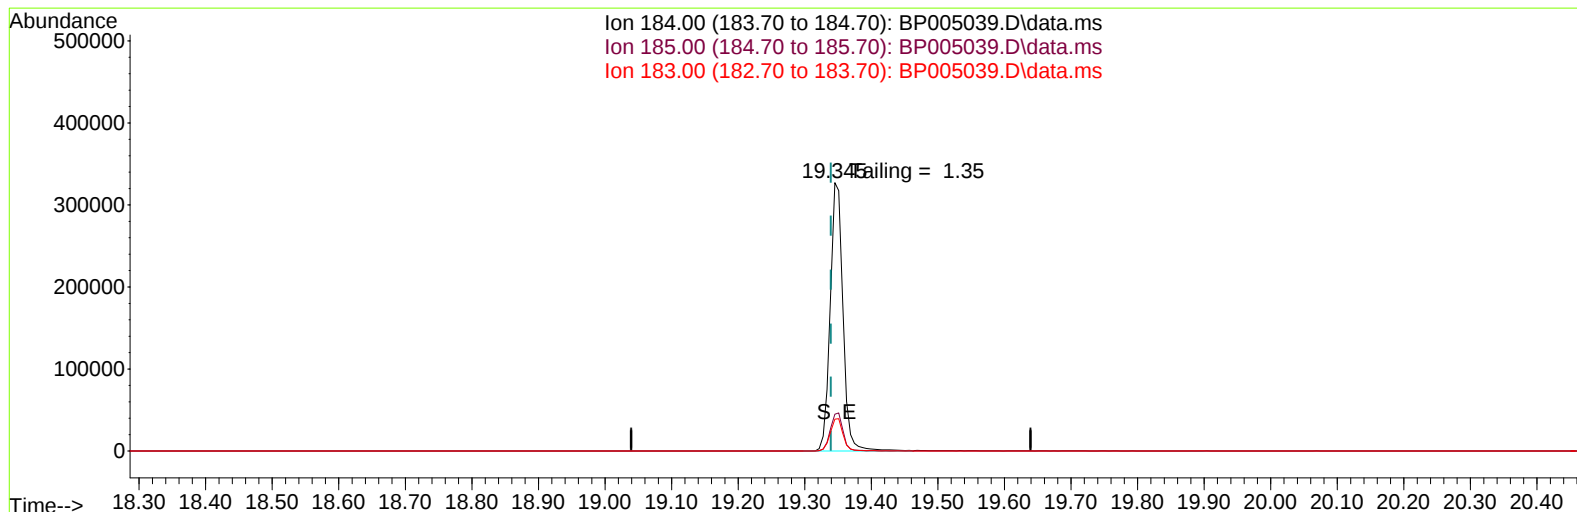

TIC: BP005039.D\data.ms

(77) Benzidine

19.345min (+ 0.006) 3949.39 ng

response 439405

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	13.76
183.00	12.00	11.88
0.00	0.00	0.00