
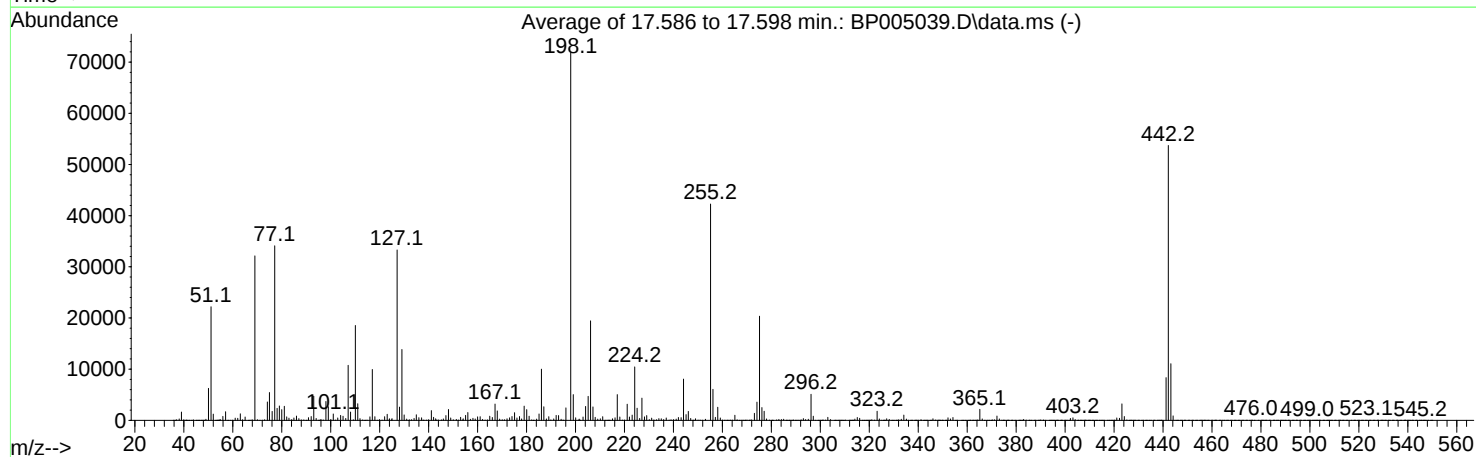


Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032521\
 Data File : BP005039.D
 Acq On : 25 Mar 2021 08:54
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP032321.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Mar 25 10:21:09 2021

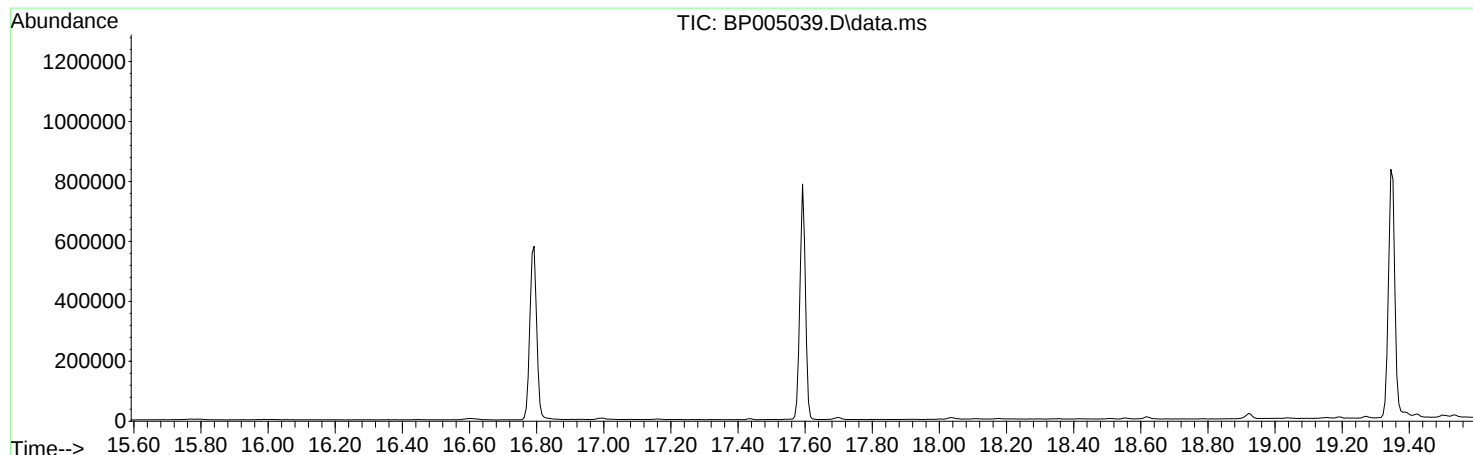




AutoFind: Scans 2465, 2466, 2467; Background Corrected with Scan 2458

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	30.9	22184	PASS
68	69	0.00	2	0.4	139	PASS
69	198	0.00	100	44.7	32137	PASS
70	69	0.00	2	0.4	129	PASS
127	198	10	80	46.3	33292	PASS
197	198	0.00	2	0.0	0	PASS
198	198	100	100	100.0	71875	PASS
199	198	5	9	7.0	5020	PASS
275	198	10	60	28.3	20343	PASS
365	198	1	100	3.0	2150	PASS
441	198	0.01	100	11.6	8361	PASS
442	442	100	100	100.0	53696	PASS
443	442	15	24	20.6	11060	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032521\
 Data File : BP005039.D
 Acq On : 25 Mar 2021 08:54
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Mar 26 03:03:34 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP032321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 25 10:21:09 2021
 Response via : Initial Calibration

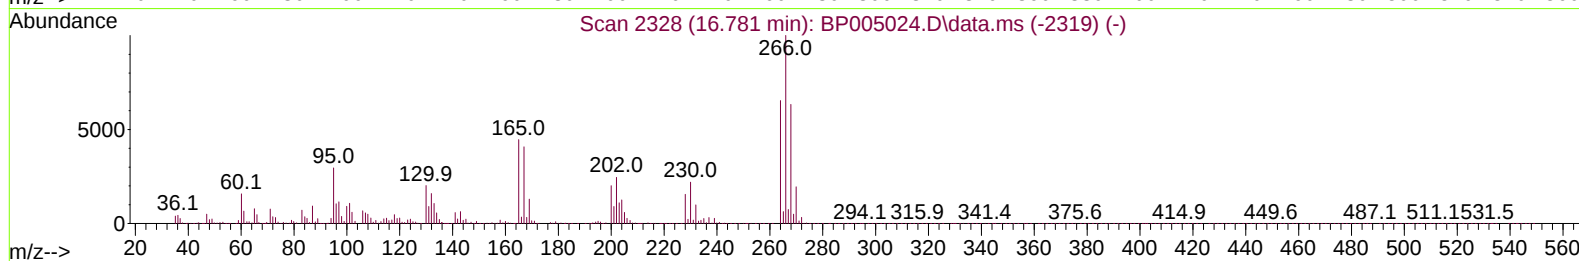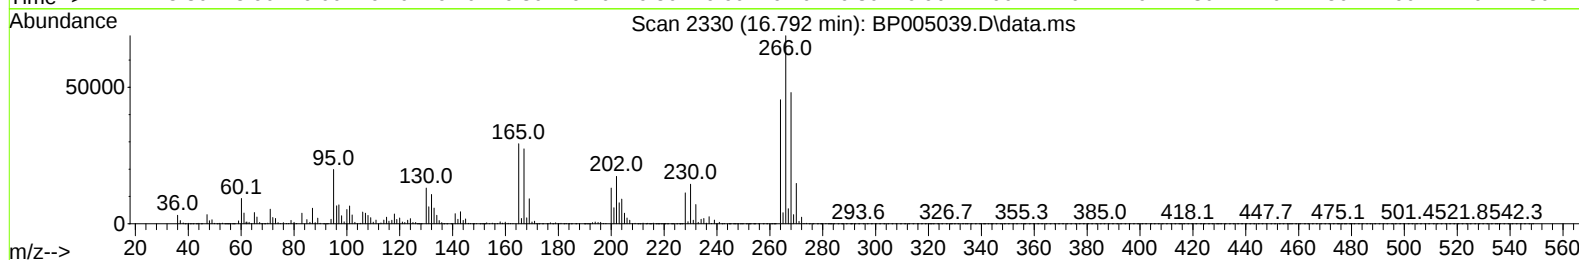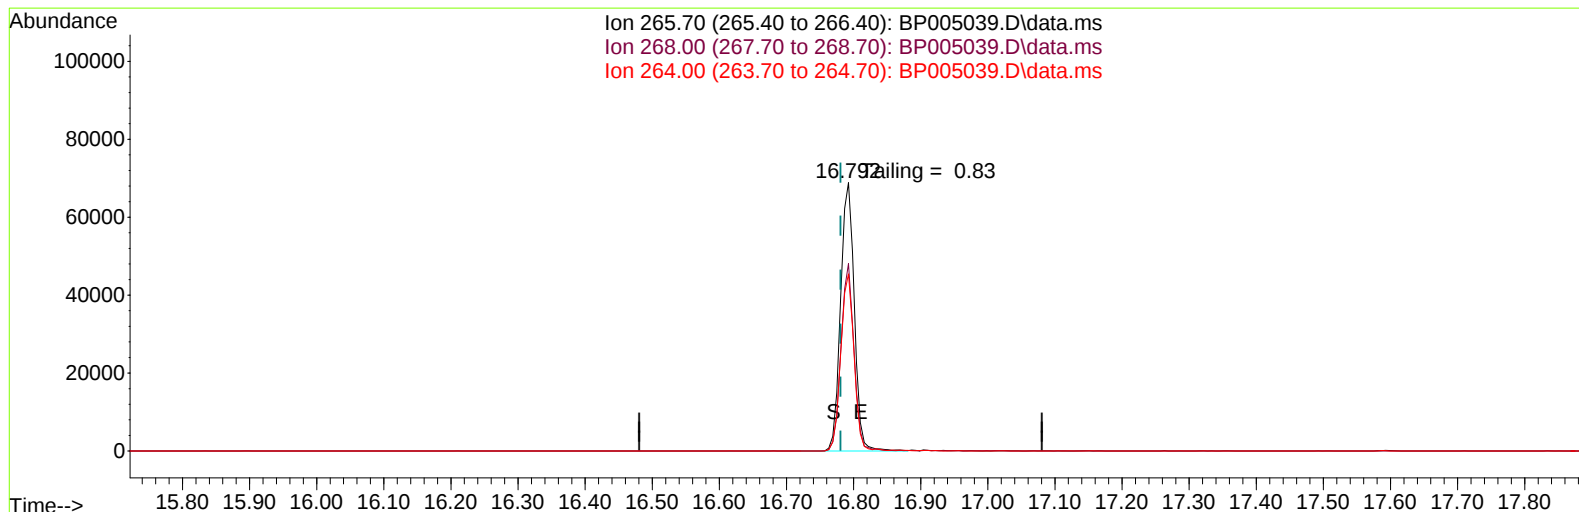

TIC: BP005039.D\data.ms

(70) Pentachlorophenol (C)

16.792min (+ 0.012) 98380.23 ng




response 98177

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	63.90	69.79
264.00	63.30	65.98
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032521\
 Data File : BP005039.D
 Acq On : 25 Mar 2021 08:54
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 DFTPP

Quant Time: Mar 26 03:03:34 2021
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\8270E-BP032321.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Thu Mar 25 10:21:09 2021
 Response via : Initial Calibration

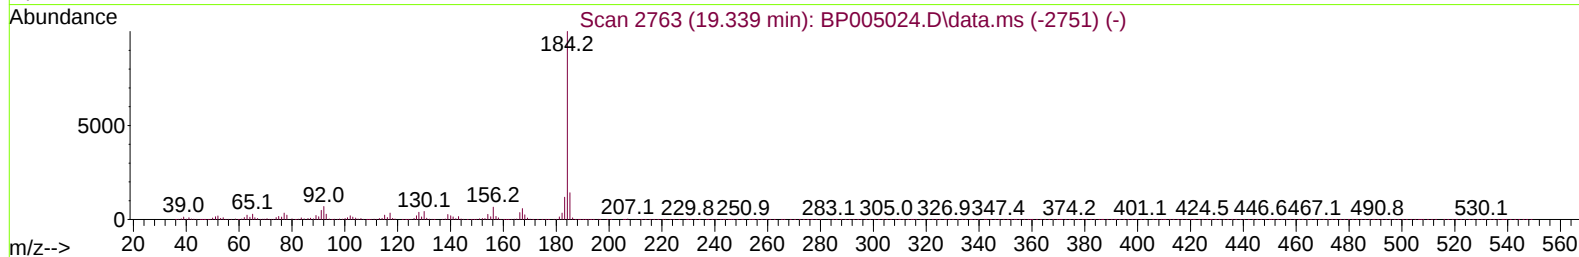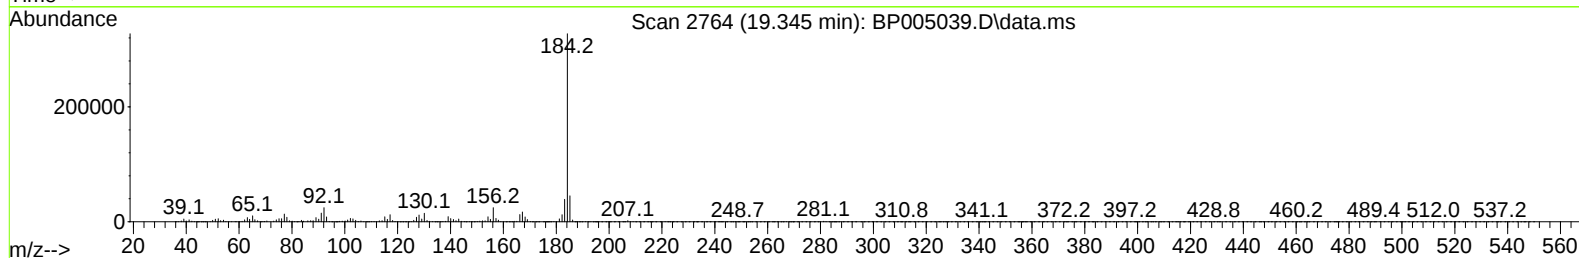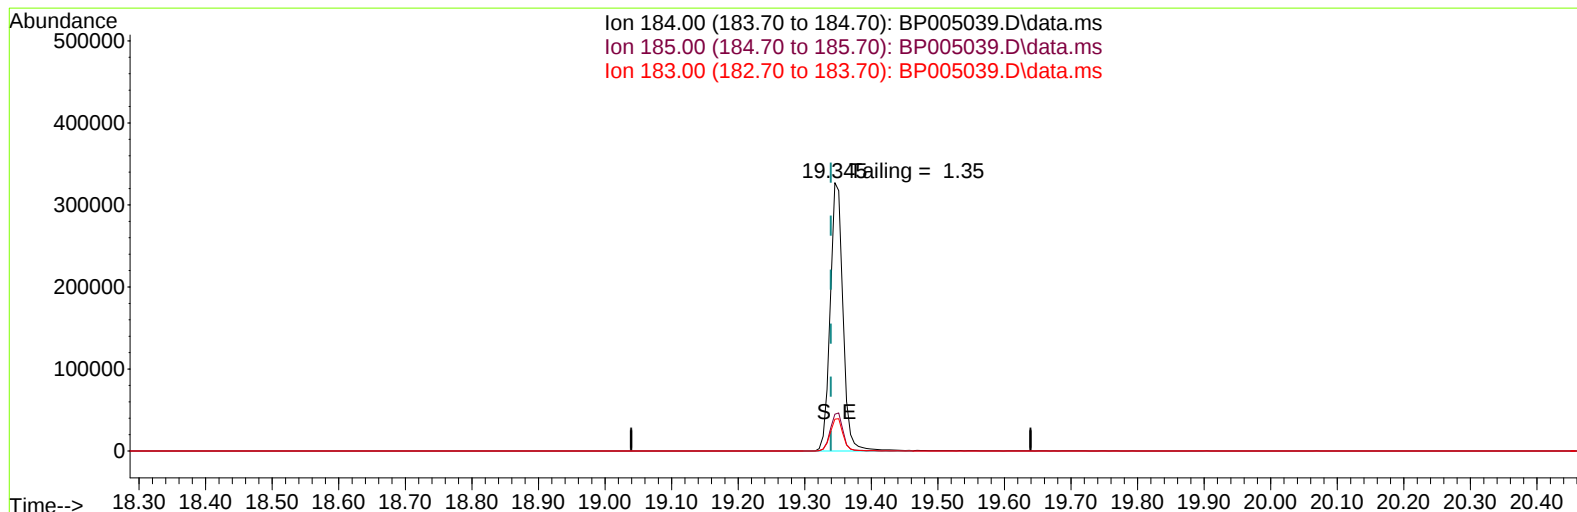

TIC: BP005039.D\data.ms

(77) Benzidine

19.345min (+ 0.006) 3949.39 ng

response 439405

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.40	13.76
183.00	12.00	11.88
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
03/25/2021	BNA_P	BP005039.D
Compound Name	Response	Retention Time
DDT	266043	20.545
DDD	3518	20.116
DDE	764	19.622
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
4282	270325	1.58

Instrument :
BNA_P
ClientSampleId :
DFTPP