




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032524\
Data File : BP019987.D
Acq On : 25 Mar 2024 18:52
Operator : MA/JU
Sample : P1813-12
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E0LY0

Manual IntegrationsAPPROVED

Quant Time: Mar 25 23:12:35 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032224.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Mar 25 10:46:59 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/26/2024
Supervised By :mohammad ahmed 03/27/2024

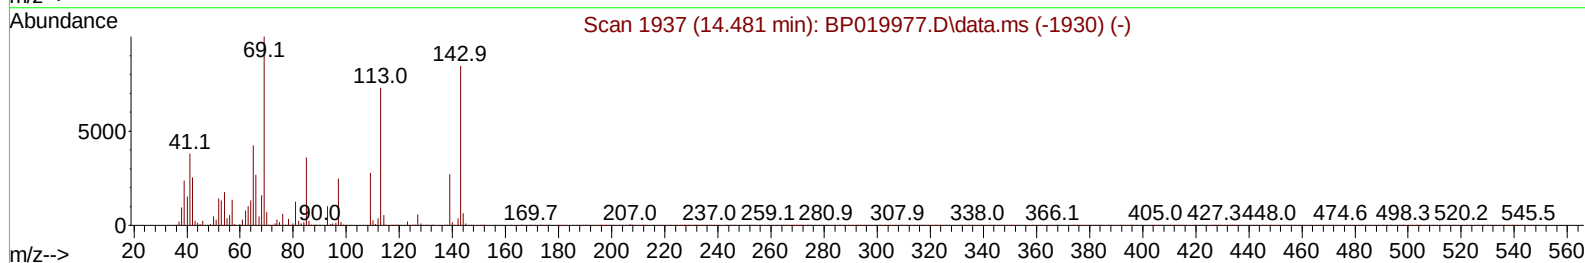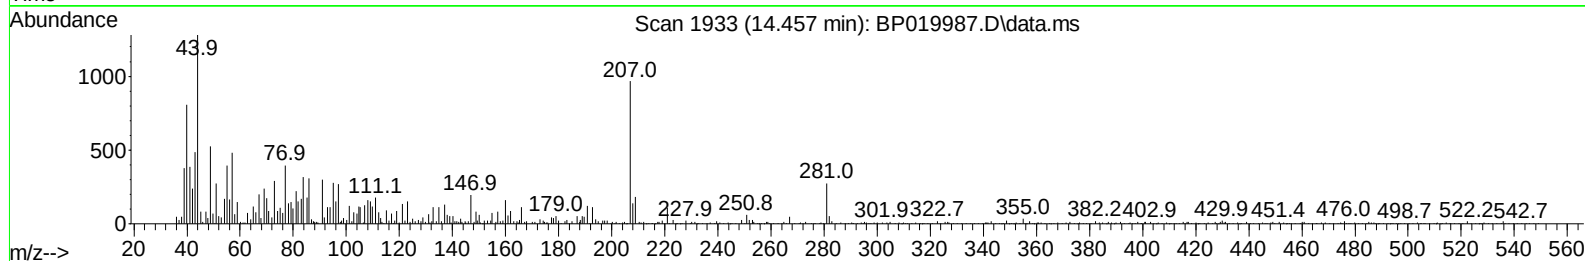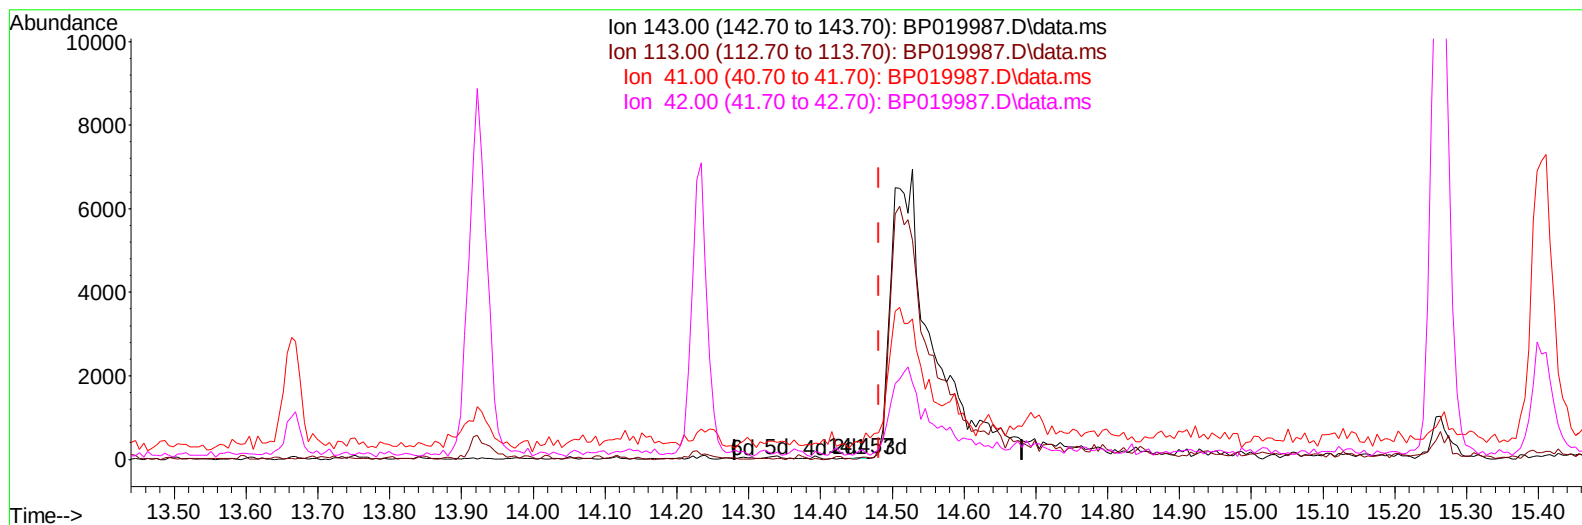

TIC: BP019987.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.457min (-0.024) 0.01 ng/u1

response 22

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	81.50	113.04#
41.00	40.90	836.96#
42.00	28.50	521.74#




Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032524\
Data File : BP019987.D
Acq On : 25 Mar 2024 18:52
Operator : MA/JU
Sample : P1813-12
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
E0LY0

Manual IntegrationsAPPROVED

Quant Time: Mar 25 23:12:35 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032224.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Mar 25 10:46:59 2024
Response via : Initial Calibration

Reviewed By :Jagrut Upadhyay 03/26/2024
Supervised By :mohammad ahmed 03/27/2024

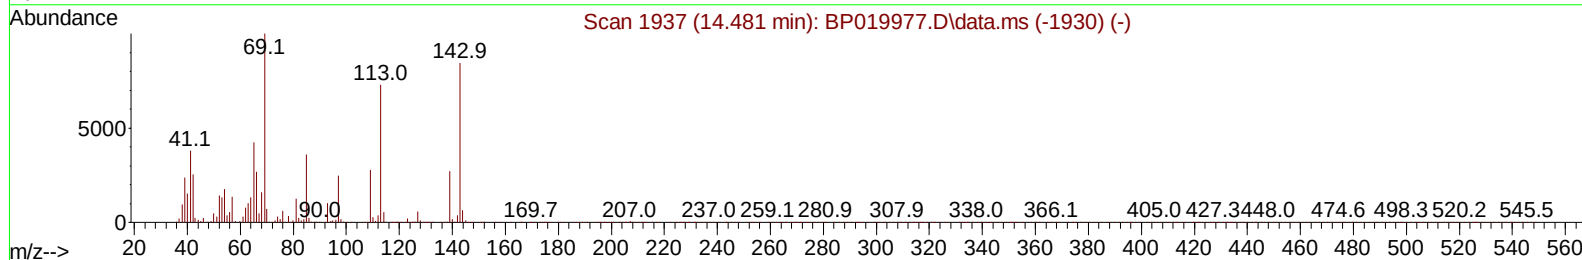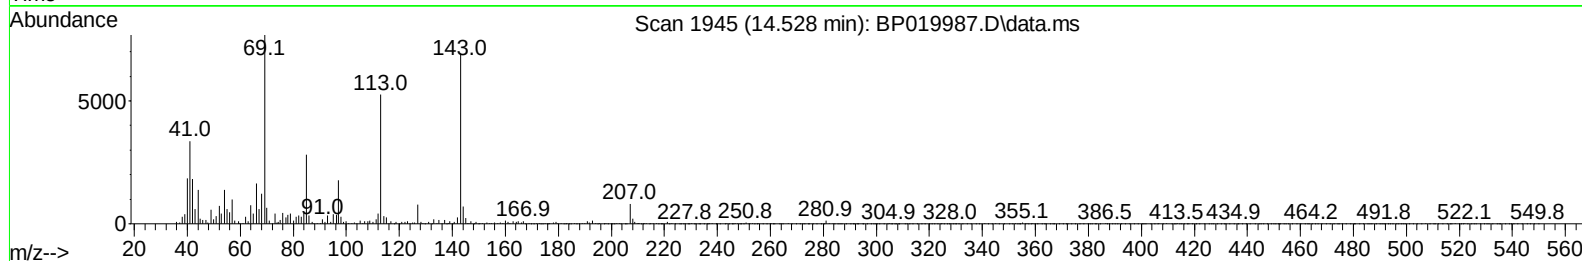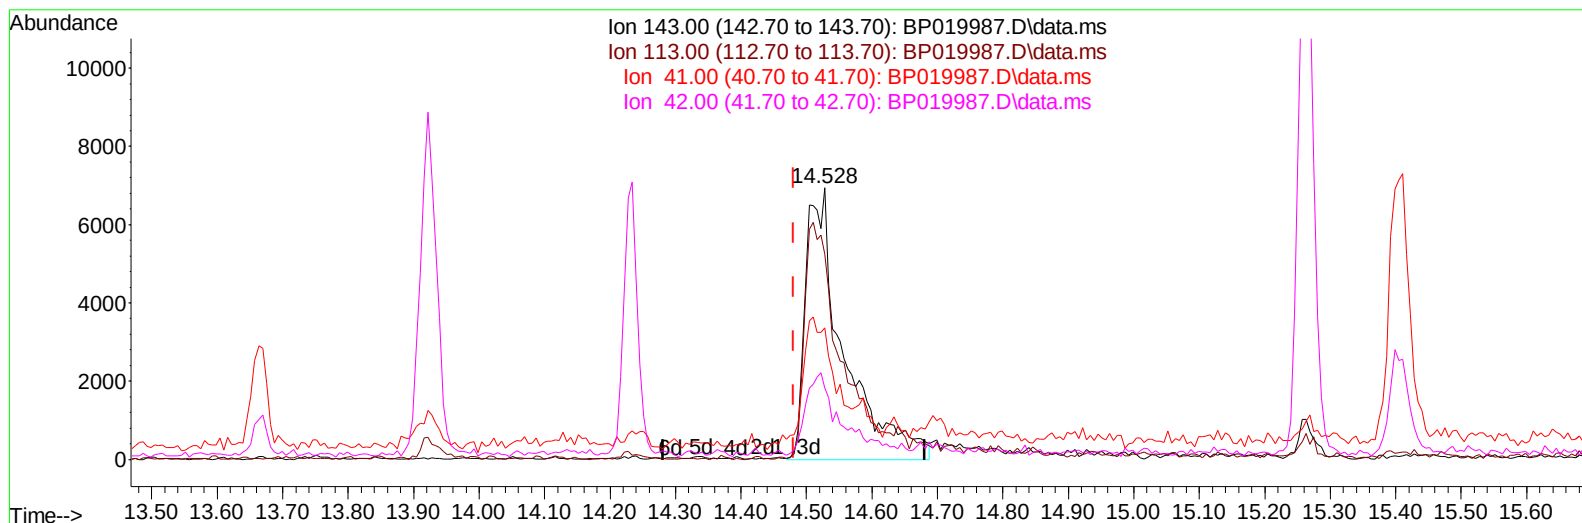

TIC: BP019987.D\data.ms

(54) 4-Nitrophenol-d4 (S)

14.528min (+ 0.047) 7.66 ng/ul m

response 28168

Ion	Exp%	Act%
143.00	100.00	100.00
113.00	81.50	75.68
41.00	40.90	48.47
42.00	28.50	26.33

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032524\
 Data File : BP019987.D
 Acq On : 25 Mar 2024 18:52
 Operator : MA/JU
 Sample : P1813-12
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 E0LY0

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 03/26/2024
 Supervised By :mohammad ahmed 03/27/2024

Quant Time: Mar 25 23:56:37 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032224.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Mar 25 10:46:59 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.616	152	108883	20.000	ng/ul	0.00
20) Naphthalene-d8	10.369	136	474545	20.000	ng/ul	0.00
38) Acenaphthene-d10	14.228	164	333695	20.000	ng/ul	-0.02
64) Phenanthrene-d10	17.063	188	694630	20.000	ng/ul	-0.01
79) Chrysene-d12	21.528	240	496208	20.000	ng/ul	-0.02
88) Perylene-d12	24.798	264	467252	20.000	ng/ul	-0.04
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.246	96	15336	6.171	ng/uL	0.00
4) Pyridine-d5	3.652	84	39250	5.231	ng/ul	0.01
7) Phenol-d5	6.811	99	79757	8.685	ng/ul	0.01
9) Bis-(2-Chloroethyl)eth...	6.975	67	269200	44.995	ng/ul	0.00
11) 2-Chlorophenol-d4	7.158	132	212417	32.209	ng/ul	0.00
15) 4-Methylphenol-d8	8.316	113	154250	21.711	ng/ul	0.01
21) Nitrobenzene-d5	8.763	128	154513	42.480	ng/ul	0.00
24) 2-Nitrophenol-d4	9.469	143	164022	40.304	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.010	165	275273	37.037	ng/ul	0.01
31) 4-Chloroaniline-d4	10.522	131	117598	12.137	ng/ul	0.00
46) Dimethylphthalate-d6	13.669	166	1110309	47.457	ng/ul	0.02
49) Acenaphthylene-d8	13.922	160	1187252	43.441	ng/ul	-0.01
54) 4-Nitrophenol-d4	14.528	143	28168m	7.658	ng/ul	0.05
60) Fluorene-d10	15.263	176	904711	45.394	ng/ul	0.00
65) 4,6-Dinitro-2-methylph...	15.410	200	168109	40.431	ng/ul	-0.01
73) Anthracene-d10	17.169	188	1458223	47.424	ng/ul	0.00
81) Pyrene-d10	19.569	212	1617916	55.573	ng/ul	0.00
92) Benzo(a)pyrene-d12	24.580	264	1115516	49.694	ng/ul	-0.03

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032524\
Data File : BP019987.D
Acq On : 25 Mar 2024 18:52
Operator : MA/JU
Sample : P1813-12
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
EOLY0

Manual IntegrationsAPPROVED

Reviewed By :Jagrut Upadhyay 03/26/2024
Supervised By :mohammad ahmed 03/27/2024

Quant Time: Mar 25 23:56:37 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032224.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Mar 25 10:46:59 2024
Response via : Initial Calibration

