

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032524\
 Data File : BP019978.D
 Acq On : 25 Mar 2024 10:14
 Operator : MA/JU
 Sample : PB159425BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK425

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032224.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP019978.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.228	20	24	31	rVB	37985	46825	1.79%	0.158%
2	3.622	87	91	112	rBV	431285	701111	26.78%	2.368%
3	3.916	139	141	147	rVB2	7655	9820	0.38%	0.033%
4	6.116	513	515	519	rBV5	1810	3015	0.12%	0.010%
5	6.787	622	629	644	rBV	504081	892988	34.11%	3.016%
6	6.946	650	656	667	rBV	432967	692049	26.44%	2.337%
7	7.134	681	688	701	rBV	478889	863727	33.00%	2.917%
8	7.599	760	767	775	rBV	390295	671753	25.66%	2.269%
9	8.304	879	887	898	rBV	602299	1067974	40.80%	3.607%
10	8.746	954	962	976	rBV	525101	894737	34.18%	3.022%
11	8.899	986	988	994	rVB7	1746	2664	0.10%	0.009%
12	9.451	1073	1082	1097	rBV	402616	757656	28.94%	2.559%
13	9.987	1164	1173	1183	rBV	466898	986845	37.70%	3.333%
14	10.346	1226	1234	1243	rBV	518884	937209	35.80%	3.165%
15	10.504	1253	1261	1290	rBV	465587	1108596	42.35%	3.744%
16	11.993	1506	1514	1520	rBV5	7135	17999	0.69%	0.061%
17	13.110	1699	1704	1711	rVB10	3672	6505	0.25%	0.022%
18	13.651	1783	1796	1813	rBV	746116	1526711	58.32%	5.156%
19	13.922	1834	1842	1856	rBV	1297511	1853149	70.79%	6.258%
20	14.239	1888	1896	1908	rBV	922450	1239171	47.34%	4.185%
21	14.492	1931	1939	1954	rBV	259437	649247	24.80%	2.193%
22	15.045	2032	2033	2039	rVB6	2251	3187	0.12%	0.011%
23	15.263	2061	2070	2087	rBV	1216501	2185930	83.51%	7.382%
24	15.398	2087	2093	2106	rBV	362336	677368	25.88%	2.288%
25	15.986	2191	2193	2200	rVB8	2620	3481	0.13%	0.012%
26	16.081	2202	2209	2213	rBV8	5945	10212	0.39%	0.034%
27	16.439	2267	2270	2275	rBV7	1992	4326	0.17%	0.015%
28	17.063	2368	2376	2386	rBV	704861	1445530	55.22%	4.882%
29	17.169	2388	2394	2411	rVV2	1427482	2298355	87.80%	7.762%
30	18.175	2563	2565	2568	rBV4	3478	4660	0.18%	0.016%
31	19.104	2720	2723	2730	rVB3	21057	31750	1.21%	0.107%
32	19.186	2734	2737	2740	rVB3	11239	14938	0.57%	0.050%
33	19.563	2794	2801	2815	rBV	1613060	2617650	100.00%	8.840%
34	21.539	3131	3137	3148	rBV	910292	1449480	55.37%	4.895%
35	24.592	3647	3656	3671	rVB2	926120	2509535	95.87%	8.475%
36	24.827	3689	3696	3711	rVB	529577	1424682	54.43%	4.811%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032524\
Data File : BP019978.D
Acq On : 25 Mar 2024 10:14
Operator : MA/JU
Sample : PB159425BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK425

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032224.MA.M
Title : SVOA CALIBRATION




Sum of corrected areas: 29610835

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032524\
Data File : BP019978.D
Acq On : 25 Mar 2024 10:14
Operator : MA/JU
Sample : PB159425BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK425

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

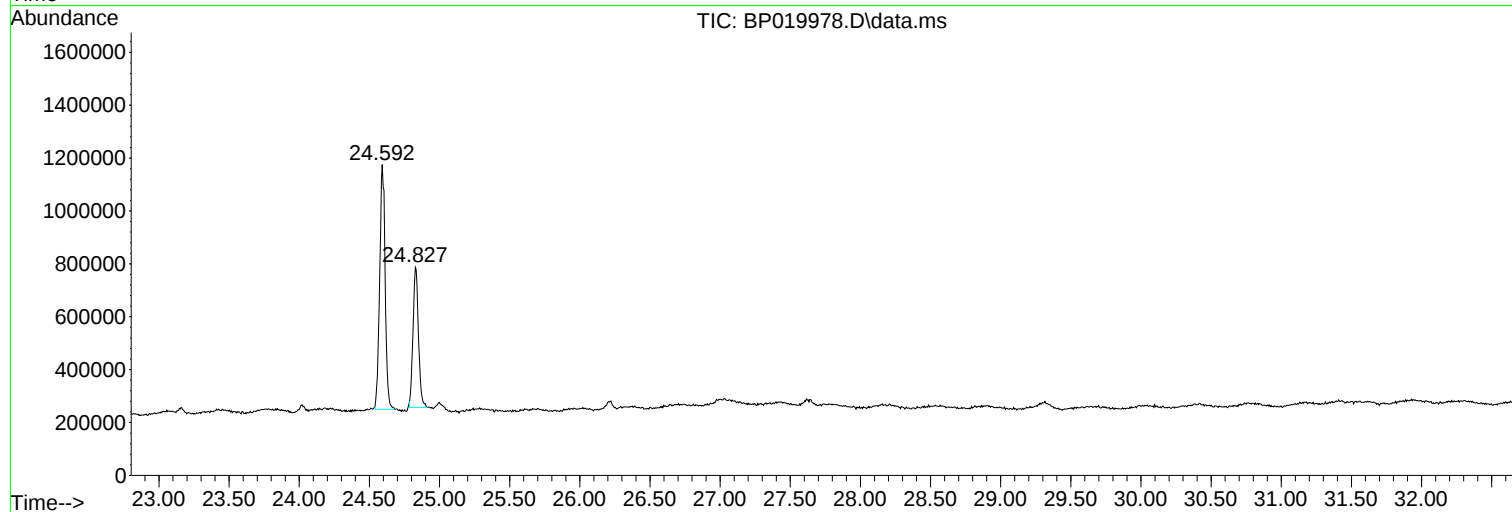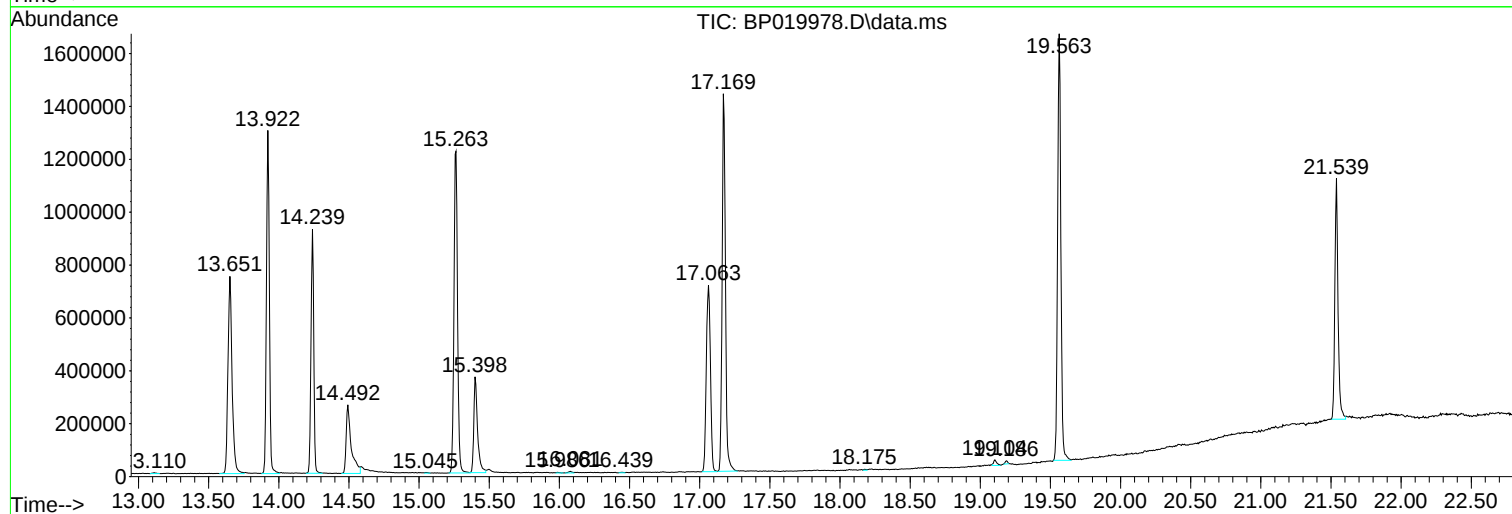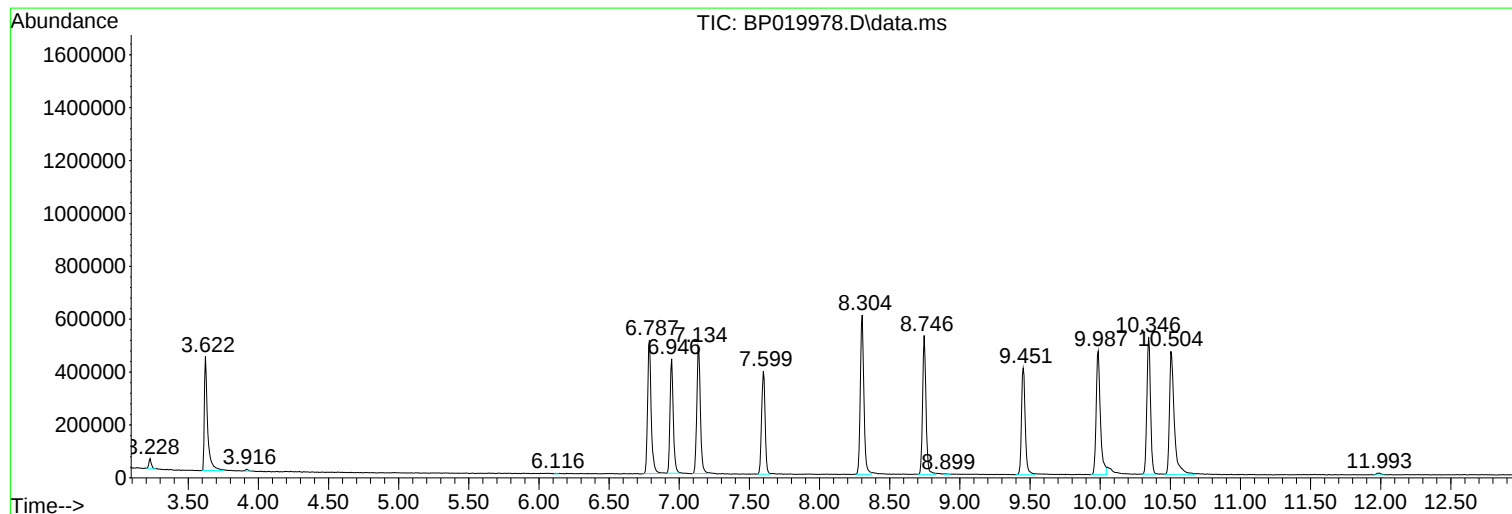

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032524\
Data File : BP019978.D
Acq On : 25 Mar 2024 10:14
Operator : MA/JU
Sample : PB159425BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK425

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032524\
Data File : BP019978.D
Acq On : 25 Mar 2024 10:14
Operator : MA/JU
Sample : PB159425BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK425

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------