

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032524\
 Data File : BP019983.D
 Acq On : 25 Mar 2024 15:59
 Operator : MA/JU
 Sample : PB159444BL
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_P
 ClientSampleId :
 SBLK444

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032224.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BP019983.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.222	19	23	32	rVB	46757	63739	1.42%	0.141%
2	3.610	86	89	111	rBV	542827	908250	20.17%	2.011%
3	3.910	137	140	144	rVB	7626	9948	0.22%	0.022%
4	6.757	617	624	640	rBV	667932	1164295	25.85%	2.578%
5	6.934	646	654	670	rVB	518671	952579	21.15%	2.109%
6	7.110	678	684	697	rBV	686179	1119697	24.86%	2.480%
7	7.569	755	762	774	rBV	492521	850379	18.88%	1.883%
8	8.269	872	881	896	rBV	831640	1483087	32.93%	3.284%
9	8.722	950	958	972	rBV	745977	1245107	27.65%	2.757%
10	9.434	1070	1079	1102	rBV	640019	1096105	24.34%	2.427%
11	9.963	1161	1169	1184	rBV	785795	1488403	33.05%	3.296%
12	10.328	1222	1231	1241	rBV	703215	1287871	28.60%	2.852%
13	10.475	1248	1256	1272	rBV	734643	1583398	35.16%	3.506%
14	11.963	1503	1509	1516	rBV3	10002	23402	0.52%	0.052%
15	13.633	1785	1793	1807	rBV	1630992	2618699	58.15%	5.799%
16	13.916	1833	1841	1853	rBV	1747506	2896949	64.32%	6.415%
17	14.228	1886	1894	1909	rBV	1157977	1933644	42.93%	4.282%
18	14.469	1929	1935	1951	rBV	522033	1172237	26.03%	2.596%
19	14.580	1951	1954	1957	rVB5	11297	18113	0.40%	0.040%
20	14.663	1965	1968	1972	rVB6	6270	8813	0.20%	0.020%
21	15.239	2058	2066	2081	rBV	2023355	3637531	80.77%	8.055%
22	15.398	2086	2093	2107	rBV	721064	1348204	29.94%	2.986%
23	15.498	2107	2110	2117	rVB3	16771	30126	0.67%	0.067%
24	15.851	2164	2170	2173	rVB6	3399	5291	0.12%	0.012%
25	16.069	2202	2207	2214	rVB3	9165	14591	0.32%	0.032%
26	16.733	2317	2320	2325	rVB6	5113	7397	0.16%	0.016%
27	16.839	2336	2338	2342	rBV4	3265	4647	0.10%	0.010%
28	17.069	2370	2377	2387	rBV	1429254	2324383	51.61%	5.147%
29	17.169	2387	2394	2415	rVB	2864426	3990993	88.62%	8.838%
30	19.116	2720	2725	2730	rBV3	36915	58092	1.29%	0.129%
31	19.192	2733	2738	2744	rBV	27753	56411	1.25%	0.125%
32	19.568	2795	2802	2816	rBV	3061249	4503660	100.00%	9.973%
33	20.410	2940	2945	2951	rBV	116789	166930	3.71%	0.370%
34	21.557	3133	3140	3151	rBV	1197810	2116295	46.99%	4.686%
35	24.621	3651	3661	3672	rVB3	1182764	3223112	71.57%	7.137%
36	24.856	3691	3701	3713	rVB	618108	1745144	38.75%	3.865%

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032524\
Data File : BP019983.D
Acq On : 25 Mar 2024 15:59
Operator : MA/JU
Sample : PB159444BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK444

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032224.MA.M
Title : SVOA CALIBRATION




Sum of corrected areas: 45157522

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032524\
Data File : BP019983.D
Acq On : 25 Mar 2024 15:59
Operator : MA/JU
Sample : PB159444BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK444

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

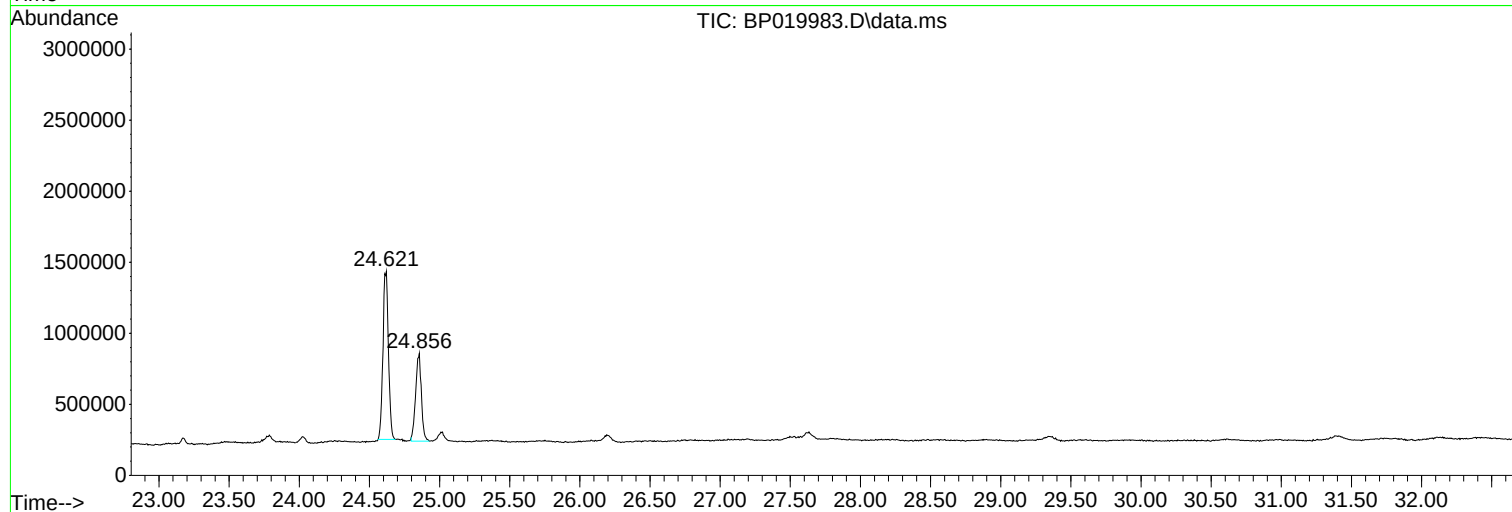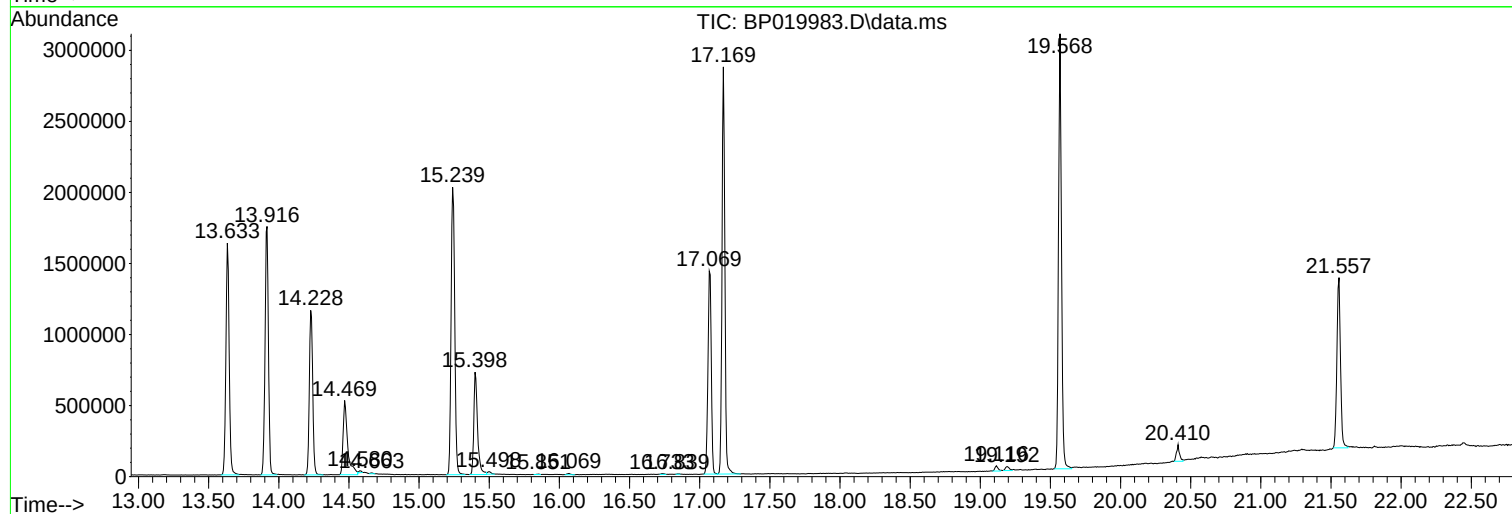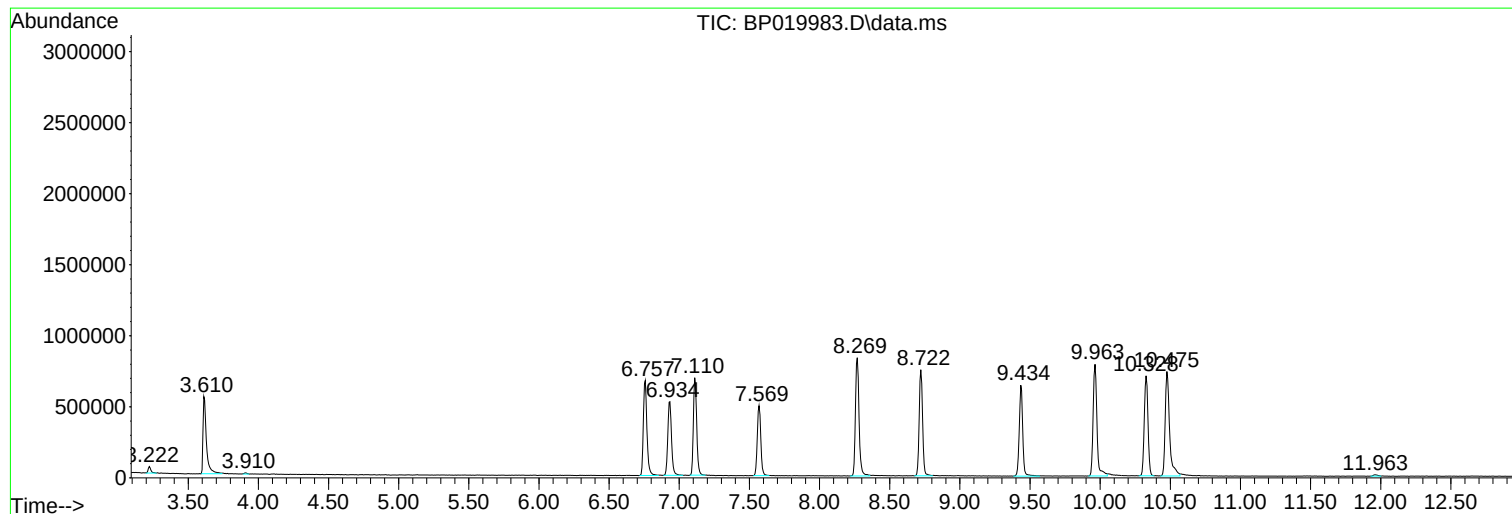

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032524\
Data File : BP019983.D
Acq On : 25 Mar 2024 15:59
Operator : MA/JU
Sample : PB159444BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK444

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_P\Data\BP032524\
Data File : BP019983.D
Acq On : 25 Mar 2024 15:59
Operator : MA/JU
Sample : PB159444BL
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_P
ClientSampleId :
SBLK444

Quant Method : Z:\svoasrv\HPCHEM1\BNA_P\Methods\SFAM-EPA-BP032224.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\DATABASE\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc